
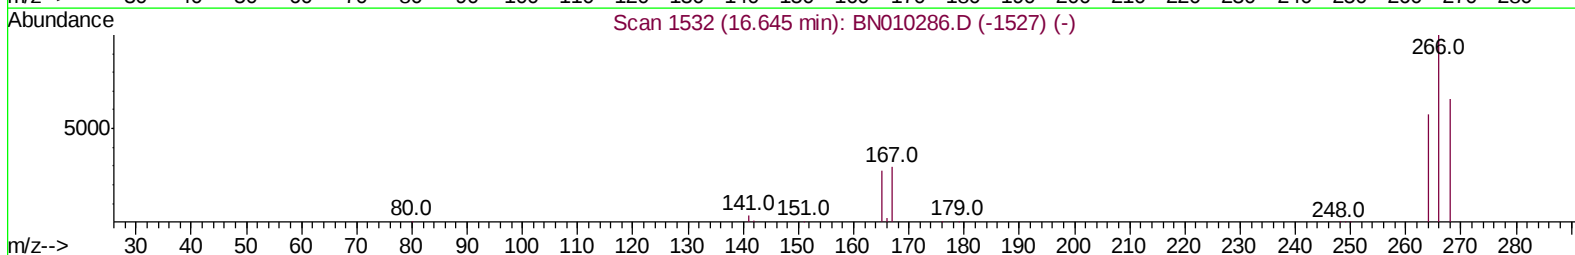
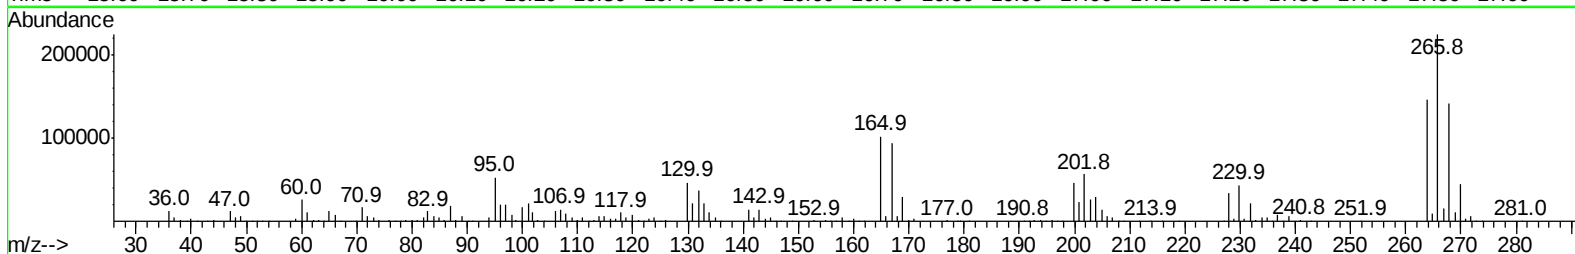


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032420\
 Data File : BN010338.D
 Acq On : 24 Mar 2020 22:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 04:25:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 19 15:26:45 2020
 Response via : Initial Calibration

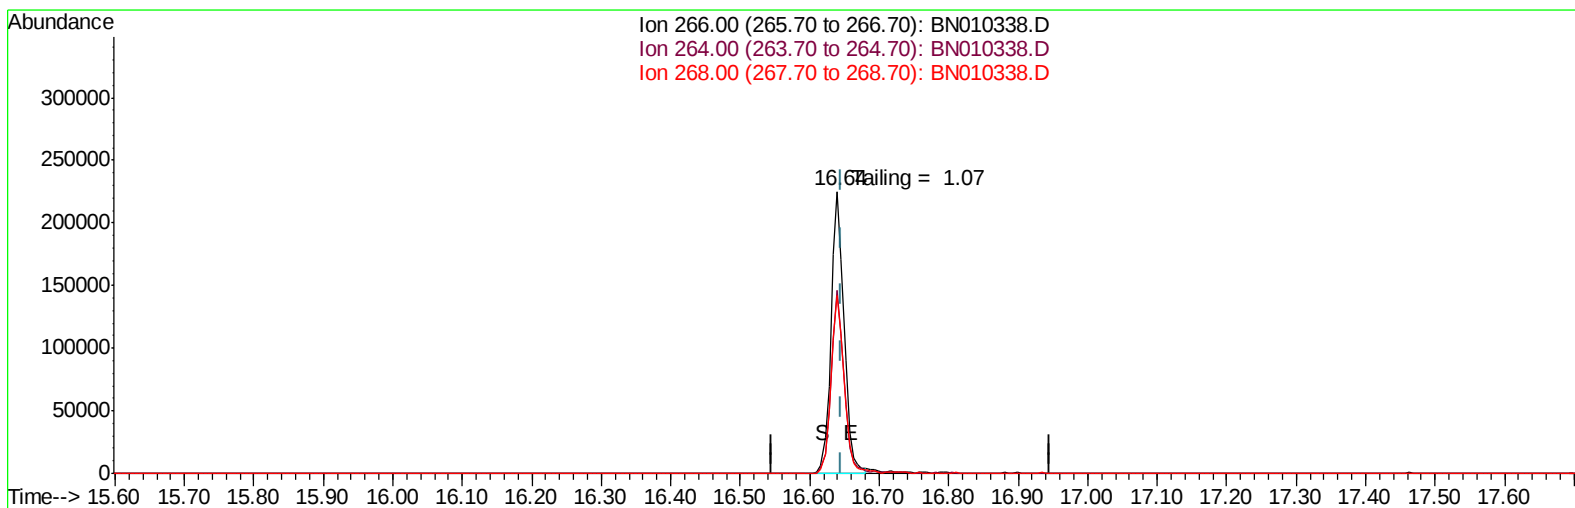

TIC: BN010338.D

(22) Pentachlorophenol

16.639min (-0.006) 0.00ng

response 294314

Ion	Exp%	Act%
266.00	100	100
264.00	59.60	64.85
268.00	68.60	63.32
0.00	0.00	0.00