
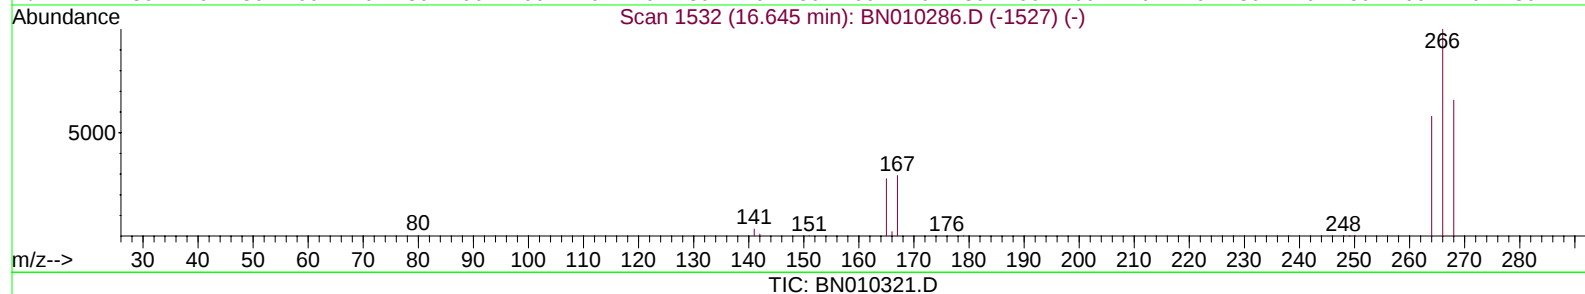
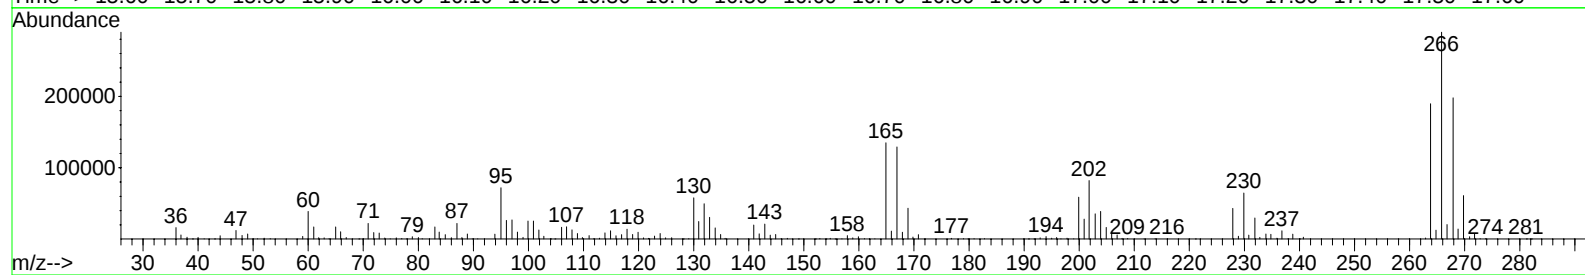


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN032420\
 Data File : BN010321.D
 Acq On : 24 Mar 2020 10:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 19:22:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 19 15:26:45 2020
 Response via : Initial Calibration

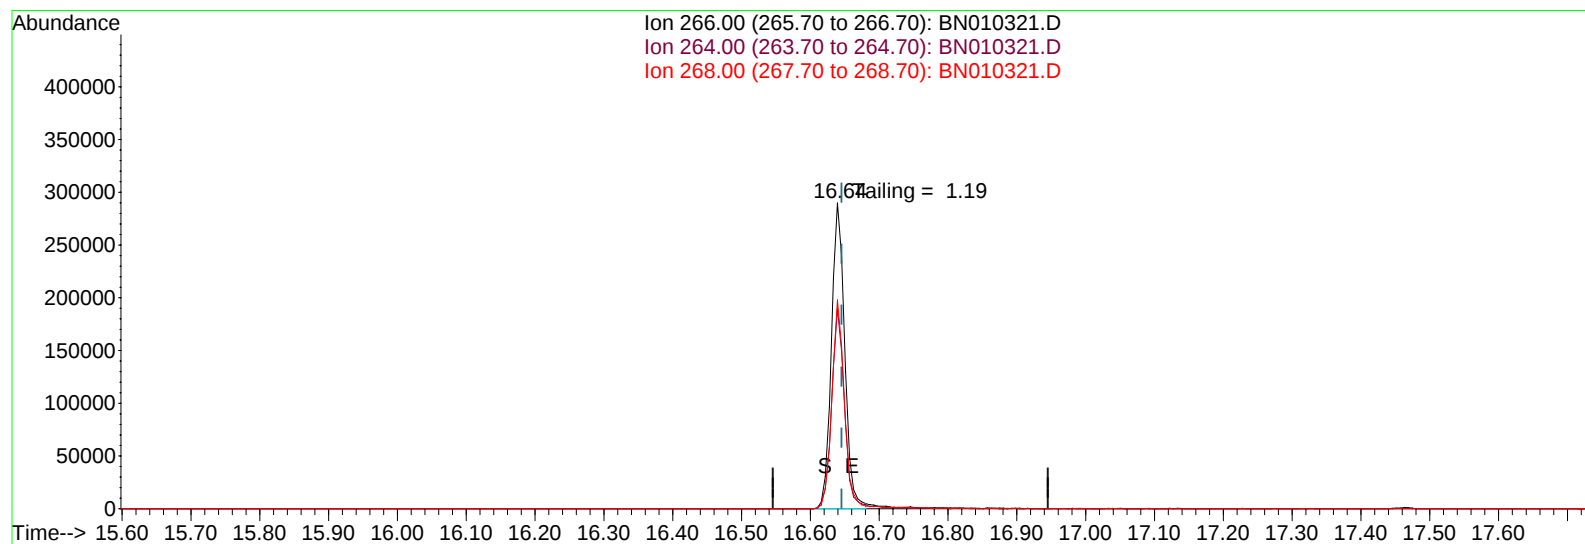

(22) Pentachlorophenol

16.639min (-0.006) 0.00ng

response 394572

Ion	Exp%	Act%
266.00	100	100
264.00	59.60	65.42
268.00	68.60	68.27
0.00	0.00	0.00