


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032420\
 Data File : BN010321.D
 Acq On : 24 Mar 2020 10:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 15:26:45 2020

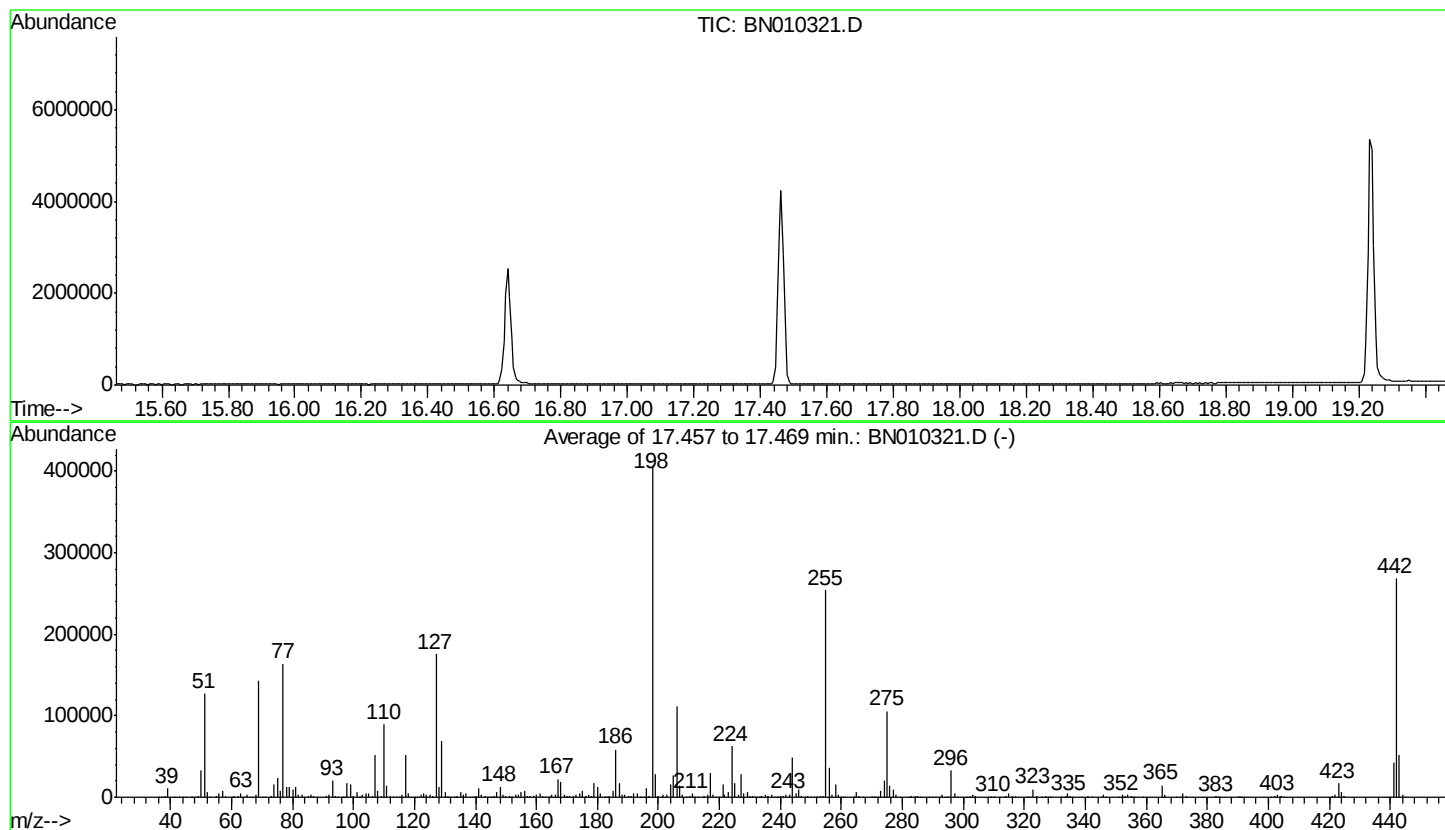

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	127056	PASS
68	69	0.00	2	2.0	2824	PASS
69	198	0.00	100	35.3	143493	PASS
70	69	0.00	2	0.6	830	PASS
127	198	10	80	43.2	175680	PASS
197	198	0.00	2	0.5	1836	PASS
198	198	100	100	100.0	406848	PASS
199	198	5	9	6.8	27826	PASS
275	198	10	60	26.1	106050	PASS
365	198	1	100	3.6	14633	PASS
441	198	0.01	100	10.3	41720	PASS
442	198	50	100	65.9	267925	PASS
443	442	15	24	19.6	52456	PASS