


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032420\
 Data File : BN010338.D
 Acq On : 24 Mar 2020 22:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 15:26:45 2020

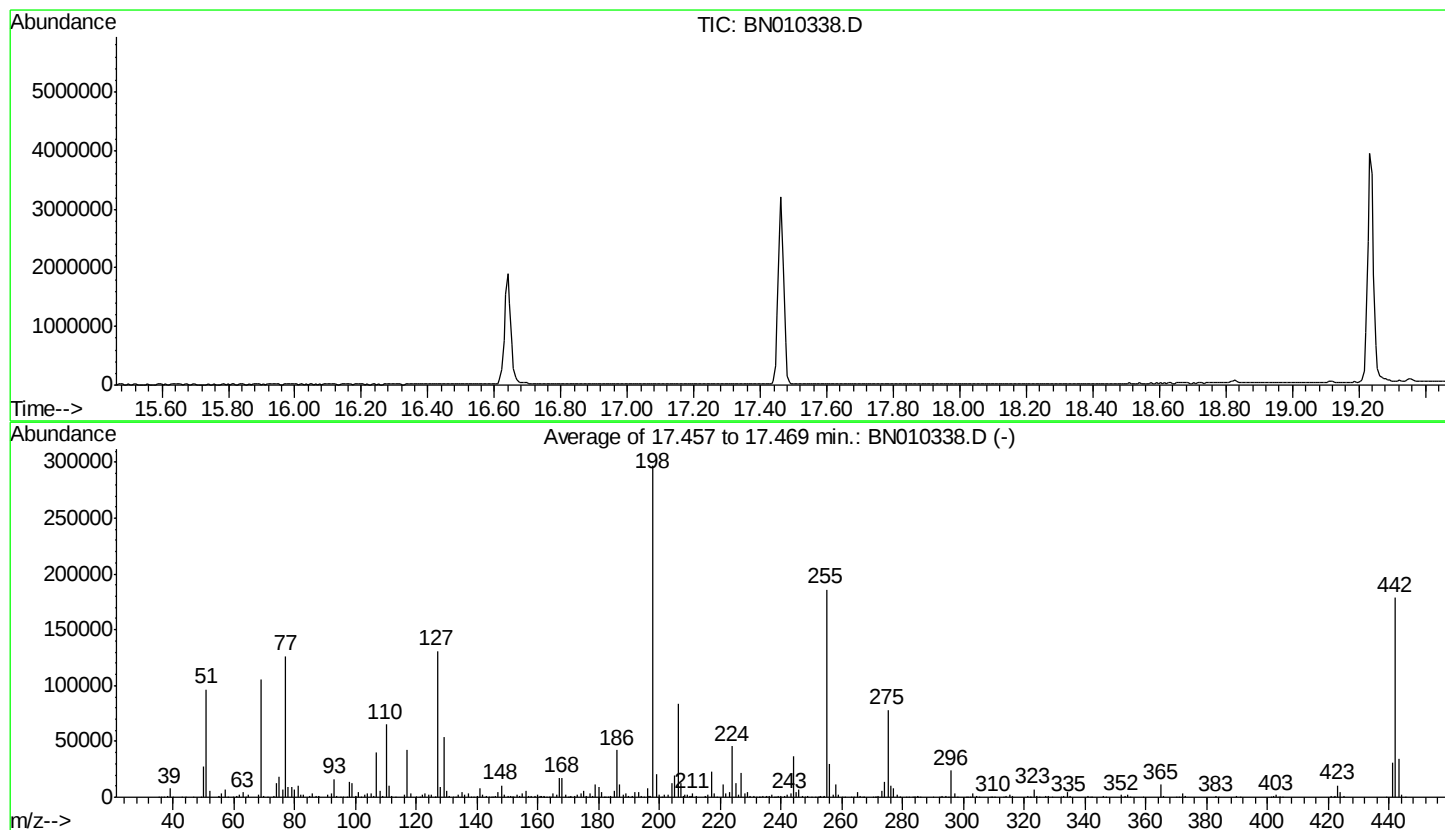

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	96613	PASS
68	69	0.00	2	2.0	2126	PASS
69	198	0.00	100	35.4	105082	PASS
70	69	0.00	2	0.8	800	PASS
127	198	10	80	44.1	130874	PASS
197	198	0.00	2	0.4	1187	PASS
198	198	100	100	100.0	297024	PASS
199	198	5	9	7.0	20715	PASS
275	198	10	60	26.3	77986	PASS
365	198	1	100	3.7	11060	PASS
441	198	0.01	100	10.4	31002	PASS
442	198	50	100	60.2	178666	PASS
443	442	15	24	19.0	33994	PASS