

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032619\
 Data File : BN004980.D
 Acq On : 26 Mar 2019 17:18
 Operator : JU/SJ
 Sample : PB118273BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118273BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.269	383	388	397	rVB	152498	215605	43.02%	8.031%
2	6.857	651	658	664	rBV	151103	229173	45.72%	8.536%
3	7.210	712	718	725	rBV	160249	249664	49.81%	9.299%
4	7.675	792	797	802	rVB	31786	46045	9.19%	1.715%
5	7.993	845	851	857	rVB	126898	190229	37.95%	7.086%
6	8.840	989	995	1003	rBV	89211	140927	28.12%	5.249%
7	10.463	1265	1271	1277	rBV	41202	65000	12.97%	2.421%
8	12.933	1685	1691	1699	rVB	260051	366359	73.09%	13.646%
9	14.322	1921	1927	1933	rVB2	61802	87945	17.55%	3.276%
10	15.822	2176	2182	2189	rVB	205975	279502	55.76%	10.411%
11	17.074	2389	2395	2401	rVB	78208	106551	21.26%	3.969%
12	19.704	2837	2842	2847	rBV	400811	501230	100.00%	18.669%
13	21.268	3104	3108	3114	rBV	87002	111067	22.16%	4.137%
14	23.515	3483	3490	3498	rVB2	51343	95462	19.05%	3.556%


Sum of corrected areas: 2684759

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032619\
Data File : BN004980.D
Acq On : 26 Mar 2019 17:18
Operator : JU/SJ
Sample : PB118273BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118273BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

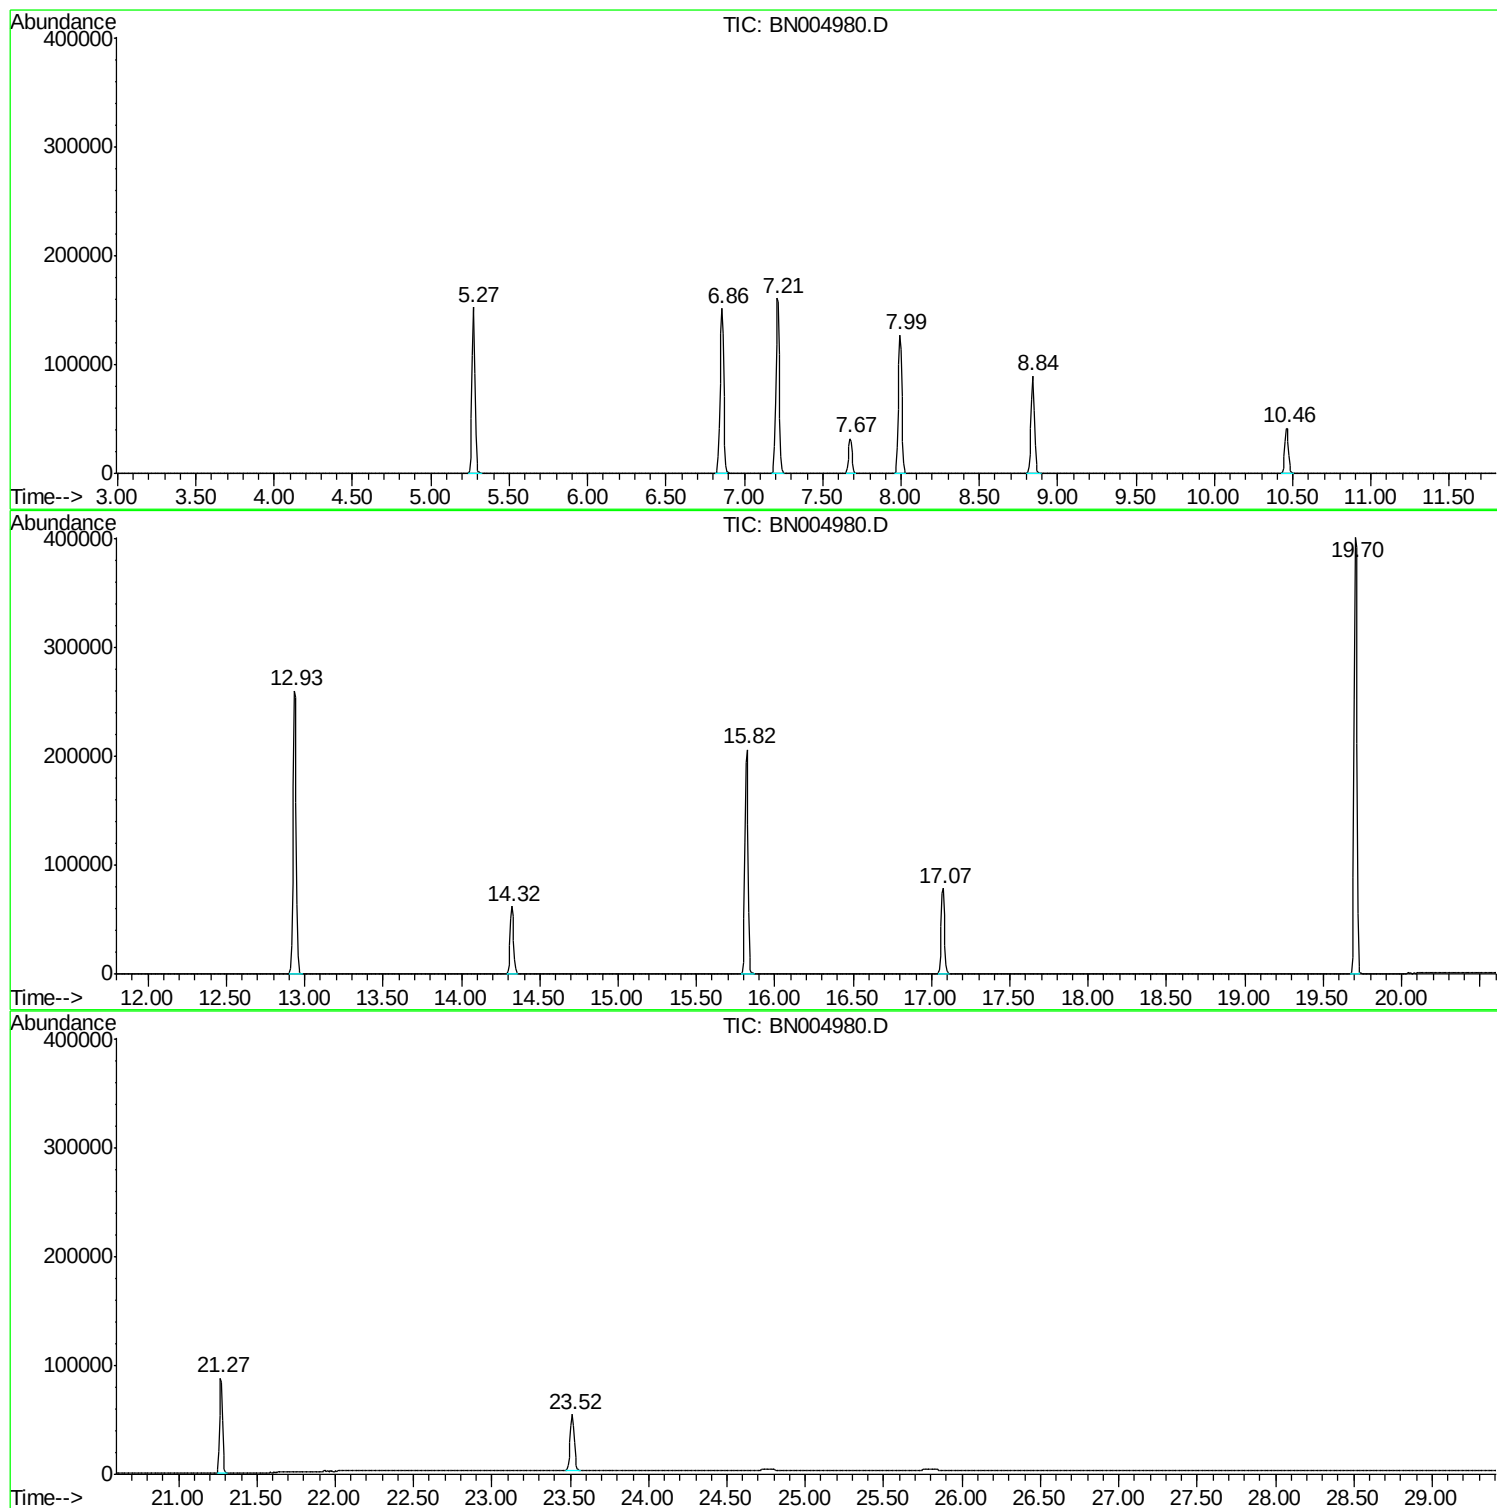

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032619\
Data File : BN004980.D
Acq On : 26 Mar 2019 17:18
Operator : JU/SJ
Sample : PB118273BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118273BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.21 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.21	108.44 ng	249664	1,4-Dichlorobenzene-d4	7.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		Tranlycypromine-propionyl	189	C12H15NO	1000123-86-3	9

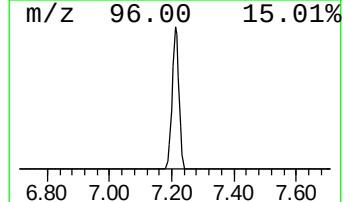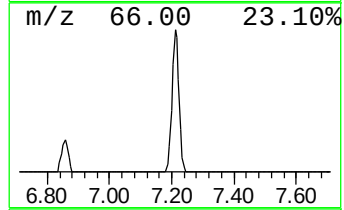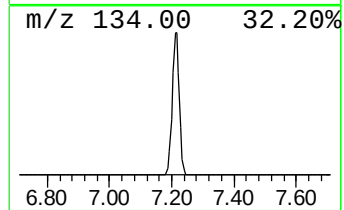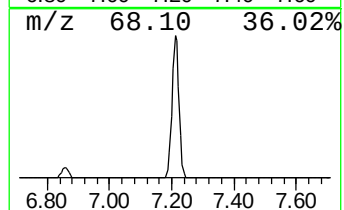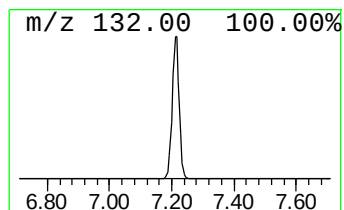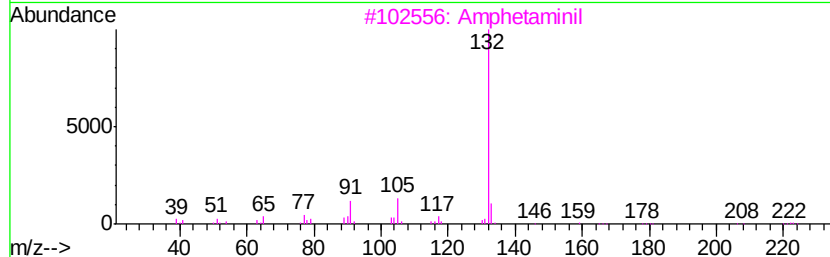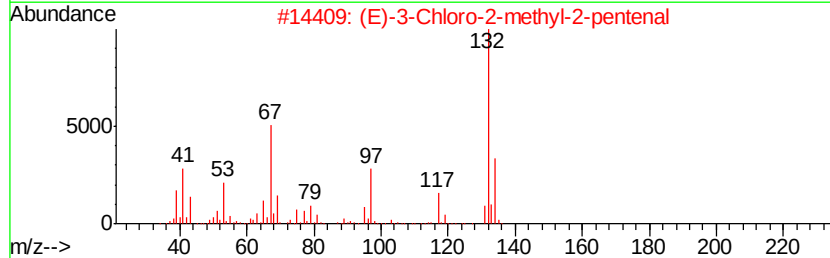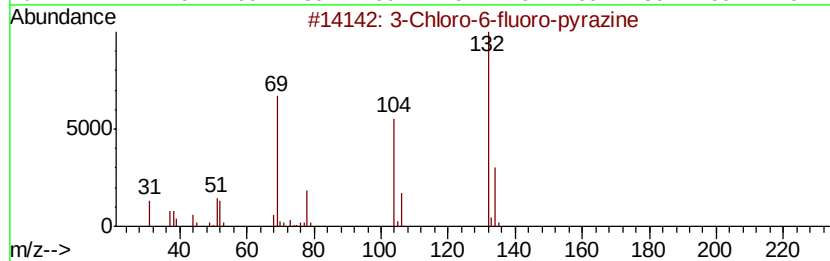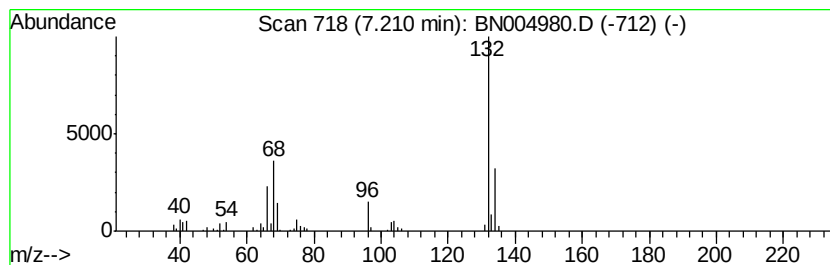

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032619\
Data File : BN004980.D
Acq On : 26 Mar 2019 17:18
Operator : JU/SJ
Sample : PB118273BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118273BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.21	7.21	108.4	ng	249664	1	7.67	46045	20.0