

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032619\
 Data File : BN004984.D
 Acq On : 26 Mar 2019 20:46
 Operator : JU/SJ
 Sample : PB118232BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118232BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.264	381	387	394	rBV	177976	246770	38.53%	7.654%
2	6.852	650	657	665	rBV	163759	260655	40.70%	8.084%
3	7.205	710	717	723	rBV	185707	284421	44.41%	8.821%
4	7.669	790	796	801	rBV	37071	53378	8.34%	1.656%
5	7.987	843	850	856	rVB	142920	218125	34.06%	6.765%
6	8.834	987	994	1001	rVB	101199	161300	25.19%	5.003%
7	10.451	1263	1269	1276	rVB	47565	75339	11.76%	2.337%
8	12.934	1684	1691	1698	rVB	296491	421176	65.77%	13.063%
9	14.316	1920	1926	1933	rVB2	69983	103549	16.17%	3.212%
10	15.816	2176	2181	2189	rBV	254836	338192	52.81%	10.489%
11	17.069	2389	2394	2402	rVB2	92488	127444	19.90%	3.953%
12	19.710	2837	2843	2848	rBV	541846	640382	100.00%	19.861%
13	21.274	3104	3109	3114	rBV	127765	150607	23.52%	4.671%
14	23.515	3483	3490	3498	rVB2	79345	142916	22.32%	4.433%


Sum of corrected areas: 3224254

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032619\
Data File : BN004984.D
Acq On : 26 Mar 2019 20:46
Operator : JU/SJ
Sample : PB118232BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118232BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

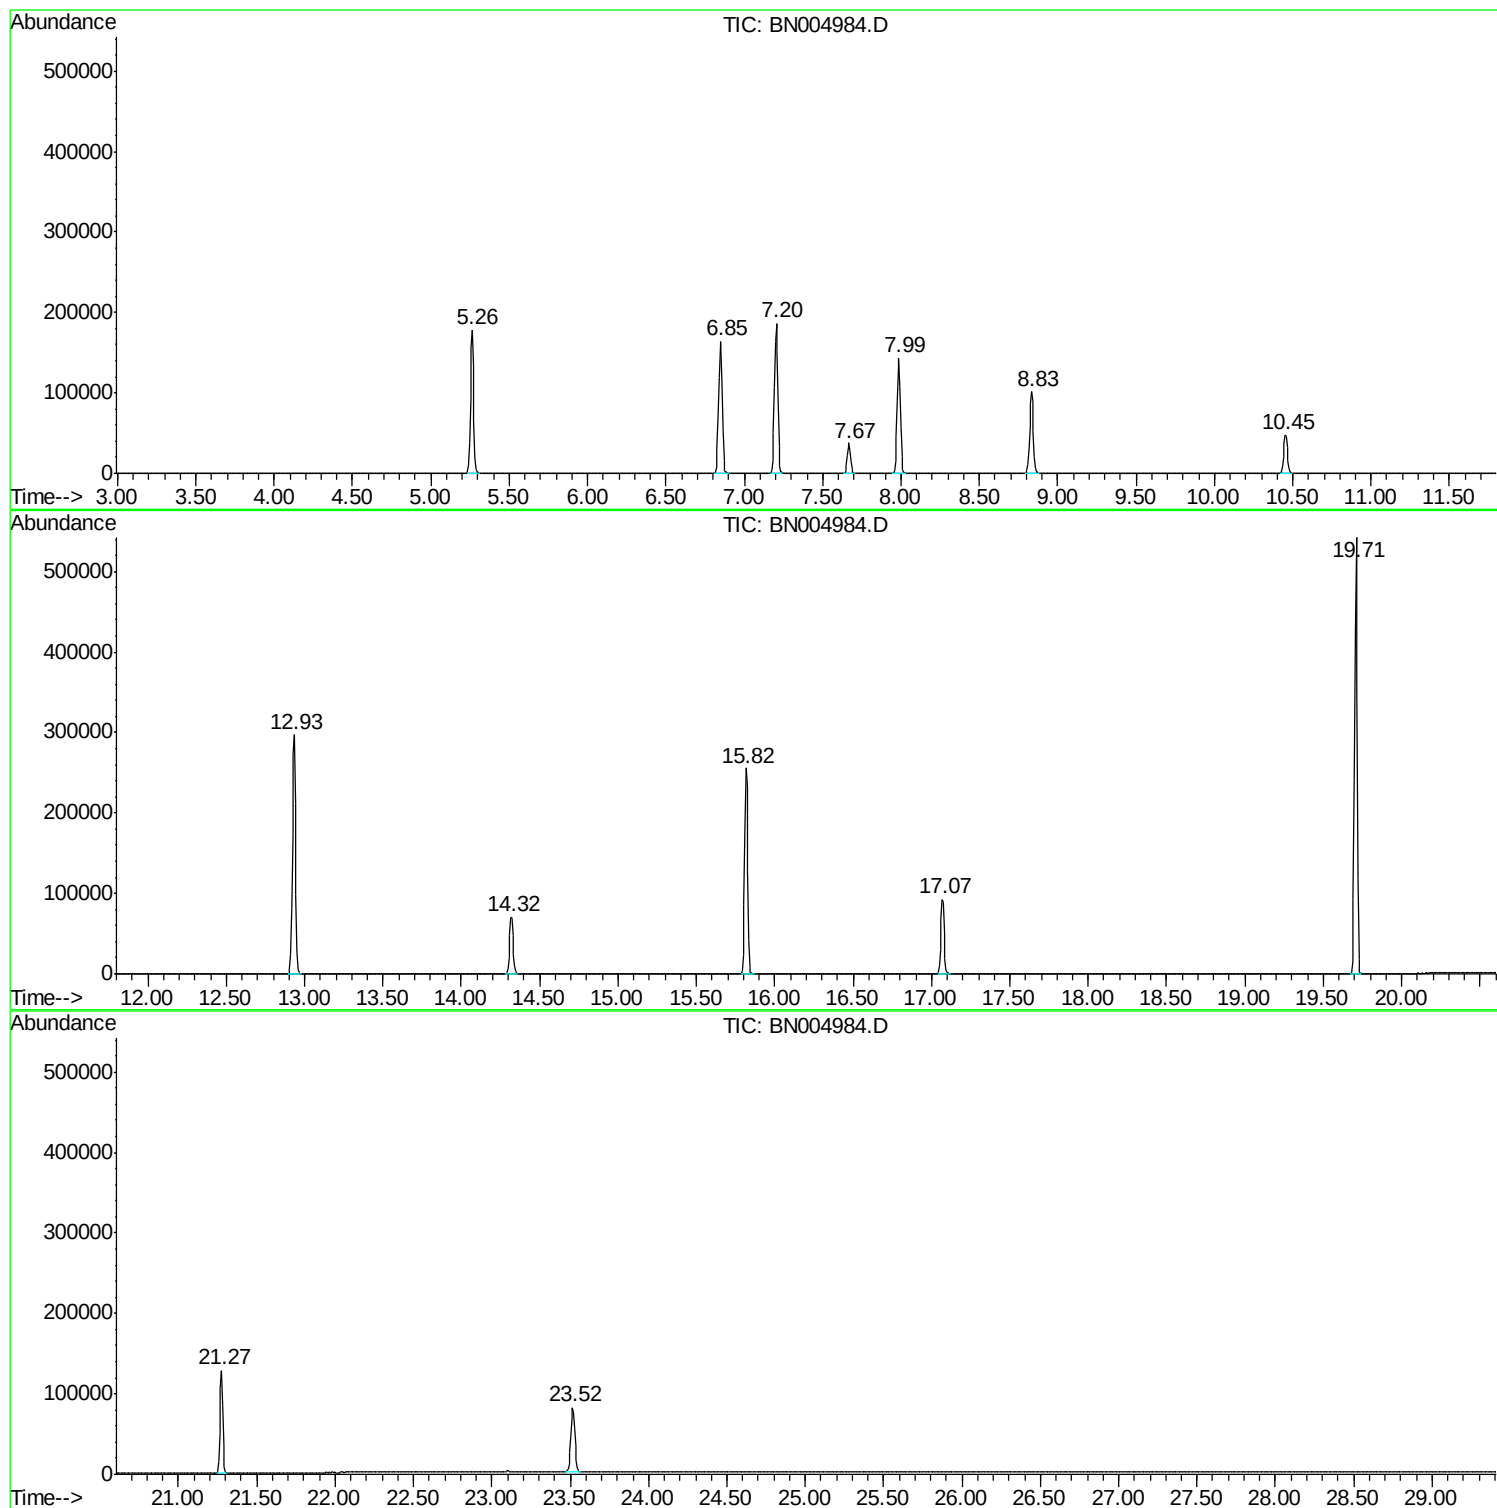

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032619\
Data File : BN004984.D
Acq On : 26 Mar 2019 20:46
Operator : JU/SJ
Sample : PB118232BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118232BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.20 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.20	106.57 ng	284421	1,4-Dichlorobenzene-d4	7.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
4		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

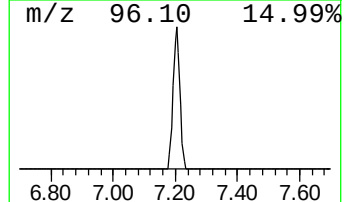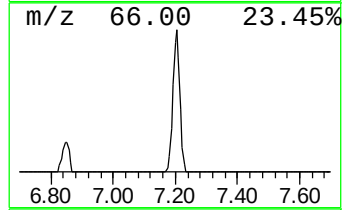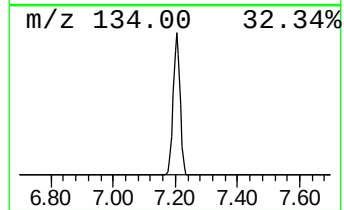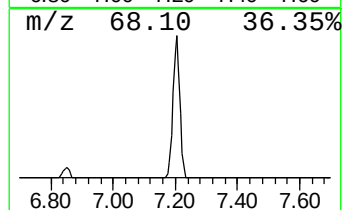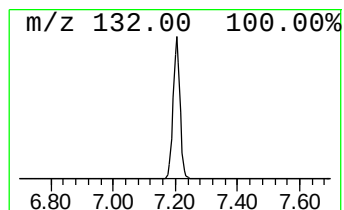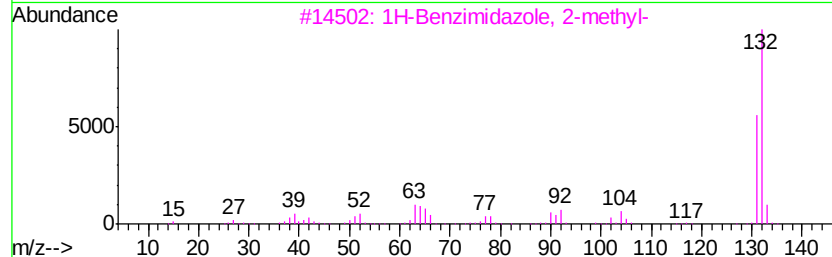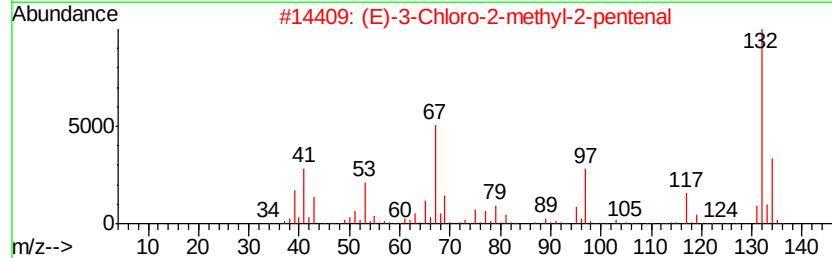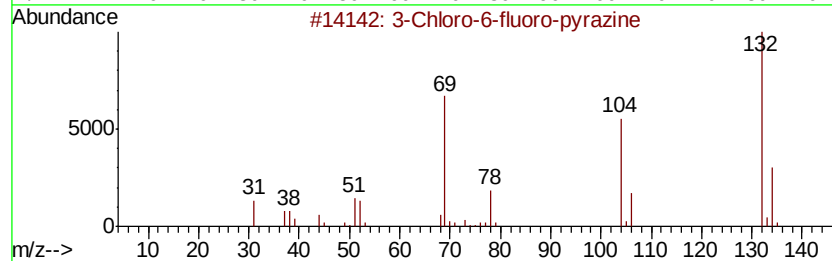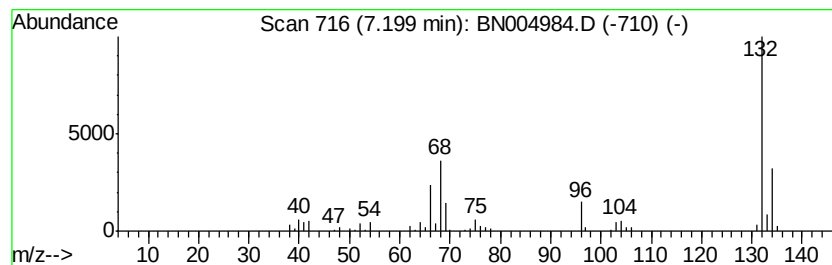

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032619\
Data File : BN004984.D
Acq On : 26 Mar 2019 20:46
Operator : JU/SJ
Sample : PB118232BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118232BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.20	7.20	106.6	ng	284421	1	7.67	53378	20.0