


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032619\
 Data File : BN004971.D
 Acq On : 26 Mar 2019 11:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 27 05:27:09 2019

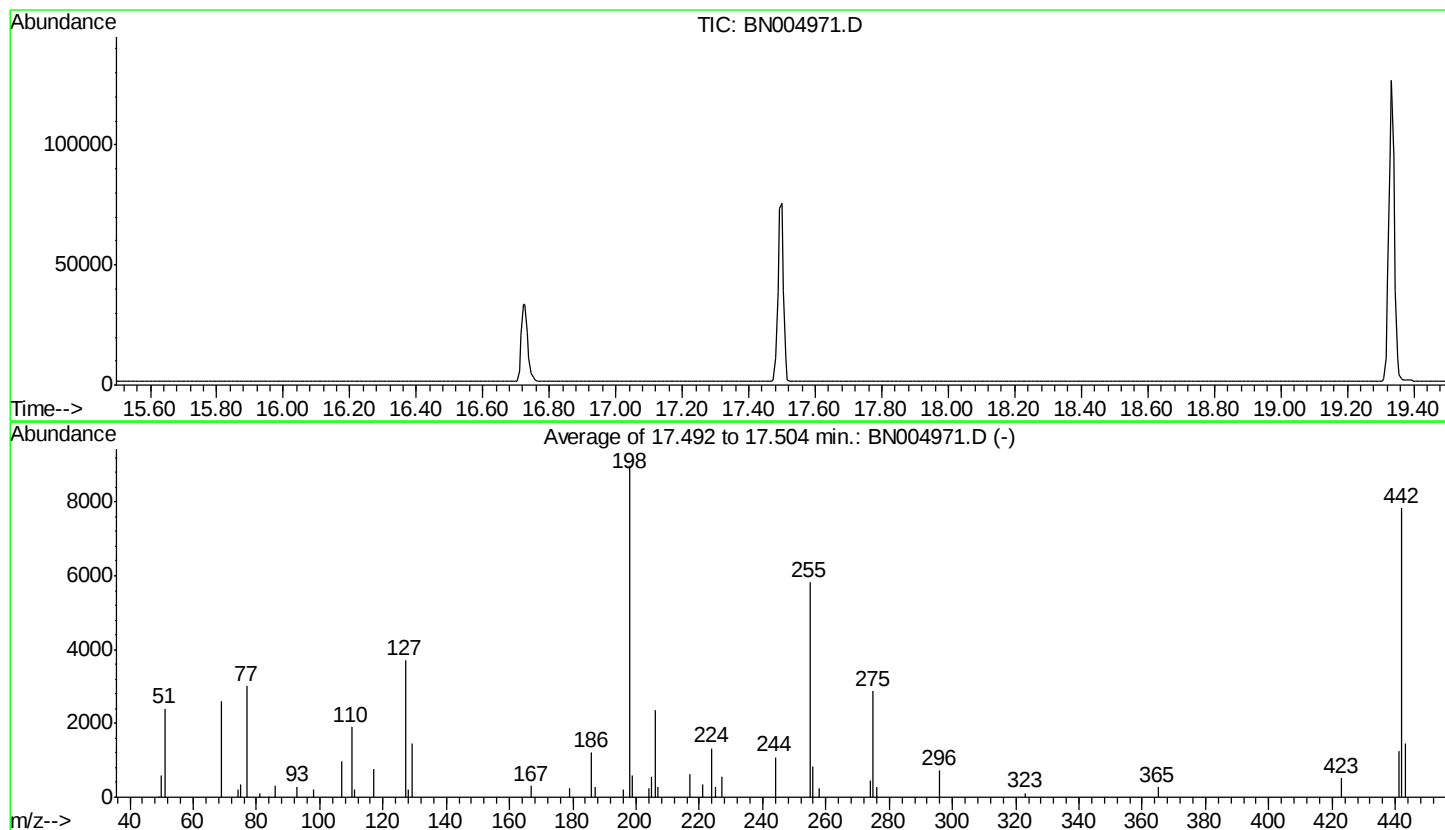

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	2402	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.1	2610	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.3	3710	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8984	PASS
199	198	5	9	6.6	594	PASS
275	198	10	60	32.0	2874	PASS
365	198	1	100	3.1	277	PASS
441	198	0.01	100	13.7	1234	PASS
442	198	50	100	87.1	7827	PASS
443	442	15	24	18.6	1458	PASS