

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032719\
 Data File : BN004997.D
 Acq On : 27 Mar 2019 16:19
 Operator : JU/SJ
 Sample : PB118303BL
 Misc : MDL 8 PPM
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118303BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.269	382	388	396	rBV	147577	198976	43.14%	8.000%
2	6.852	651	657	666	rVB	135512	208281	45.16%	8.374%
3	7.210	711	718	724	rBV	150444	227448	49.31%	9.145%
4	7.675	792	797	803	rVB	31884	45778	9.93%	1.841%
5	7.993	845	851	857	rVB	112458	173584	37.63%	6.979%
6	8.840	988	995	1002	rBV	80932	126891	27.51%	5.102%
7	10.457	1264	1270	1278	rVB	41564	65962	14.30%	2.652%
8	12.934	1685	1691	1698	rVB	239045	333117	72.22%	13.394%
9	14.322	1922	1927	1933	rBV2	61242	88299	19.14%	3.550%
10	15.816	2176	2181	2191	rBV	182369	249107	54.01%	10.016%
11	17.069	2389	2394	2402	rVB2	78728	106506	23.09%	4.282%
12	19.704	2837	2842	2847	rBV	391219	461233	100.00%	18.545%
13	21.269	3103	3108	3115	rBV	84446	108805	23.59%	4.375%
14	23.504	3481	3488	3498	rBV	48530	93146	20.19%	3.745%


Sum of corrected areas: 2487133

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032719\
Data File : BN004997.D
Acq On : 27 Mar 2019 16:19
Operator : JU/SJ
Sample : PB118303BL
Misc : MDL 8 PPM
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118303BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

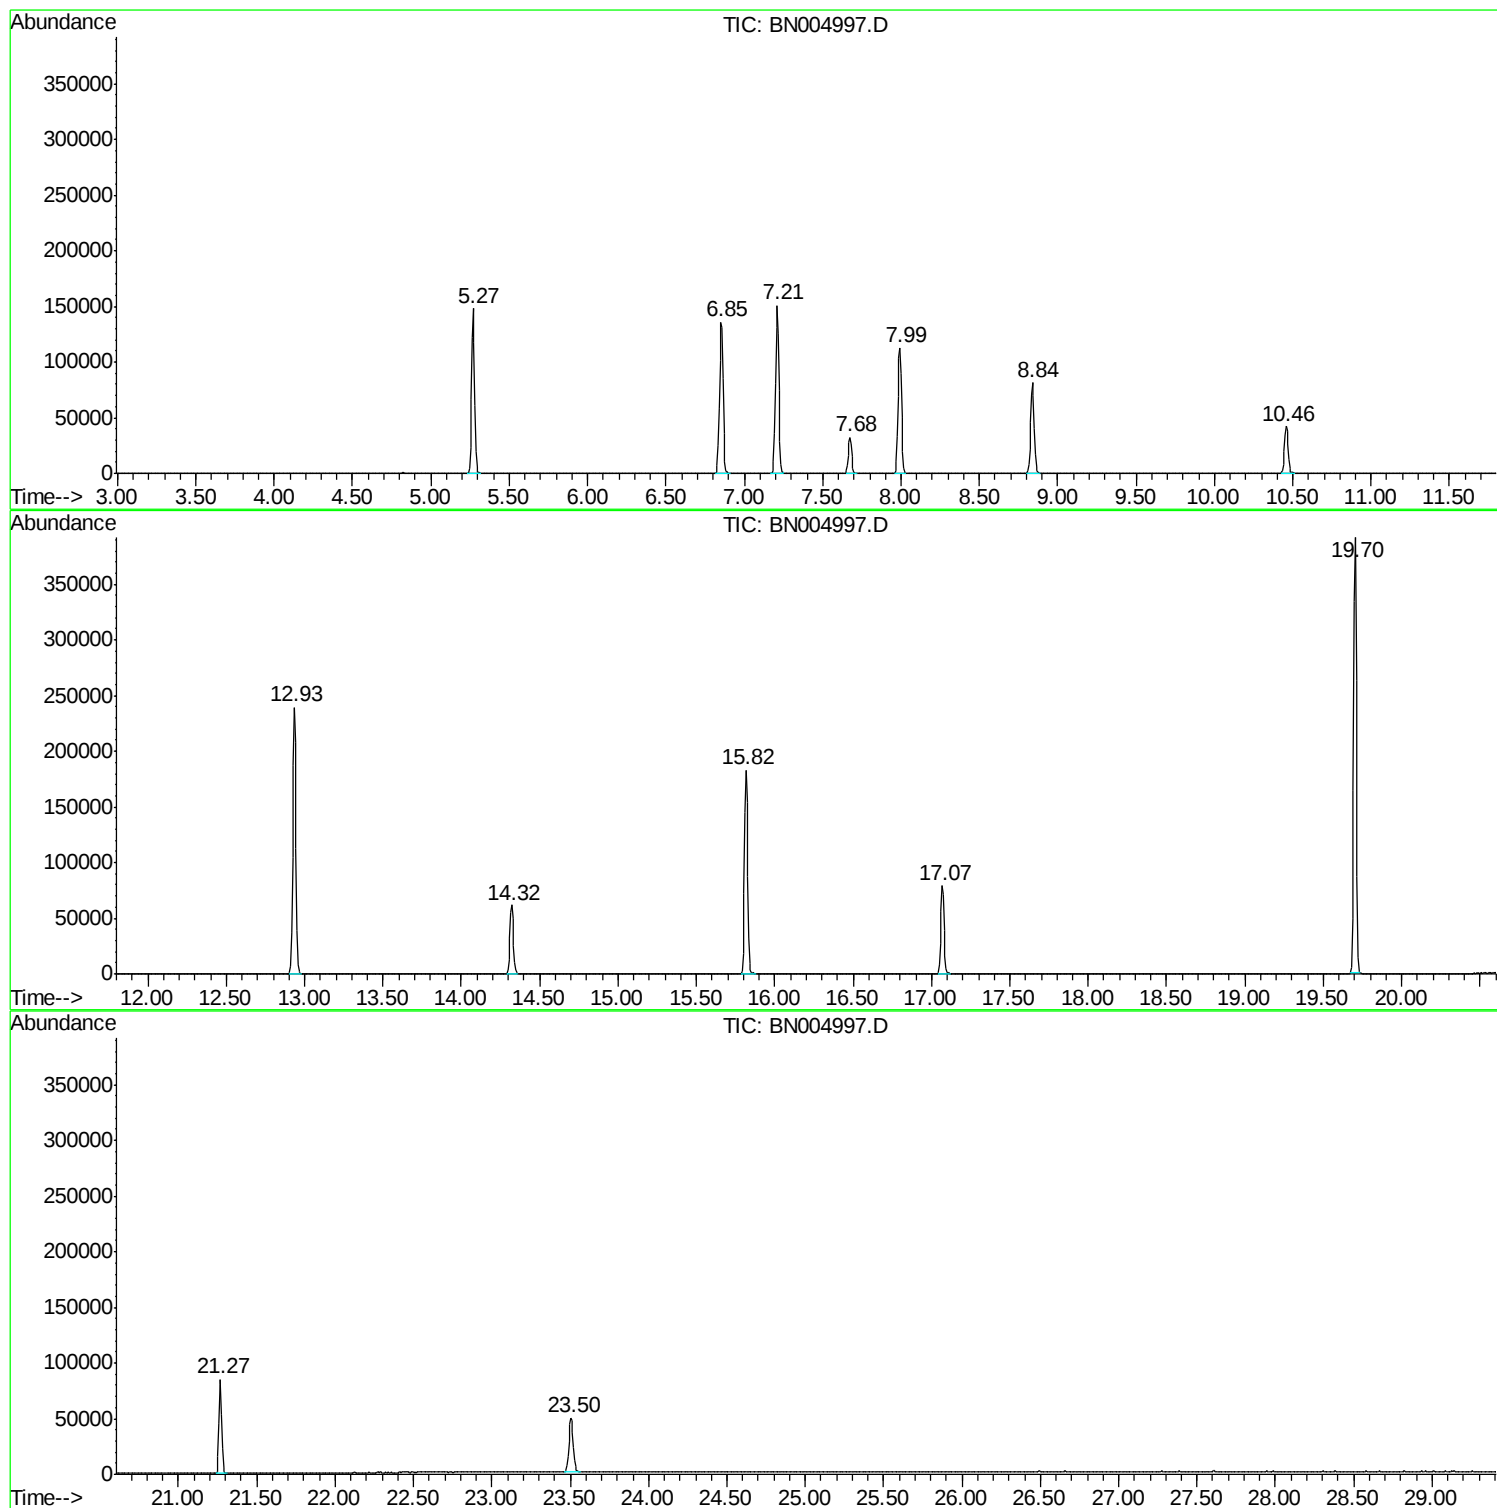

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032719\
Data File : BN004997.D
Acq On : 27 Mar 2019 16:19
Operator : JU/SJ
Sample : PB118303BL
Misc : MDL 8 PPM
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118303BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.21 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.21	99.37 ng	227448	1,4-Dichlorobenzene-d4	7.68

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

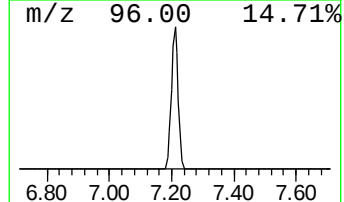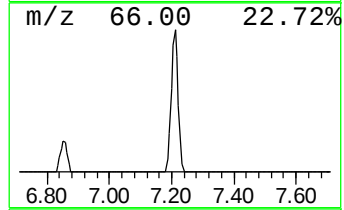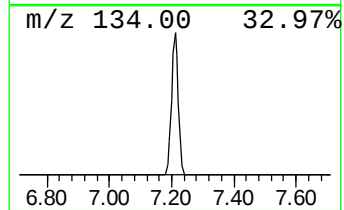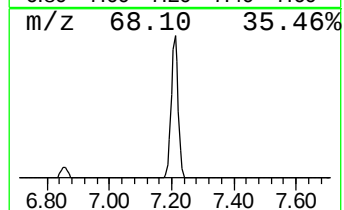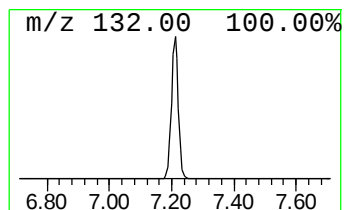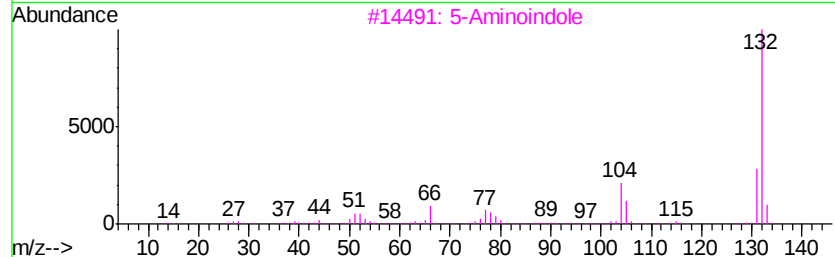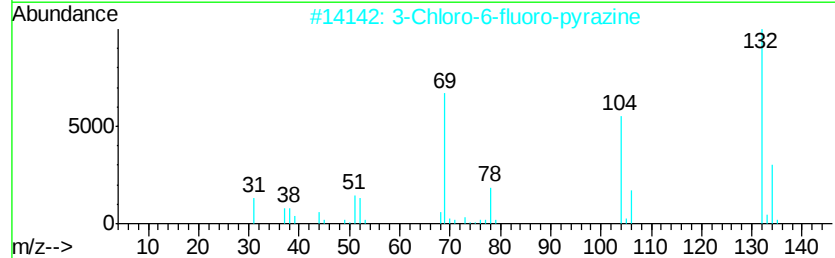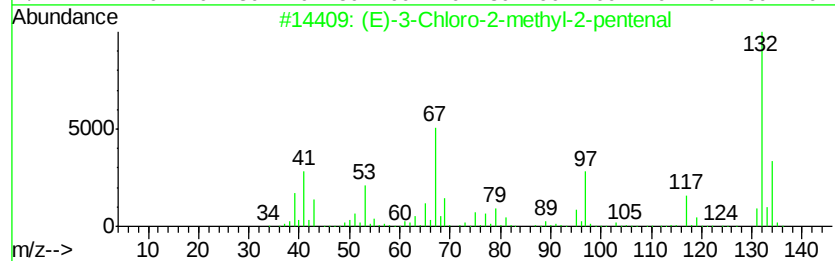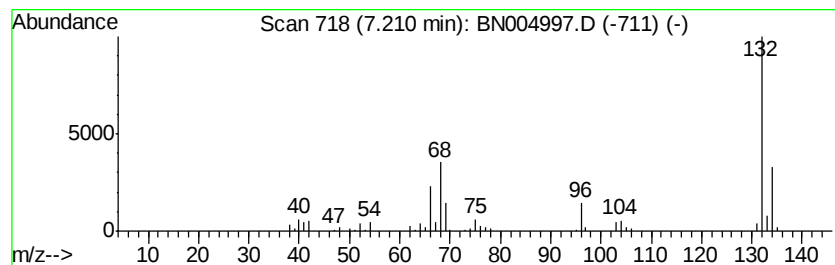

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032719\
Data File : BN004997.D
Acq On : 27 Mar 2019 16:19
Operator : JU/SJ
Sample : PB118303BL
Misc : MDL 8 PPM
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118303BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.21	7.21	99.4	ng	227448	1	7.68	45778	20.0