

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032719\
 Data File : BN005005.D
 Acq On : 27 Mar 2019 21:38
 Operator : JU/SJ
 Sample : PB118091BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118091BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.269	383	388	395	rVB	133878	178322	46.74%	8.195%
2	6.852	651	657	666	rVB	120921	186648	48.92%	8.578%
3	7.210	711	718	724	rBV	134921	203056	53.23%	9.332%
4	7.675	791	797	802	rBB	30225	43757	11.47%	2.011%
5	7.993	844	851	857	rBV	100660	155738	40.82%	7.157%
6	8.840	989	995	1004	rVB	72078	112162	29.40%	5.155%
7	10.457	1263	1270	1278	rBV	40556	62253	16.32%	2.861%
8	12.934	1684	1691	1699	rVB	212277	293314	76.88%	13.480%
9	14.322	1922	1927	1932	rVB2	56729	83288	21.83%	3.828%
10	15.816	2176	2181	2190	rBV	157711	207055	54.27%	9.516%
11	17.069	2389	2394	2403	rVB	74381	98418	25.80%	4.523%
12	19.704	2836	2842	2849	rVB	313788	381504	100.00%	17.533%
13	21.269	3103	3108	3115	rBB	72448	92360	24.21%	4.245%
14	23.504	3482	3488	3497	rBV2	41327	78034	20.45%	3.586%


Sum of corrected areas: 2175909

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032719\
Data File : BN005005.D
Acq On : 27 Mar 2019 21:38
Operator : JU/SJ
Sample : PB118091BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118091BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

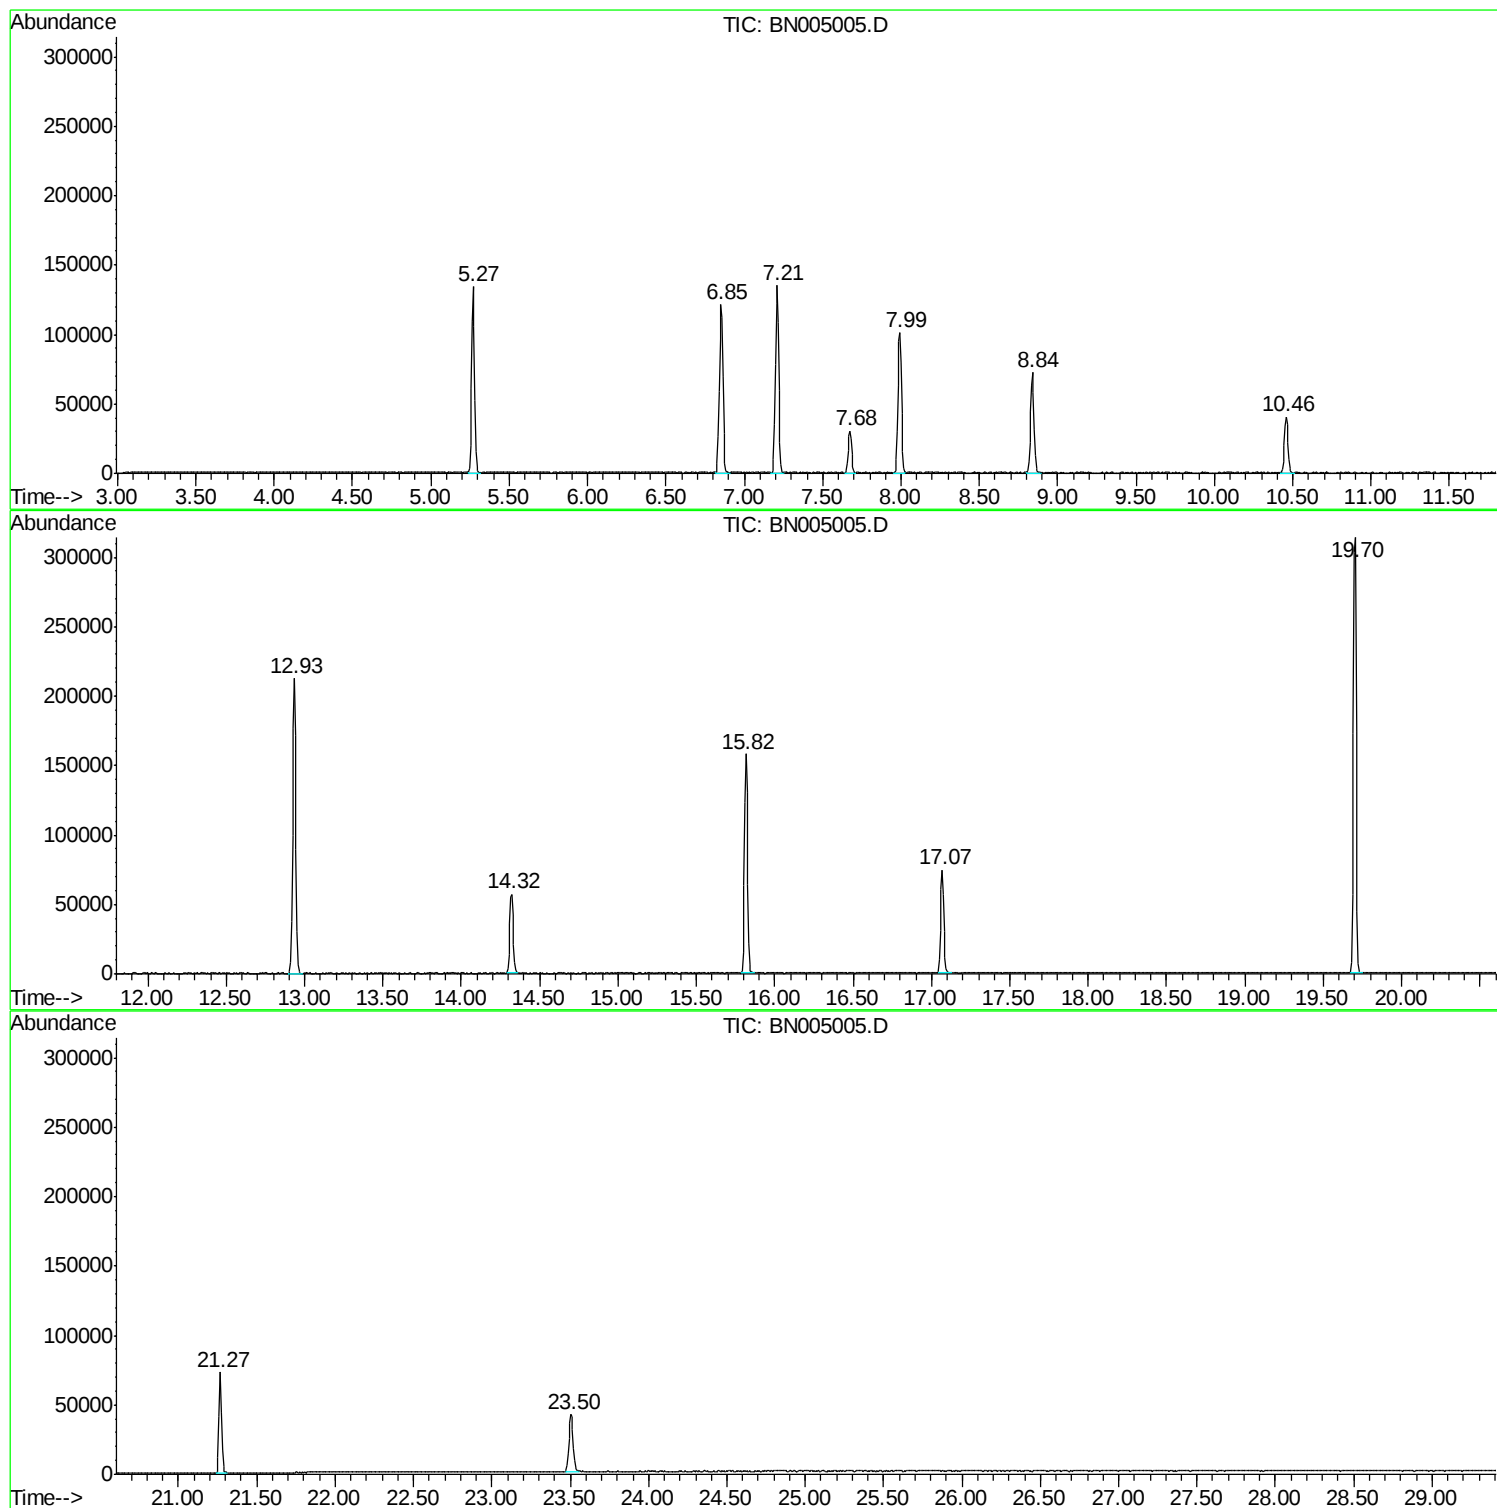

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032719\
Data File : BN005005.D
Acq On : 27 Mar 2019 21:38
Operator : JU/SJ
Sample : PB118091BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118091BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.21 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.21	92.81 ng	203056	1,4-Dichlorobenzene-d4	7.68

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

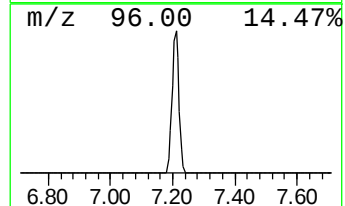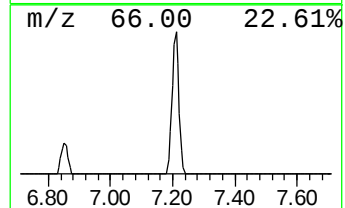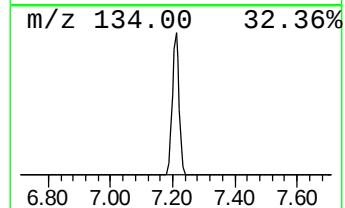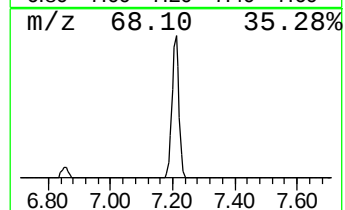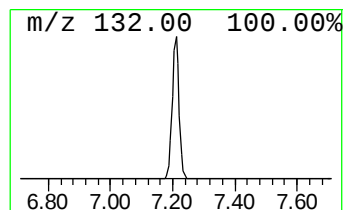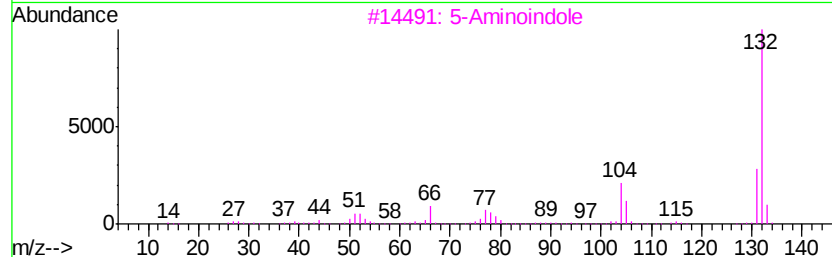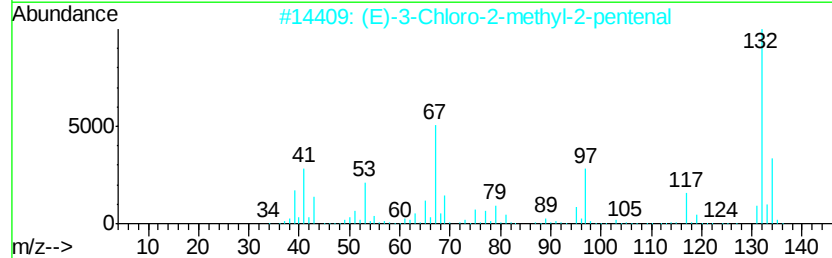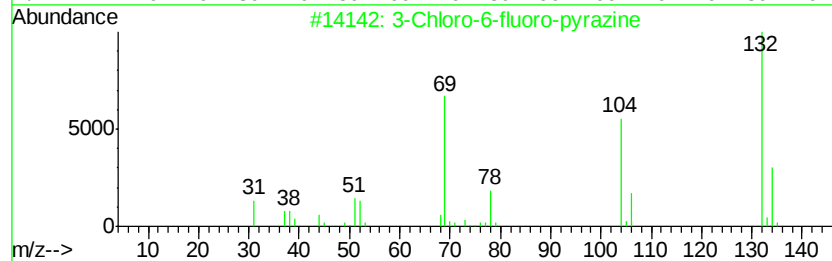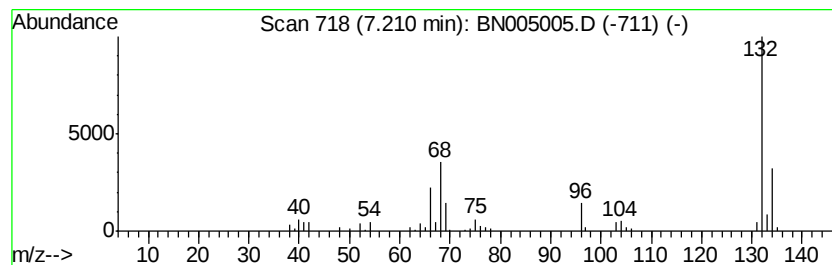

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032719\
Data File : BN005005.D
Acq On : 27 Mar 2019 21:38
Operator : JU/SJ
Sample : PB118091BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118091BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.21	7.21	92.8	ng	203056	1	7.68	43757	20.0