
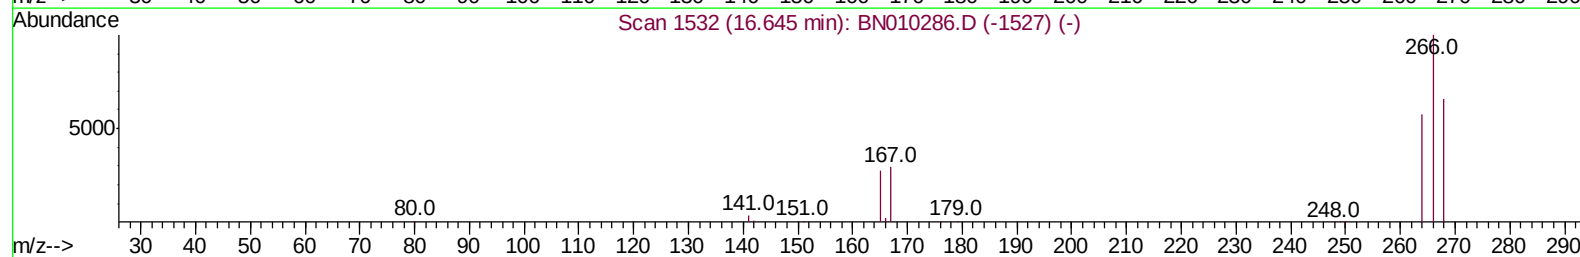
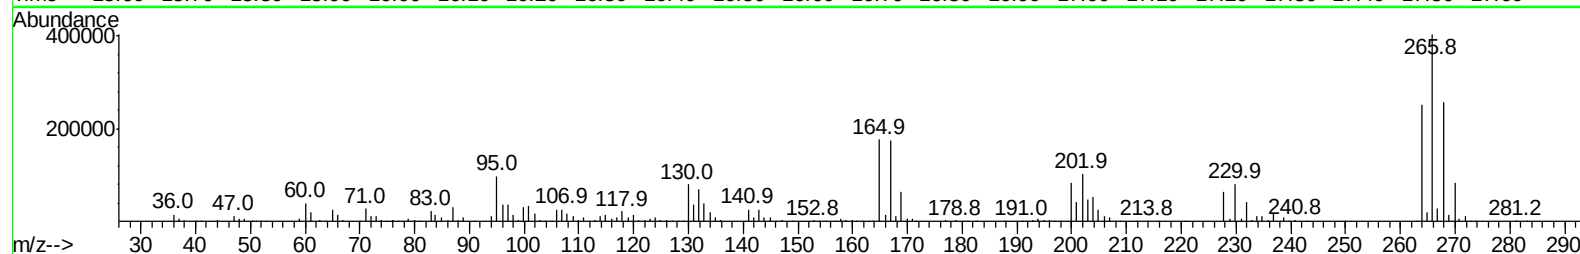


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN032720\
Data File : BN010348.D
Acq On : 27 Mar 2020 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 21:45:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 19 15:26:45 2020
Response via : Initial Calibration

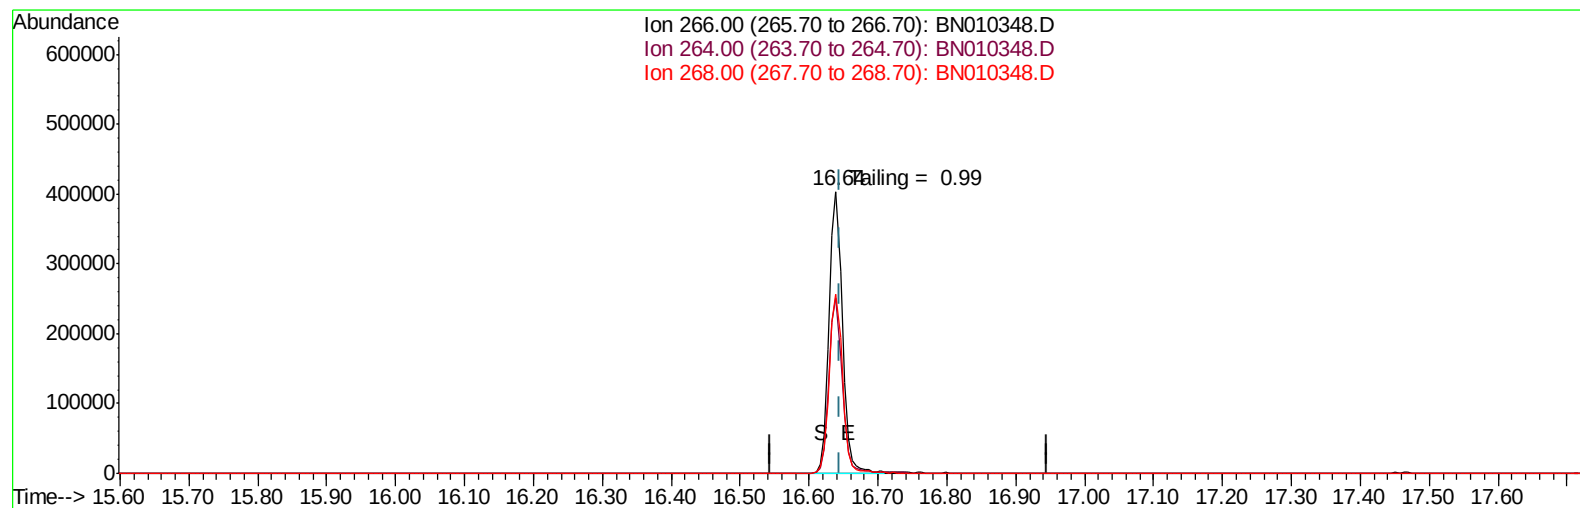

TIC: BN010348.D

(22) Pentachlorophenol

16.639min (-0.006) 0.00ng

response 537788

Ion	Exp%	Act%
266.00	100	100
264.00	59.60	62.28
268.00	68.60	63.55
0.00	0.00	0.00