


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN032720\
 Data File : BN010348.D
 Acq On : 27 Mar 2020 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 15:26:45 2020

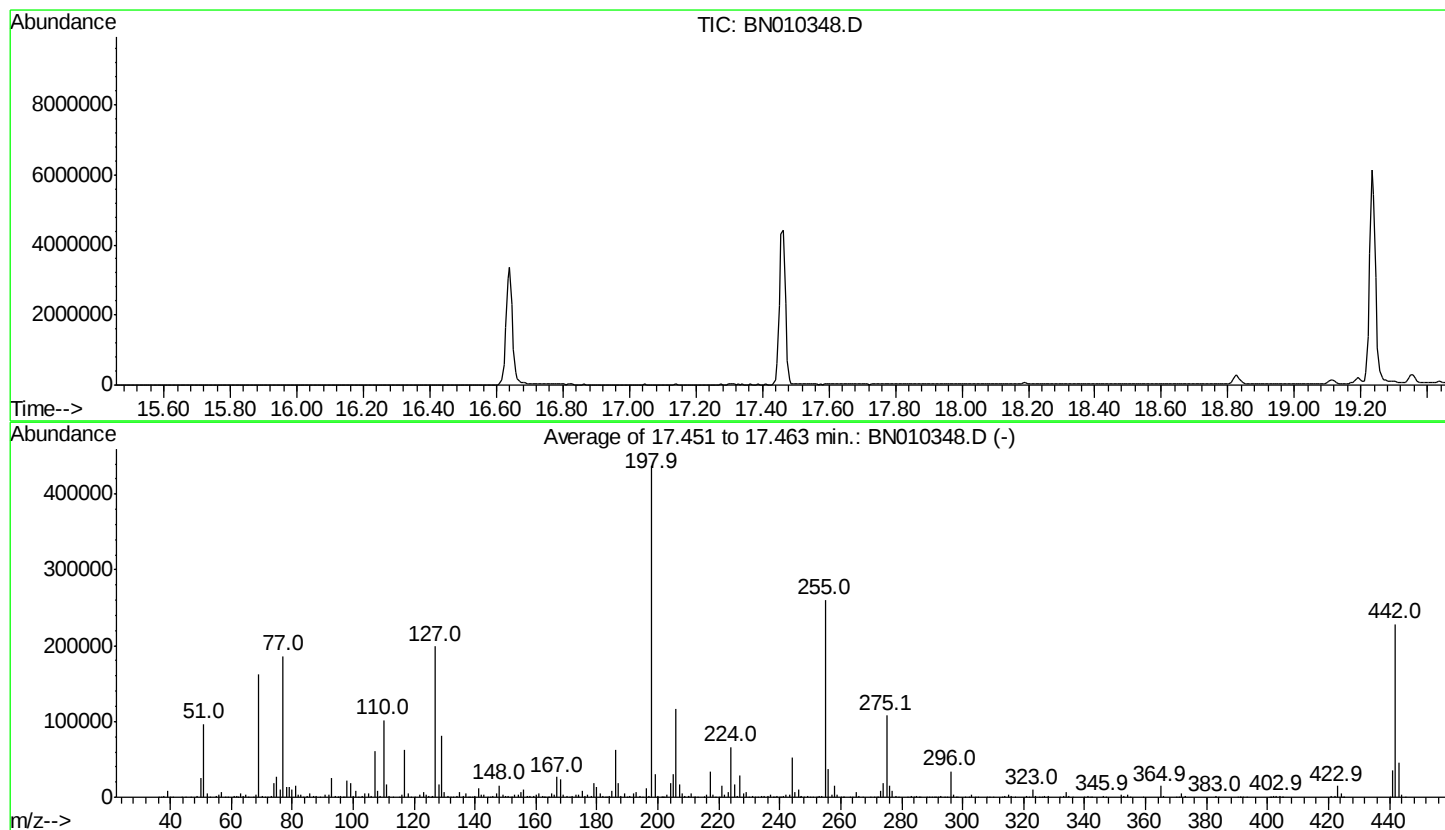

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.1	96509	PASS
68	69	0.00	2	2.0	3242	PASS
69	198	0.00	100	37.2	162952	PASS
70	69	0.00	2	0.7	1118	PASS
127	198	10	80	45.4	198736	PASS
197	198	0.00	2	0.4	1779	PASS
198	198	100	100	100.0	437546	PASS
199	198	5	9	7.1	31064	PASS
275	198	10	60	24.6	107437	PASS
365	198	1	100	3.4	14759	PASS
441	198	0.01	100	8.2	35861	PASS
442	198	50	100	52.3	228813	PASS
443	442	15	24	20.2	46264	PASS