




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032724\
 Data File : BN030508.D
 Acq On : 27 Mar 2024 16:54
 Operator : MA/JU
 Sample : P1848-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0LY4

Manual IntegrationsAPPROVED

Quant Time: Mar 27 17:25:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2024
 Supervised By :mohammad ahmed 03/29/2024

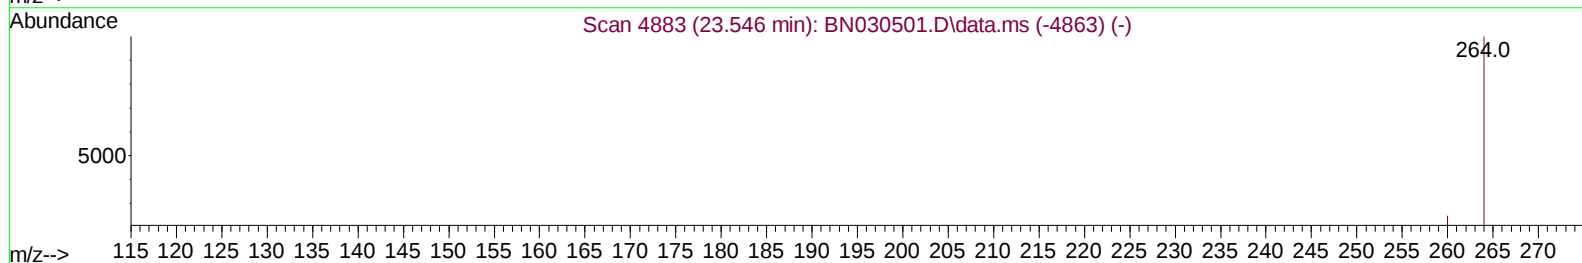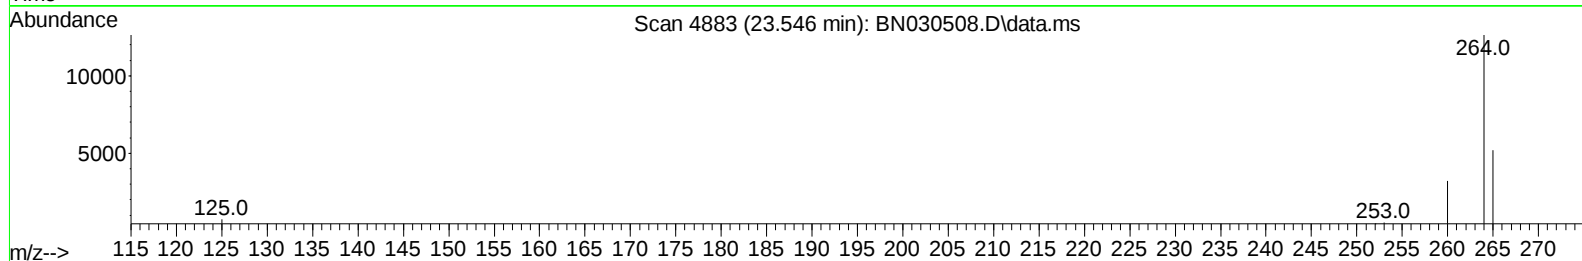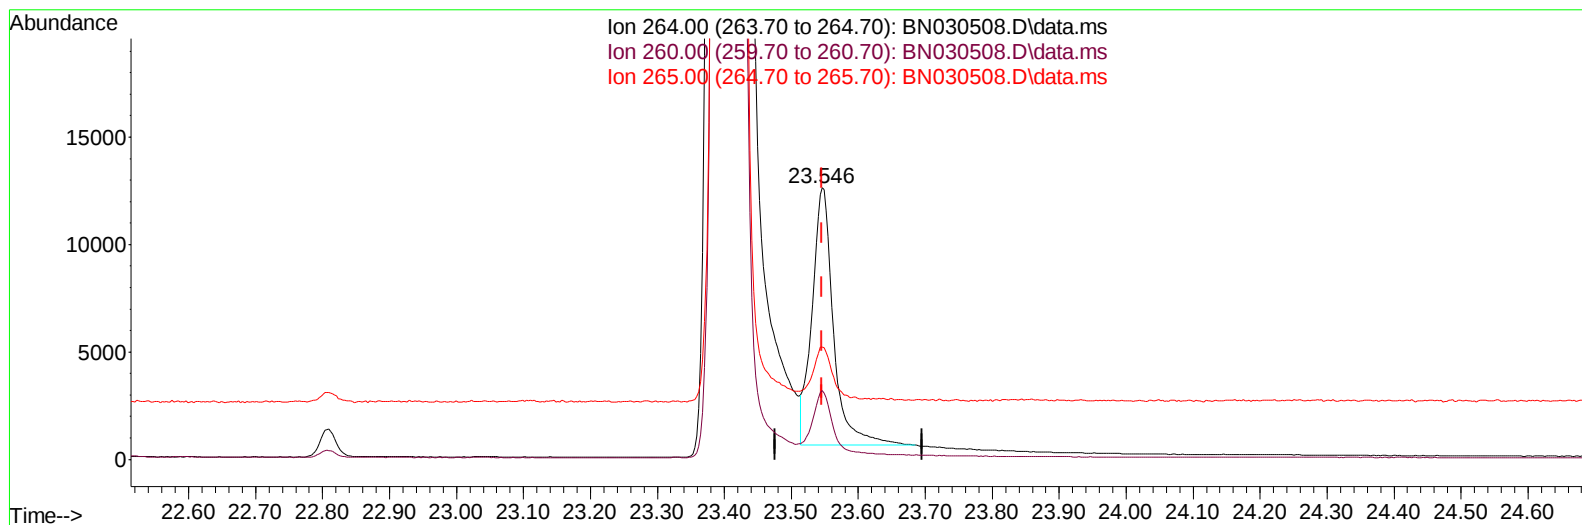

TIC: BN030508.D\data.ms

(23) Perylene-d12 (I)

23.546min (+ 0.000) 0.40 ng/u1

response 26920

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	25.39
265.00	52.70	41.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032724\
Data File : BN030508.D
Acq On : 27 Mar 2024 16:54
Operator : MA/JU
Sample : P1848-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0LY4

Manual IntegrationsAPPROVED

Quant Time: Mar 27 17:25:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2024
Supervised By :mohammad ahmed 03/29/2024

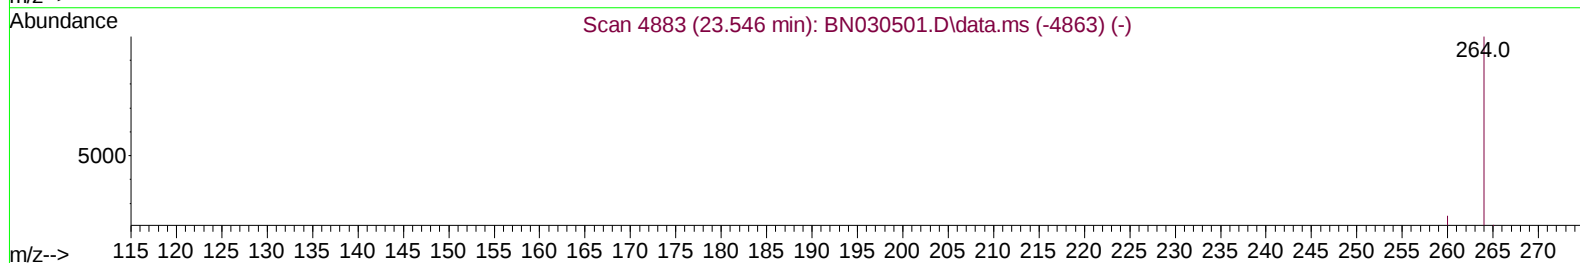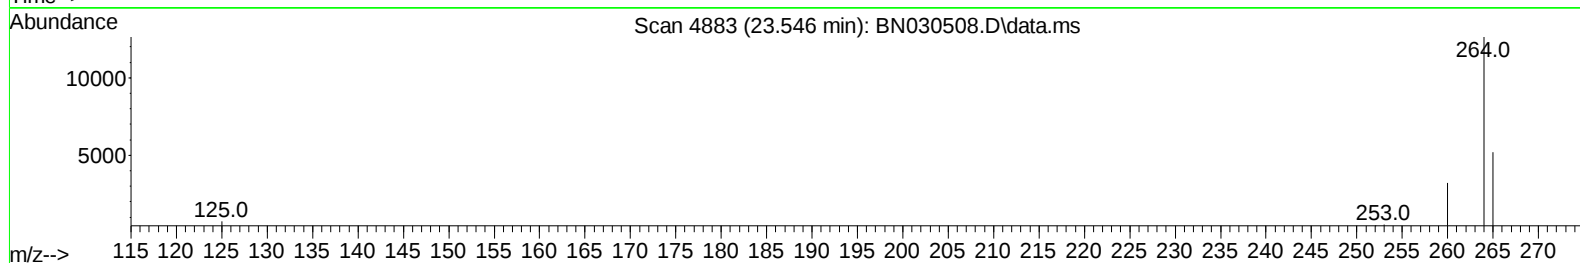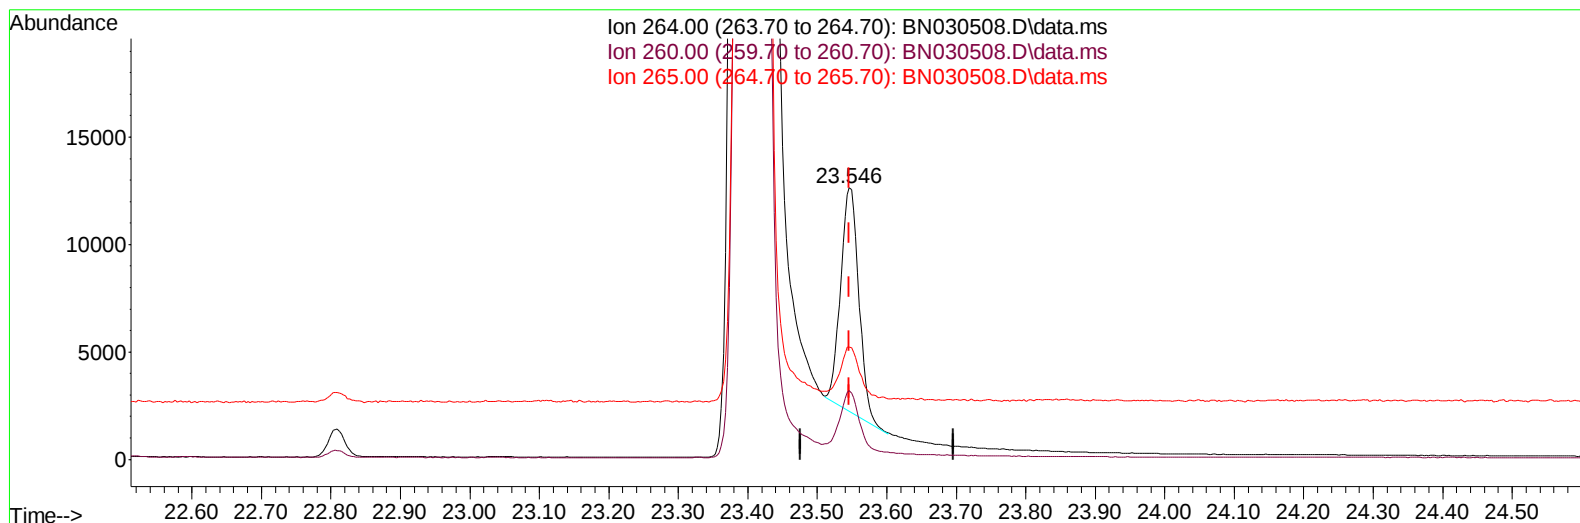

TIC: BN030508.D\data.ms

(23) Perylene-d12 (I)

23.546min (+ 0.000) 0.40 ng/ul m

response 18793

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	25.39
265.00	52.70	41.28#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032724\
 Data File : BN030508.D
 Acq On : 27 Mar 2024 16:54
 Operator : MA/JU
 Sample : P1848-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0LY4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2024
 Supervised By :mohammad ahmed 03/29/2024

Quant Time: Mar 27 17:25:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.724	152		5930	0.400	ng/ul	0.00
4) Naphthalene-d8	10.506	136		19778	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.362	164		13108	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.107	188		31936	0.400	ng/ul	0.00
17) Chrysene-d12	21.298	240		25662	0.400	ng/ul	0.00
23) Perylene-d12	23.546	264		18793m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.218	96		33090	5.093	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.101	152		10463	0.351	ng/ul	0.00
18) Fluoranthene-d10	19.136	212		33497	0.422	ng/ul	0.00
Target Compounds							
						Qvalue	
2) 1,4-Dioxane	3.252	88		264	0.040	ng/ul#	41

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032724\
Data File : BN030508.D
Acq On : 27 Mar 2024 16:54
Operator : MA/JU
Sample : P1848-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0LY4

Manual IntegrationsAPPROVED

Quant Time: Mar 27 17:25:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2024
Supervised By :mohammad ahmed 03/29/2024

