




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032724\
 Data File : BN030511.D
 Acq On : 27 Mar 2024 18:43
 Operator : MA/JU
 Sample : P1848-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0LY6

Manual IntegrationsAPPROVED

Quant Time: Mar 27 23:32:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2024
 Supervised By :mohammad ahmed 03/29/2024

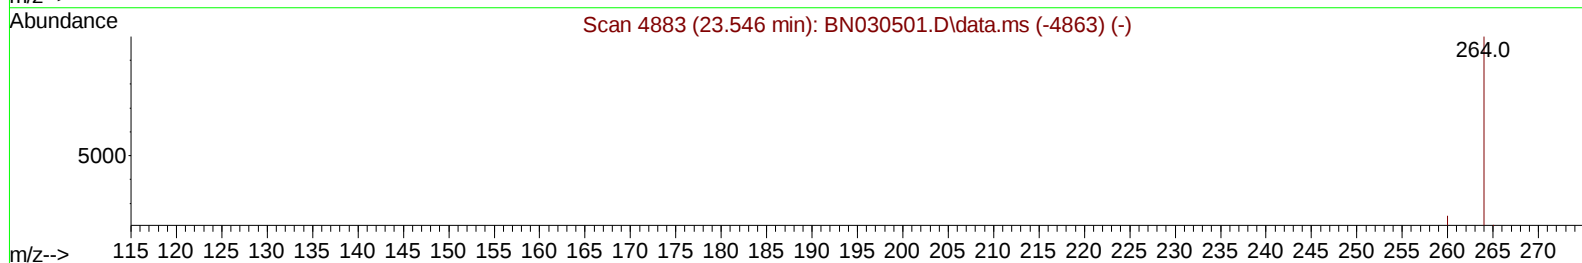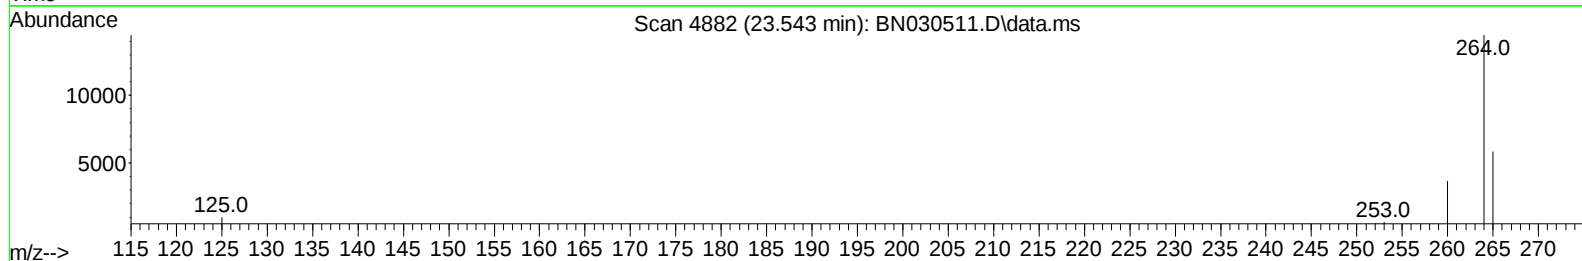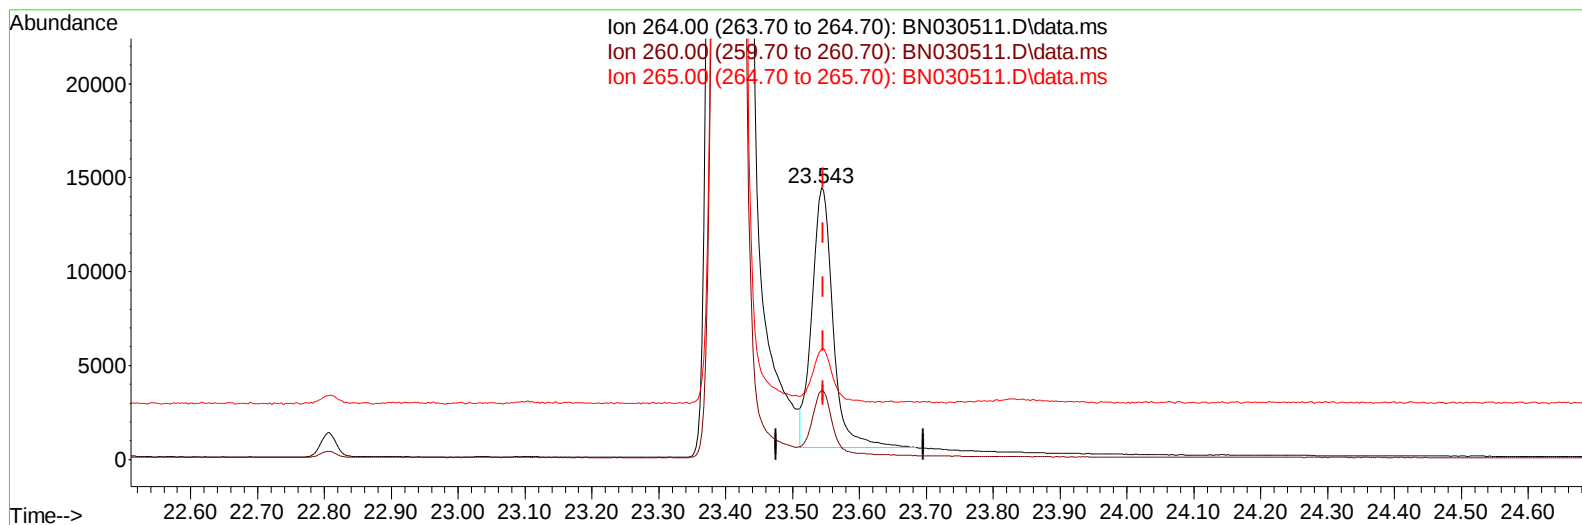

TIC: BN030511.D\data.ms

(23) Perylene-d12 (I)

23.543min (-0.003) 0.40 ng/u1

response 30317

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	25.33
265.00	52.70	40.62#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032724\
Data File : BN030511.D
Acq On : 27 Mar 2024 18:43
Operator : MA/JU
Sample : P1848-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOLY6

Manual IntegrationsAPPROVED

Quant Time: Mar 27 23:32:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2024
Supervised By :mohammad ahmed 03/29/2024

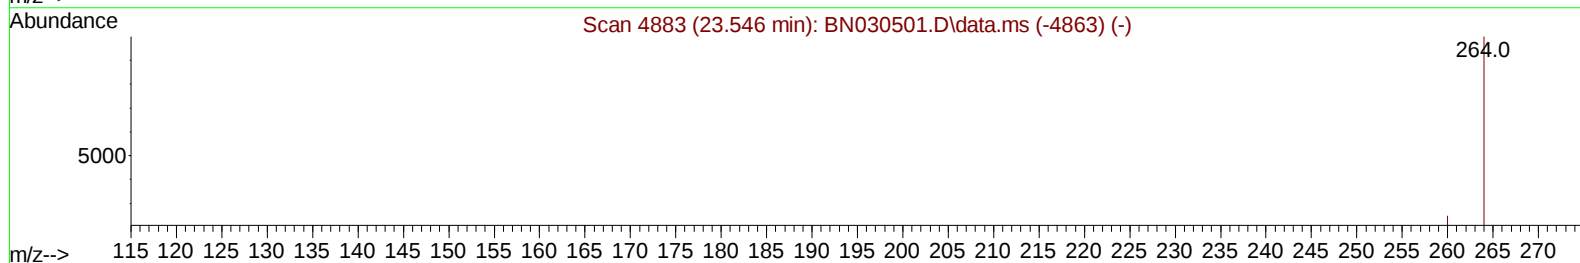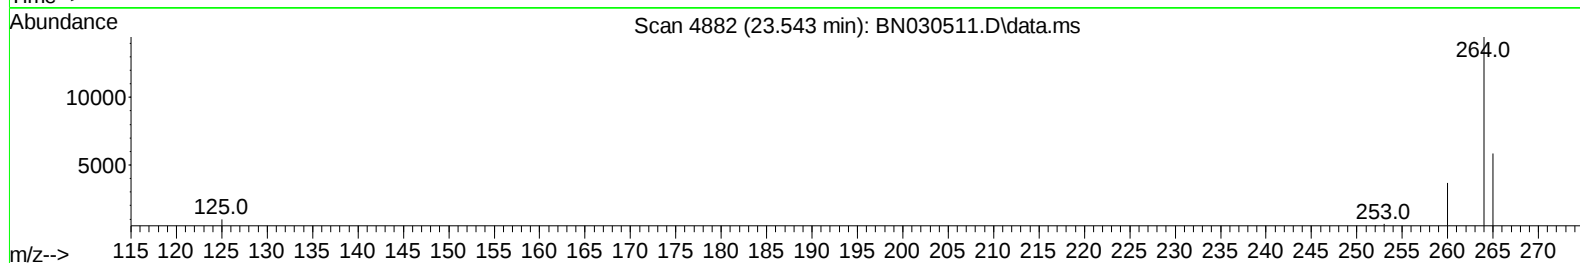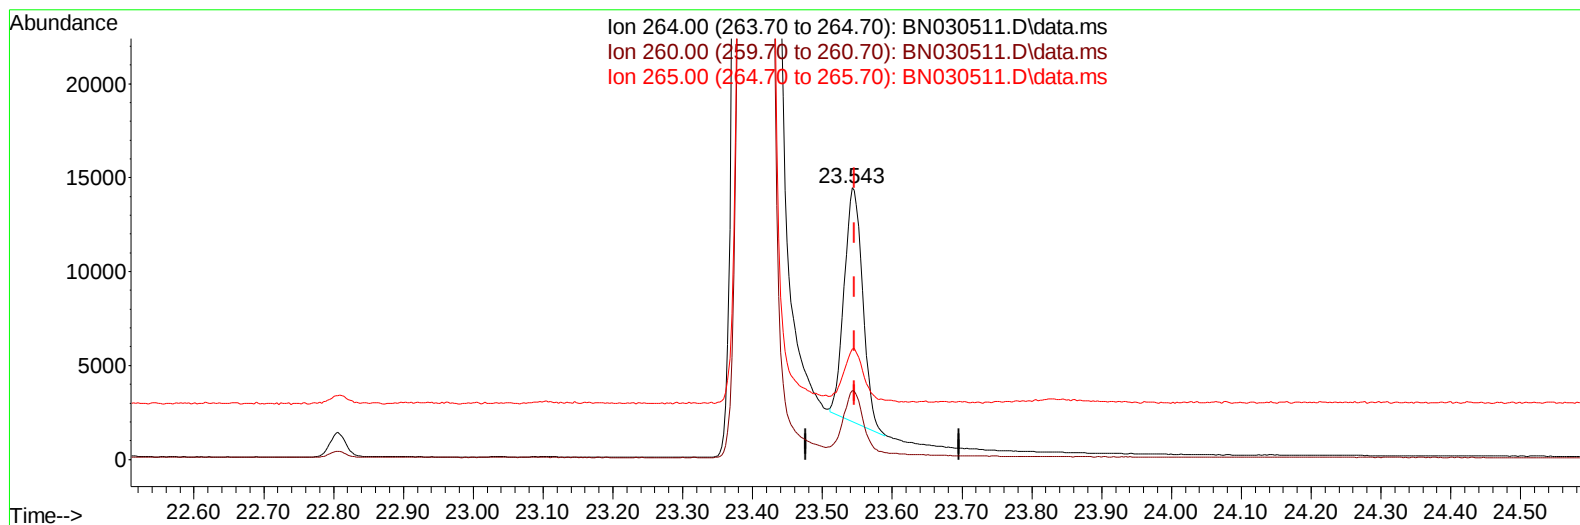

TIC: BN030511.D\data.ms

(23) Perylene-d12 (I)

23.543min (-0.003) 0.40 ng/ul m

response 23044

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	25.33
265.00	52.70	40.62#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032724\
 Data File : BN030511.D
 Acq On : 27 Mar 2024 18:43
 Operator : MA/JU
 Sample : P1848-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0LY6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2024
 Supervised By :mohammad ahmed 03/29/2024

Quant Time: Mar 27 23:32:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.724	152	6548	0.400	ng/ul	0.00
4) Naphthalene-d8	10.507	136	21931	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.359	164	14574	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.104	188	35612	0.400	ng/ul	0.00
17) Chrysene-d12	21.298	240	29173	0.400	ng/ul	0.00
23) Perylene-d12	23.543	264	23044m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	31911	4.448	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.097	152	10826	0.328	ng/ul	0.00
18) Fluoranthene-d10	19.137	212	30696	0.340	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032724\
Data File : BN030511.D
Acq On : 27 Mar 2024 18:43
Operator : MA/JU
Sample : P1848-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0LY6

Manual IntegrationsAPPROVED

Quant Time: Mar 27 23:32:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2024
Supervised By :mohammad ahmed 03/29/2024

