


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032819\
 Data File : BN005015.D
 Acq On : 28 Mar 2019 16:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 29 03:42:17 2019

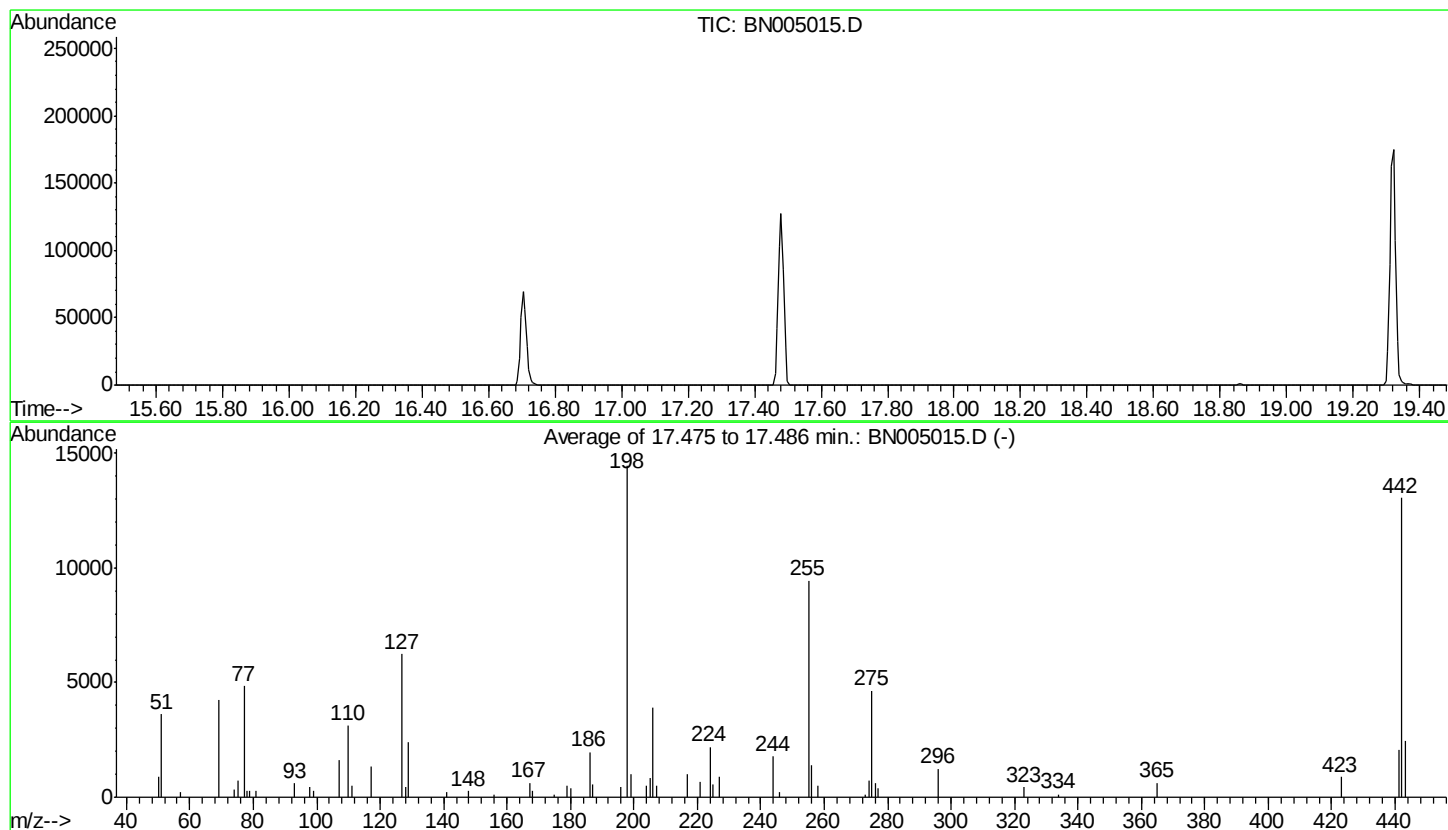

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	3611	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.5	4267	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.1	6235	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14467	PASS
199	198	5	9	6.9	991	PASS
275	198	10	60	32.1	4642	PASS
365	198	1	100	4.3	618	PASS
441	198	0.01	100	14.4	2089	PASS
442	198	50	100	90.2	13052	PASS
443	442	15	24	18.9	2472	PASS