
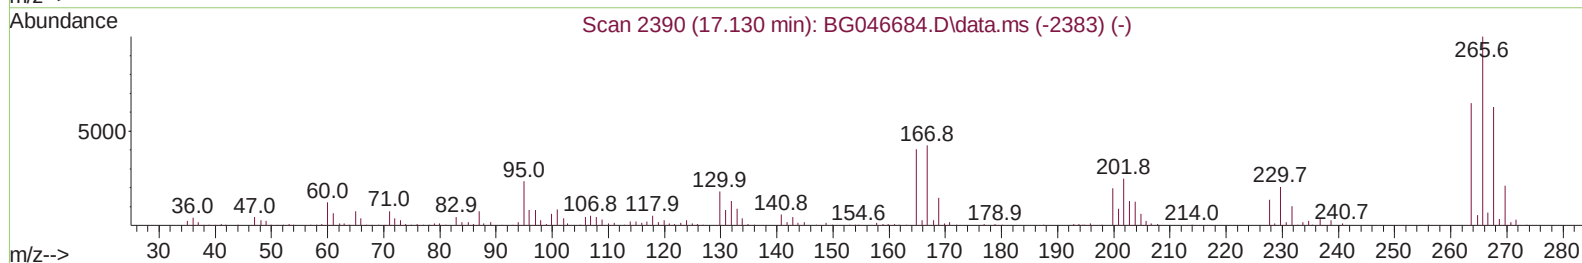
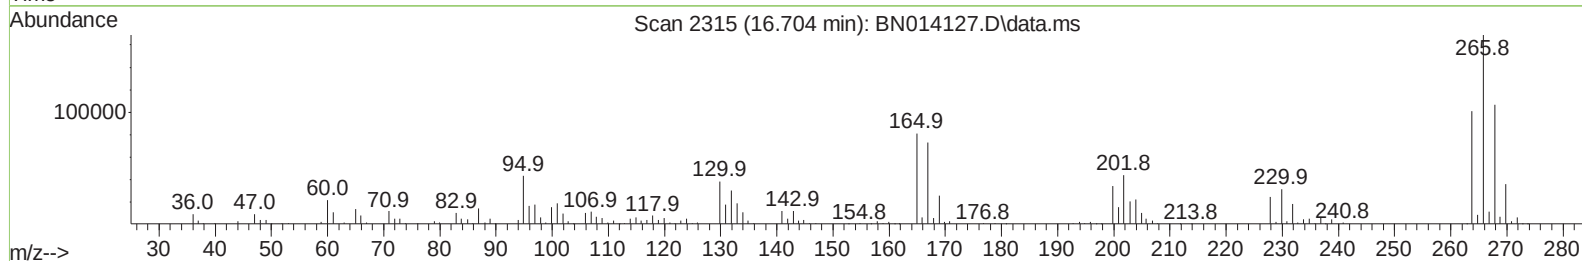


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032921\
Data File : BN014127.D
Acq On : 29 Mar 2021 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 11:58:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

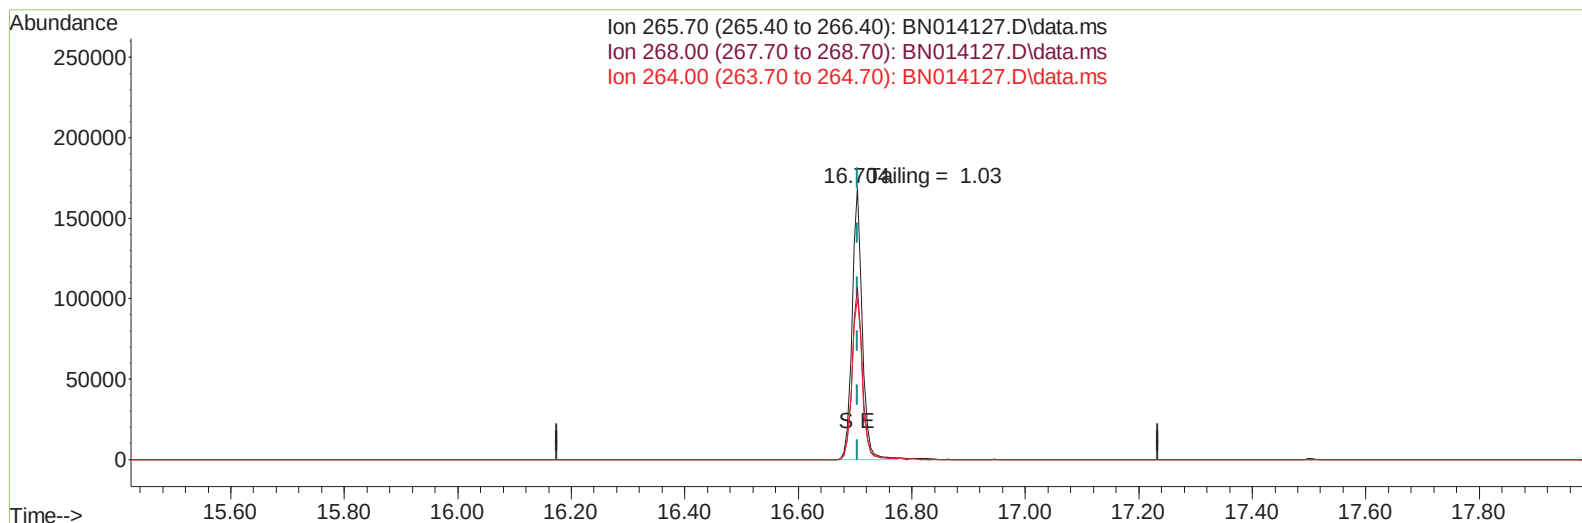

TIC: BN014127.D\data.ms

(70) Pentachlorophenol (C)**16.704min (-0.000) 20670.90 ng****response 212346**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.28
264.00	61.60	59.62
0.00	0.00	0.00



Abundance

Ion 184.00 (183.70 to 184.70): BN014127.D\data.ms
 Ion 185.00 (184.70 to 185.70): BN014127.D\data.ms
 Ion 183.00 (182.70 to 183.70): BN014127.D\data.ms

19.298 min, Tailing = 1.02

S.E

Time-->

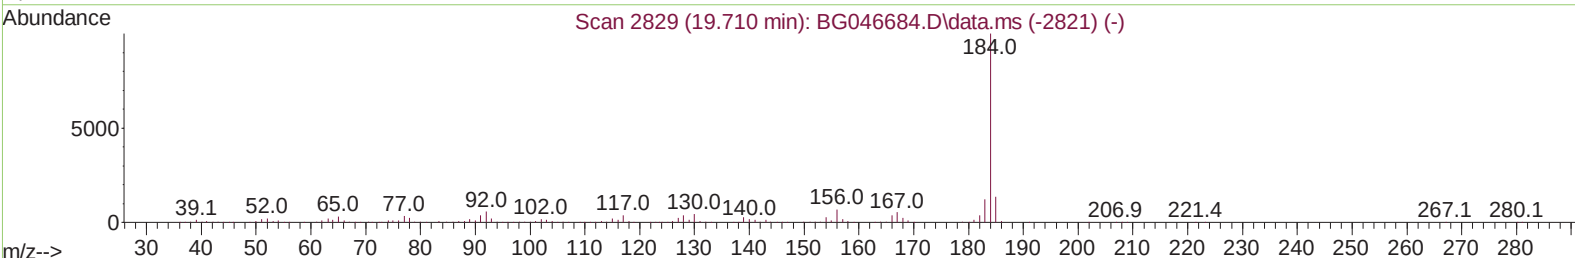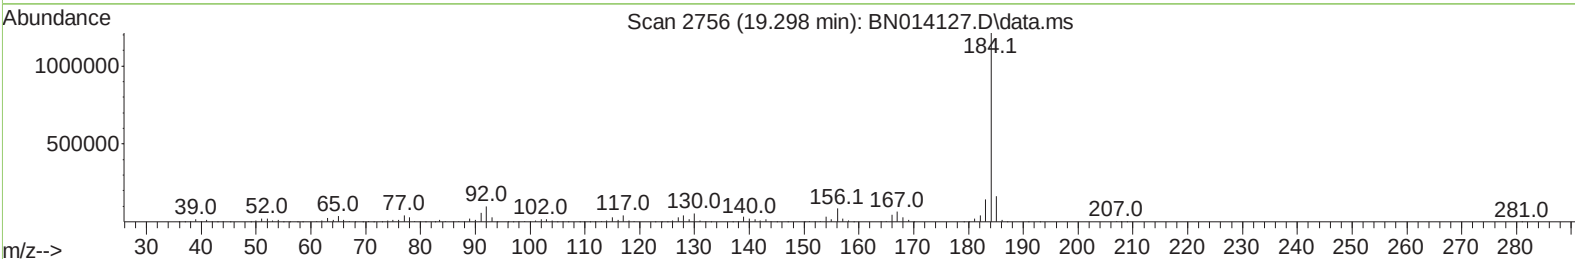

TIC: BN014127.D\data.ms

response **1380507**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.51
183.00	13.20	11.79
0.00	0.00	0.00