
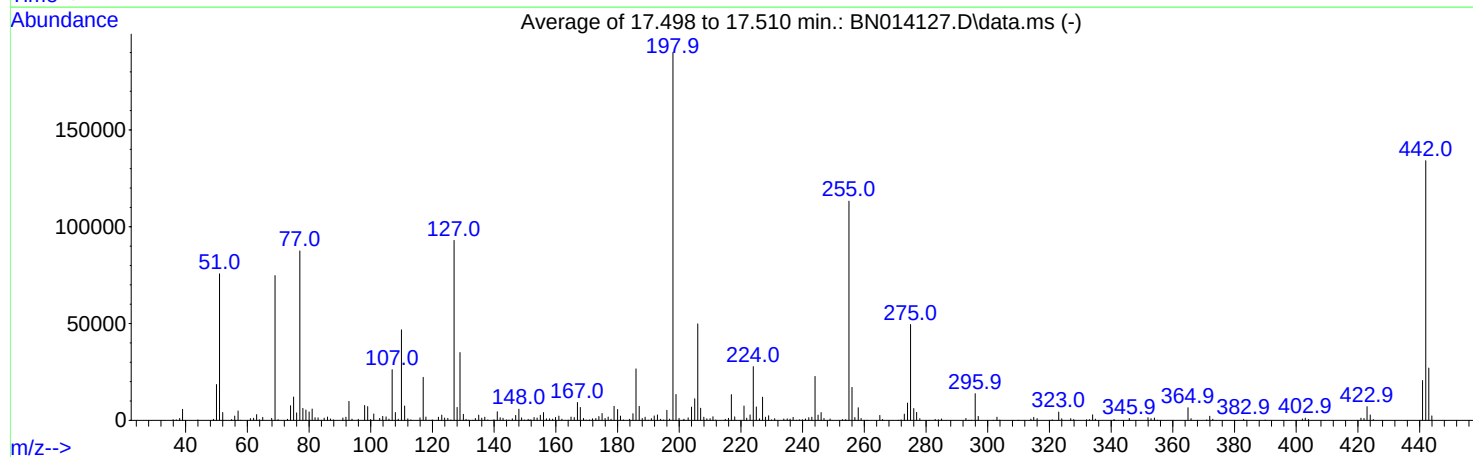


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032921\
 Data File : BN014127.D
 Acq On : 29 Mar 2021 11:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 29 12:24:58 2021

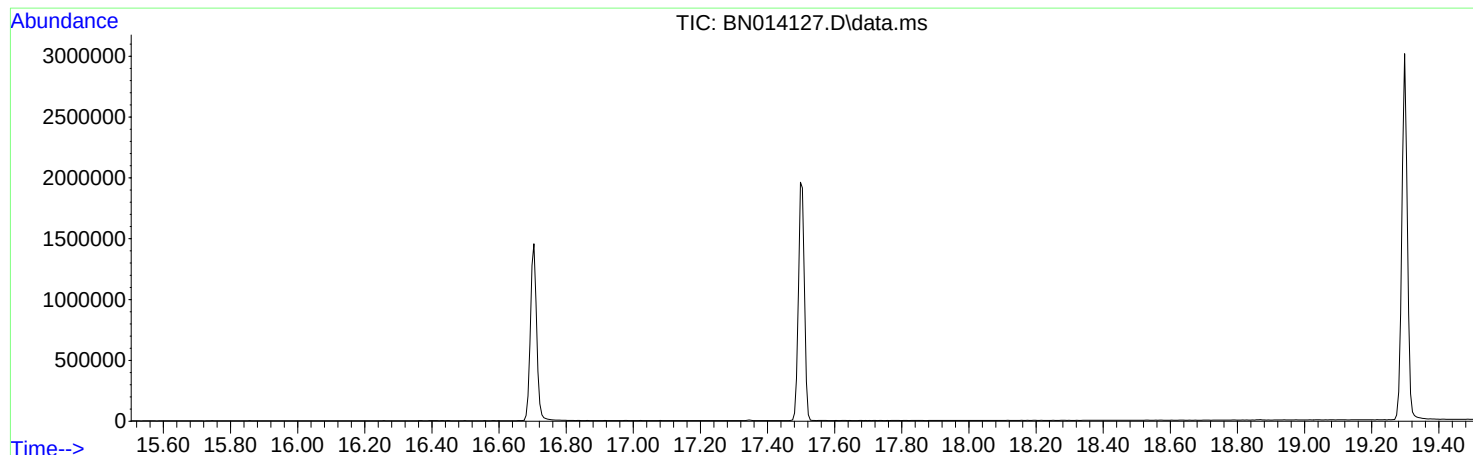




AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	75741	PASS
68	69	0.00	2	1.5	1118	PASS
69	198	0.00	100	39.4	74813	PASS
70	69	0.00	2	0.5	406	PASS
127	198	10	80	48.9	92968	PASS
197	198	0.00	2	0.3	646	PASS
198	198	100	100	100.0	190021	PASS
199	198	5	9	7.0	13366	PASS
275	198	10	60	26.1	49536	PASS
365	198	1	100	3.4	6537	PASS
441	198	0.01	100	10.9	20624	PASS
442	442	50	100	100.0	134136	PASS
443	442	15	24	20.1	27008	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032921\
Data File : BN014127.D
Acq On : 29 Mar 2021 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 29 11:58:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

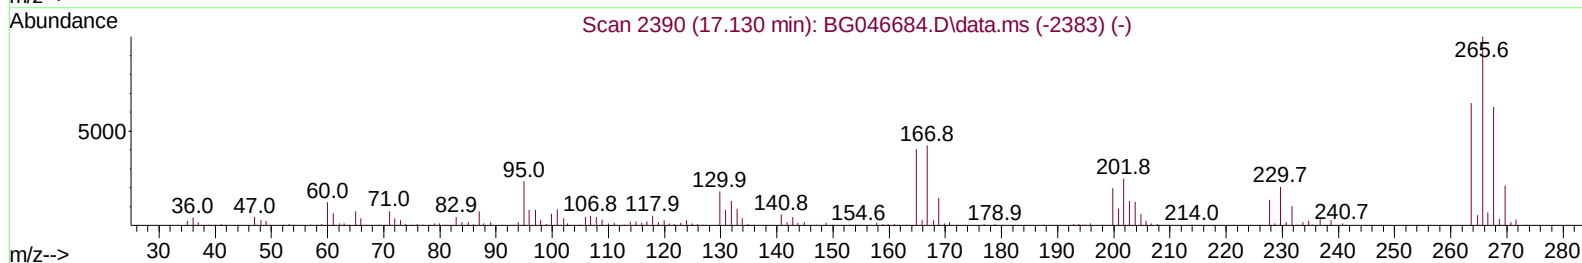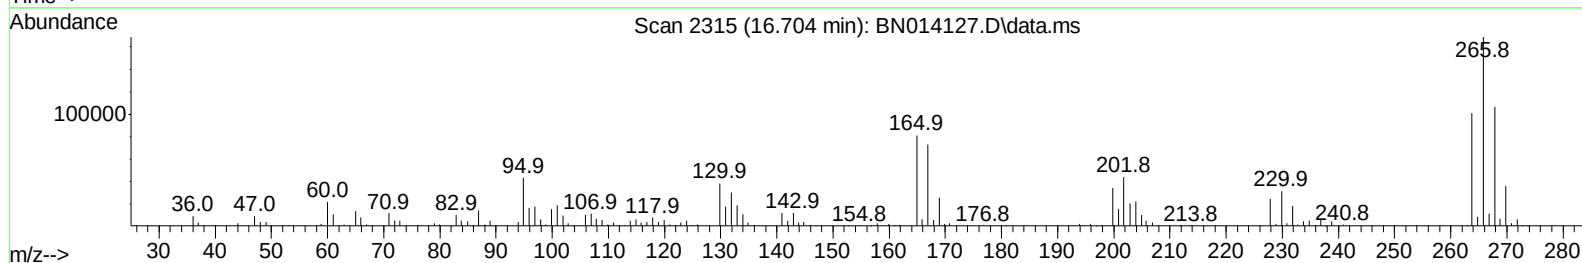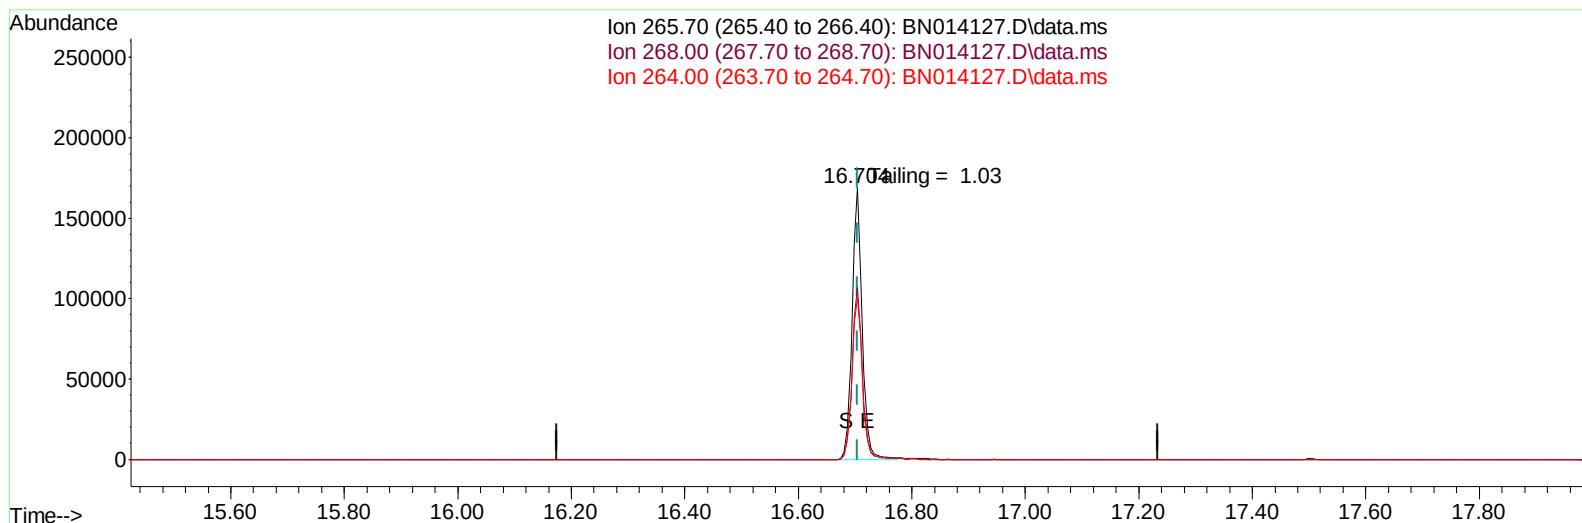

TIC: BN014127.D\data.ms

(70) Pentachlorophenol (C)

16.704min (-0.000) 20670.90 ng




response 212346

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.28
264.00	61.60	59.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032921\
Data File : BN014127.D
Acq On : 29 Mar 2021 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 29 11:58:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

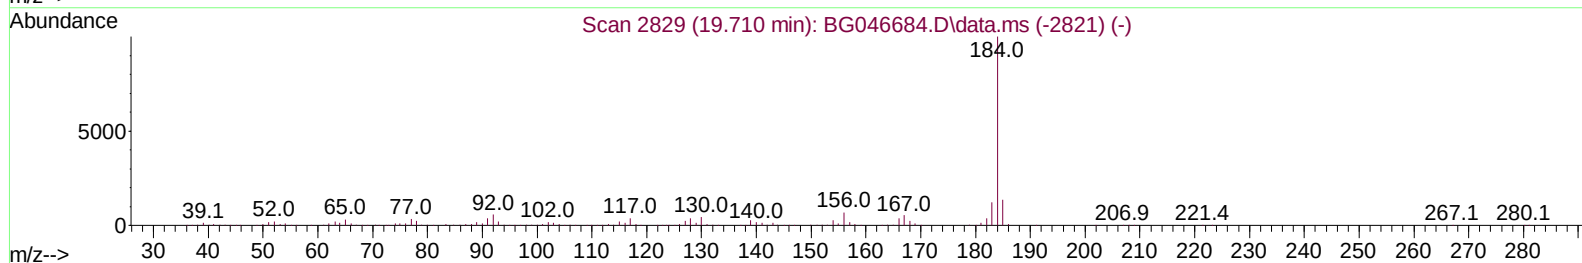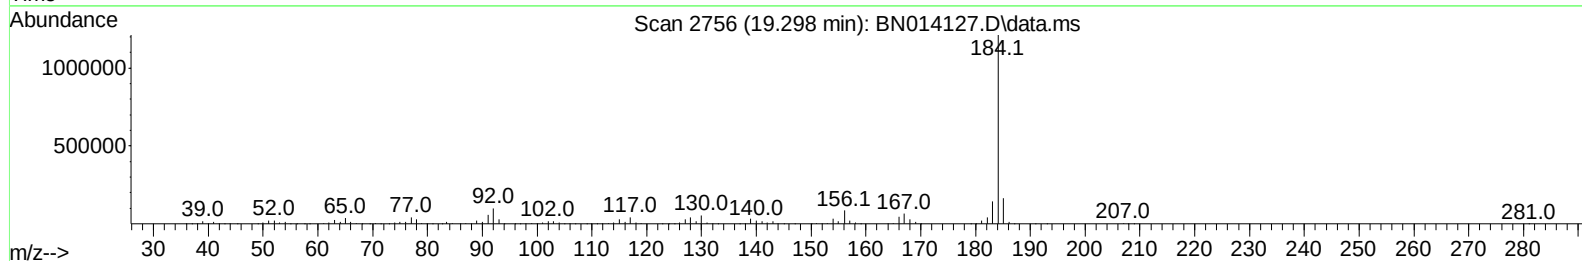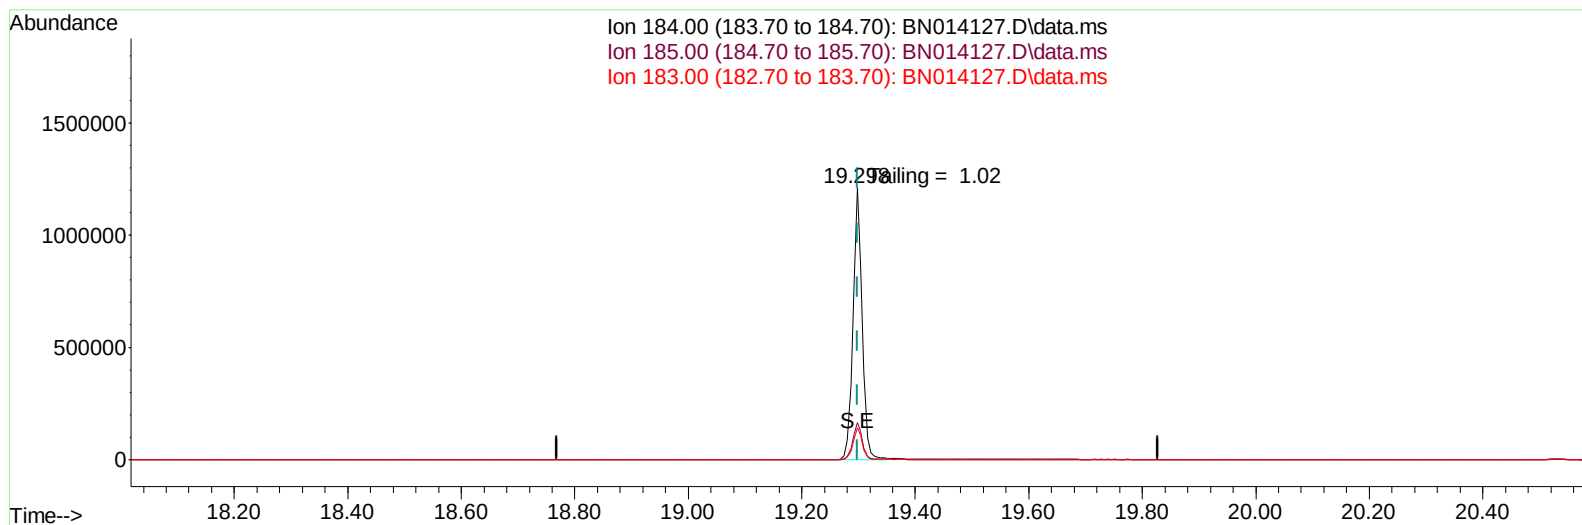

TIC: BN014127.D\data.ms

(77) Benzidine

19.298min (-0.000) 0.00 ng

response 1380507

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.51
183.00	13.20	11.79
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/29/2021	BNA_N	<u>BN014127.D</u>
Compound Name	Response	Retention Time
DDT	646966	20.533
DDD	1907	20.092
DDE	721	19.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2628	649594	0.40