
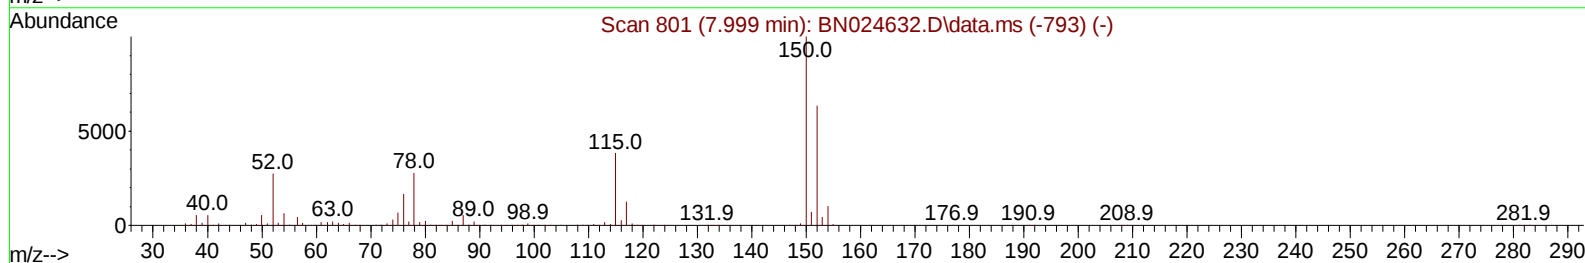
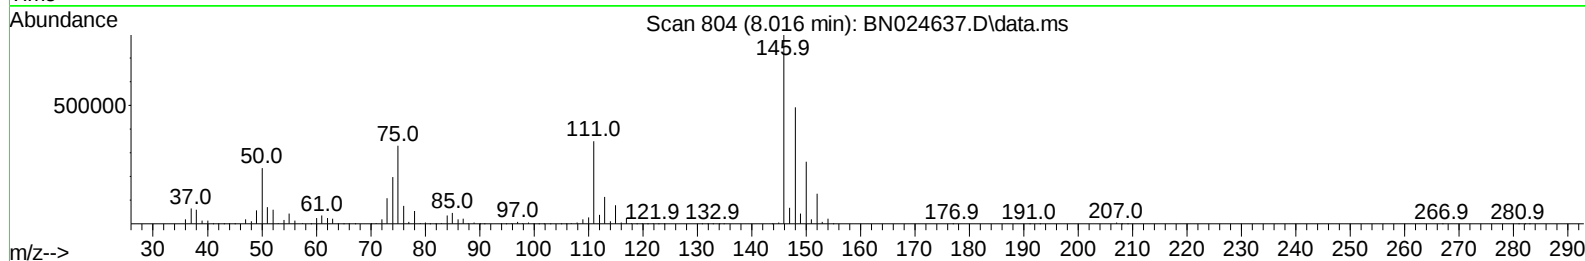


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024637.D
Acq On : 30 Mar 2023 11:40
Operator : CG/JU
Sample : 02085-05DL 2X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Mar 30 13:51:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 06:03:59 2023
Response via : Initial Calibration

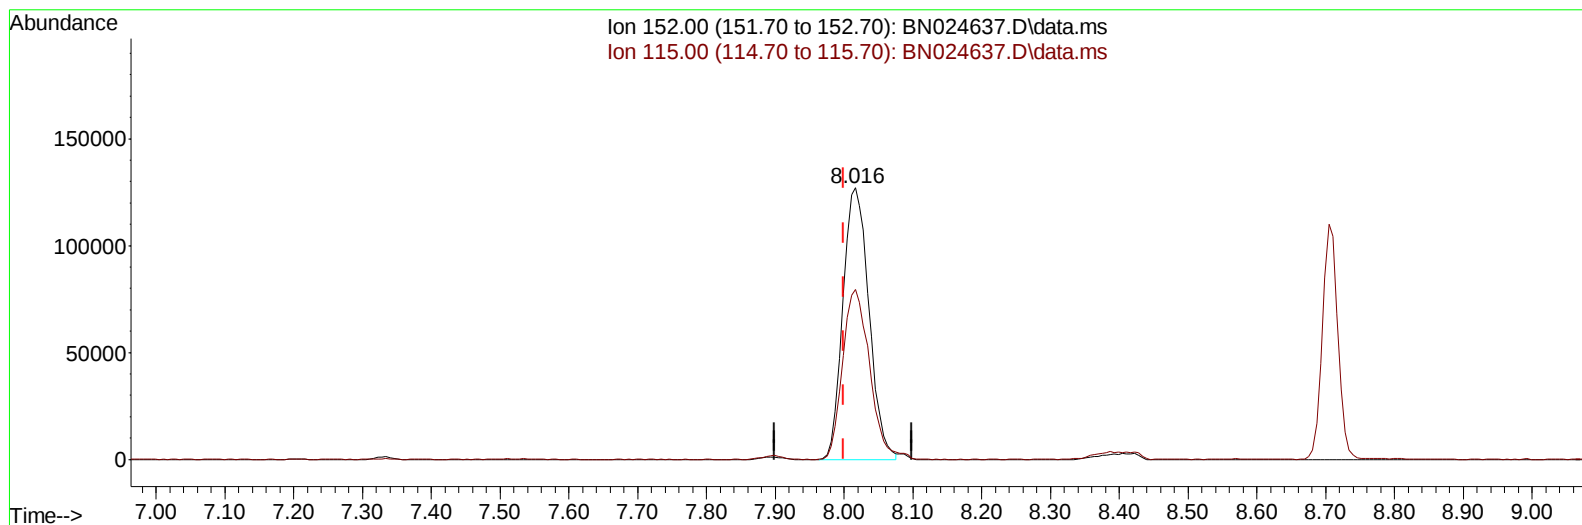

TIC: BN024637.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)




8.016min (+ 0.017) 20.00 ng/ul

response 335404

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	60.20	62.56
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024637.D
Acq On : 30 Mar 2023 11:40
Operator : CG/JU
Sample : 02085-05DL 2X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Mar 30 13:51:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 06:03:59 2023
Response via : Initial Calibration

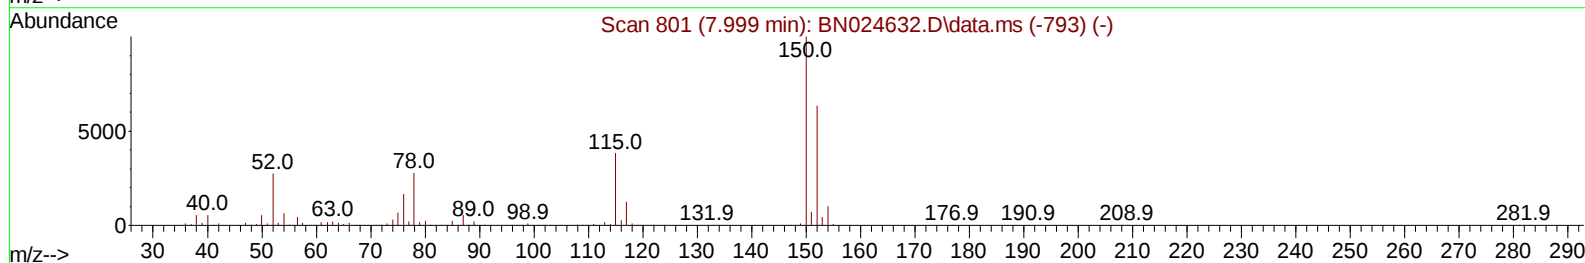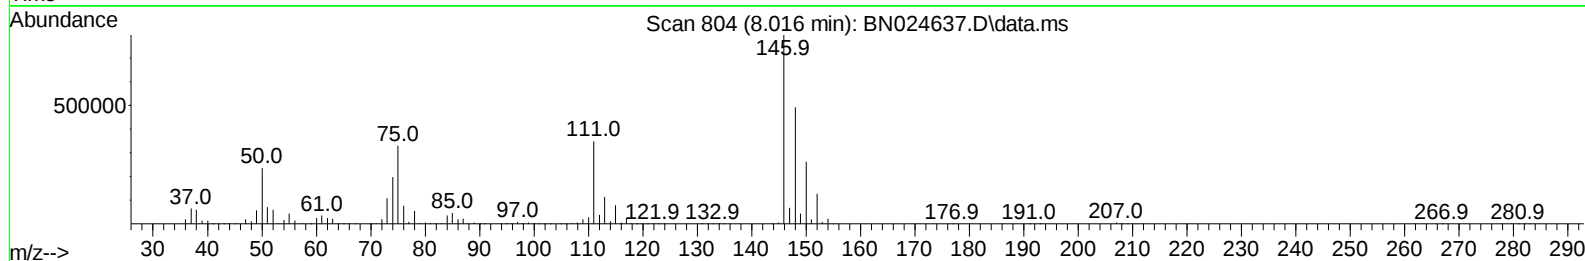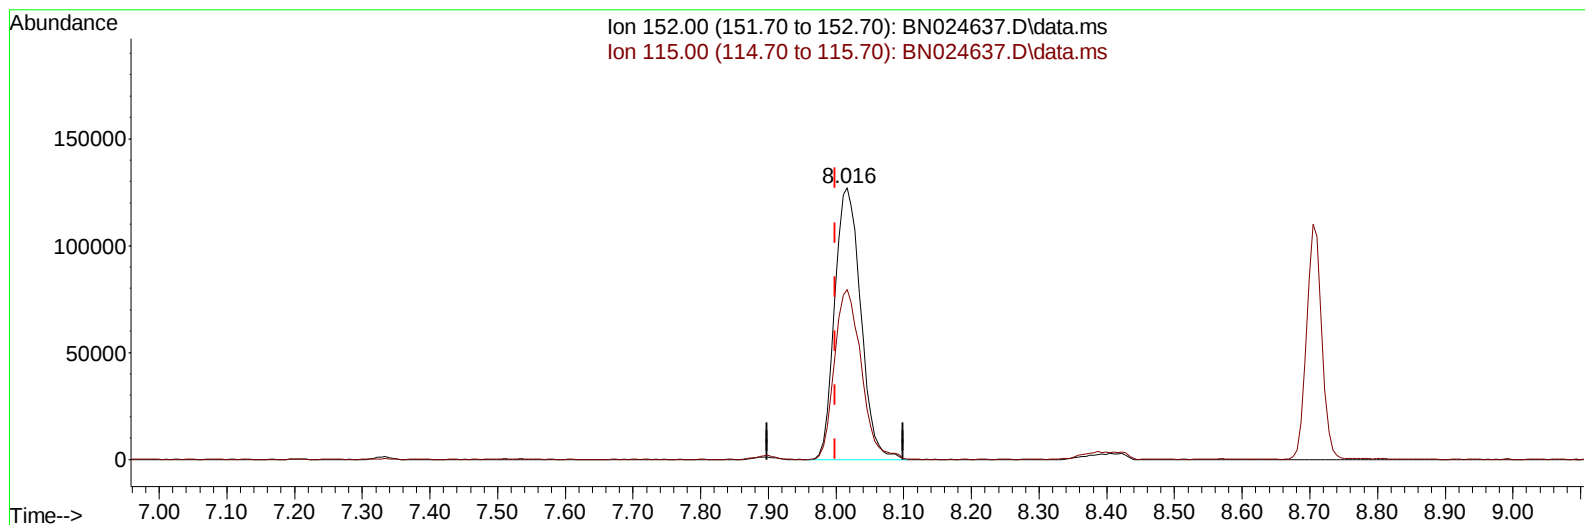

TIC: BN024637.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

8.016min (+ 0.017) 20.00 ng/ul m

response 337897

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	60.20	62.56
0.00	0.00	0.00
0.00	0.00	0.00