

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024586.D
 Acq On : 28 Mar 2023 15:45
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SICV210

Quant Time: Mar 29 03:33:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 29 03:32:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	297017	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	1356560	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	865358	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	1869119	20.000	ng/ul	0.00
79) Chrysene-d12	21.574	240	1757680	20.000	ng/ul	0.00
88) Perylene-d12	24.057	264	1993877	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	53952	7.043	ng/uL	0.00
4) Pyridine-d5	3.799	84	400901	18.123	ng/ul	0.00
7) Phenol-d5	7.157	99	492175	17.510	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	359561	19.809	ng/ul	0.00
11) 2-Chlorophenol-d4	7.528	132	379754	18.223	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	403399	17.945	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	196844	18.335	ng/ul	0.00
24) 2-Nitrophenol-d4	9.899	143	215602	18.553	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	388358	18.400	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	587484	18.242	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	1236058	18.575	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	1445808	19.080	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	246741	17.716	ng/ul	0.00
60) Fluorene-d10	15.634	176	1037423	18.169	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	210092	17.065	ng/ul	0.00
73) Anthracene-d10	17.486	188	1623907	18.472	ng/ul	0.00
81) Pyrene-d10	19.774	212	1855238	18.255	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.904	264	1838020	18.193	ng/ul	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	58606	7.100	ng/uL	98
5) Pyridine	3.822	79	400872	17.410	ng/ul	96
6) Benzaldehyde	7.134	77	349731	27.259	ng/ul	98
8) Phenol	7.187	94	533913	18.299	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.422	93	425864	18.509	ng/ul	99
12) 2-Chlorophenol	7.563	128	406079	18.678	ng/ul	98
13) 2-Methylphenol	8.446	108	402706	18.482	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.540	45	755466	18.484	ng/ul	99
16) Acetophenone	8.834	105	678875	19.346	ng/ul	98
17) N-Nitroso-di-n-propyla...	8.816	70	358348	19.404	ng/ul	99
18) 4-Methylphenol	8.775	108	444412	18.371	ng/ul	97
19) Hexachloroethane	9.087	117	154778	18.025	ng/ul	98
22) Nitrobenzene	9.216	77	514436	18.448	ng/ul	99
23) Isophorone	9.740	82	968182	18.679	ng/ul	99
25) 2-Nitrophenol	9.928	139	238337	18.865	ng/ul	99
26) 2,4-Dimethylphenol	9.987	107	487526	18.578	ng/ul	98
27) Bis(2-Chloroethoxy)met...	10.222	93	604893	18.185	ng/ul	99
29) 2,4-Dichlorophenol	10.463	162	399744	18.672	ng/ul	97
30) Naphthalene	10.869	128	1373713	18.224	ng/ul	99
32) 4-Chloroaniline	10.981	127	615176	18.863	ng/ul	99
33) Hexachlorobutadiene	11.151	225	226765	18.393	ng/ul	97
34) Caprolactam	11.757	113	144052	19.456	ng/ul	93
35) 4-Chloro-3-methylphenol	12.092	107	461373	18.850	ng/ul	97
36) 2-Methylnaphthalene	12.475	142	968677	19.195	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024586.D
 Acq On : 28 Mar 2023 15:45
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SICV210

Quant Time: Mar 29 03:33:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 29 03:32:05 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.692	142	919859	18.397	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.840	216	483079	18.832	ng/ul	99
40) Hexachlorocyclopentadiene	12.816	237	284811	17.644	ng/ul	97
41) 2,4,6-Trichlorophenol	13.081	196	318675	18.647	ng/ul	99
42) 2,4,5-Trichlorophenol	13.145	196	353074	18.797	ng/ul	97
43) 1,1'-Biphenyl	13.475	154	1296771	18.861	ng/ul	97
44) 2-Chloronaphthalene	13.522	162	987481	18.398	ng/ul	99
45) 2-Nitroaniline	13.722	65	325743	19.533	ng/ul	92
47) Dimethylphthalate	14.098	163	1242031	18.380	ng/ul	100
48) 2,6-Dinitrotoluene	14.216	165	265432	20.736	ng/ul	97
50) Acenaphthylene	14.363	152	1586675	19.125	ng/ul	99
51) 3-Nitroaniline	14.545	138	304286	22.364	ng/ul	98
52) Acenaphthene	14.704	153	1068528	18.483	ng/ul	97
53) 2,4-Dinitrophenol	14.751	184	146872	16.892	ng/ul	98
55) 4-Nitrophenol	14.845	109	201469	18.906	ng/ul	95
56) Dibenzofuran	15.039	168	1537238	19.109	ng/ul	100
57) 2,4-Dinitrotoluene	15.004	165	361300	19.267	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.263	232	317332	20.273	ng/ul	98
59) Diethylphthalate	15.457	149	1243225	18.800	ng/ul	99
61) Fluorene	15.686	166	1221742	18.941	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.681	204	574972	18.787	ng/ul	96
63) 4-Nitroaniline	15.710	138	315137	23.511	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.763	198	221794	18.218	ng/ul	99
67) N-Nitrosodiphenylamine	15.892	169	1081665	19.352	ng/ul	97
68) 4-Bromophenyl-phenylether	16.575	248	353366	18.942	ng/ul	96
69) Hexachlorobenzene	16.692	284	397613	18.110	ng/ul	98
70) Atrazine	16.839	200	359823	18.843	ng/ul	99
71) Pentachlorophenol	17.033	266	245571	18.297	ng/ul	93
72) Phenanthrene	17.428	178	1949604	18.614	ng/ul	99
74) Anthracene	17.522	178	1985085	18.866	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.445	216	476039	17.814	ng/ul	98
76) Pentachlorobenzene	14.957	250	460410	17.737	ng/ul	96
77) Carbazole	17.792	167	1838669	19.435	ng/ul	100
78) Di-n-butylphthalate	18.351	149	2019308	18.836	ng/ul	99
80) Fluoranthene	19.439	202	2178468	18.075	ng/ul	99
82) Pyrene	19.804	202	2395490	18.854	ng/ul	98
83) Butylbenzylphthalate	20.698	149	887850	18.353	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.492	252	889190	21.642	ng/ul	95
85) Benzo(a)anthracene	21.563	228	2287682	18.425	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.480	149	1274558	18.896	ng/ul	98
87) Chrysene	21.616	228	2164942	18.427	ng/ul	98
89) Di-n-octyl phthalate	22.439	149	2191255	18.142	ng/ul	100
90) Benzo(b)fluoranthene	23.304	252	2385315	18.270	ng/ul	97
91) Benzo(k)fluoranthene	23.351	252	2291300	18.383	ng/ul	99
93) Benzo(a)pyrene	23.957	252	2087825	18.261	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	26.668	276	2623025	18.004	ng/ul	98
95) Dibenzo(a,h)anthracene	26.686	278	2161732	17.891	ng/ul	99
96) Benzo(g,h,i)perylene	27.474	276	2091181	17.275	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024586.D
Acq On : 28 Mar 2023 15:45
Operator : CG/JU
Sample : SSTDICV020
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SICV210

Quant Time: Mar 29 03:33:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 29 03:32:05 2023
Response via : Initial Calibration




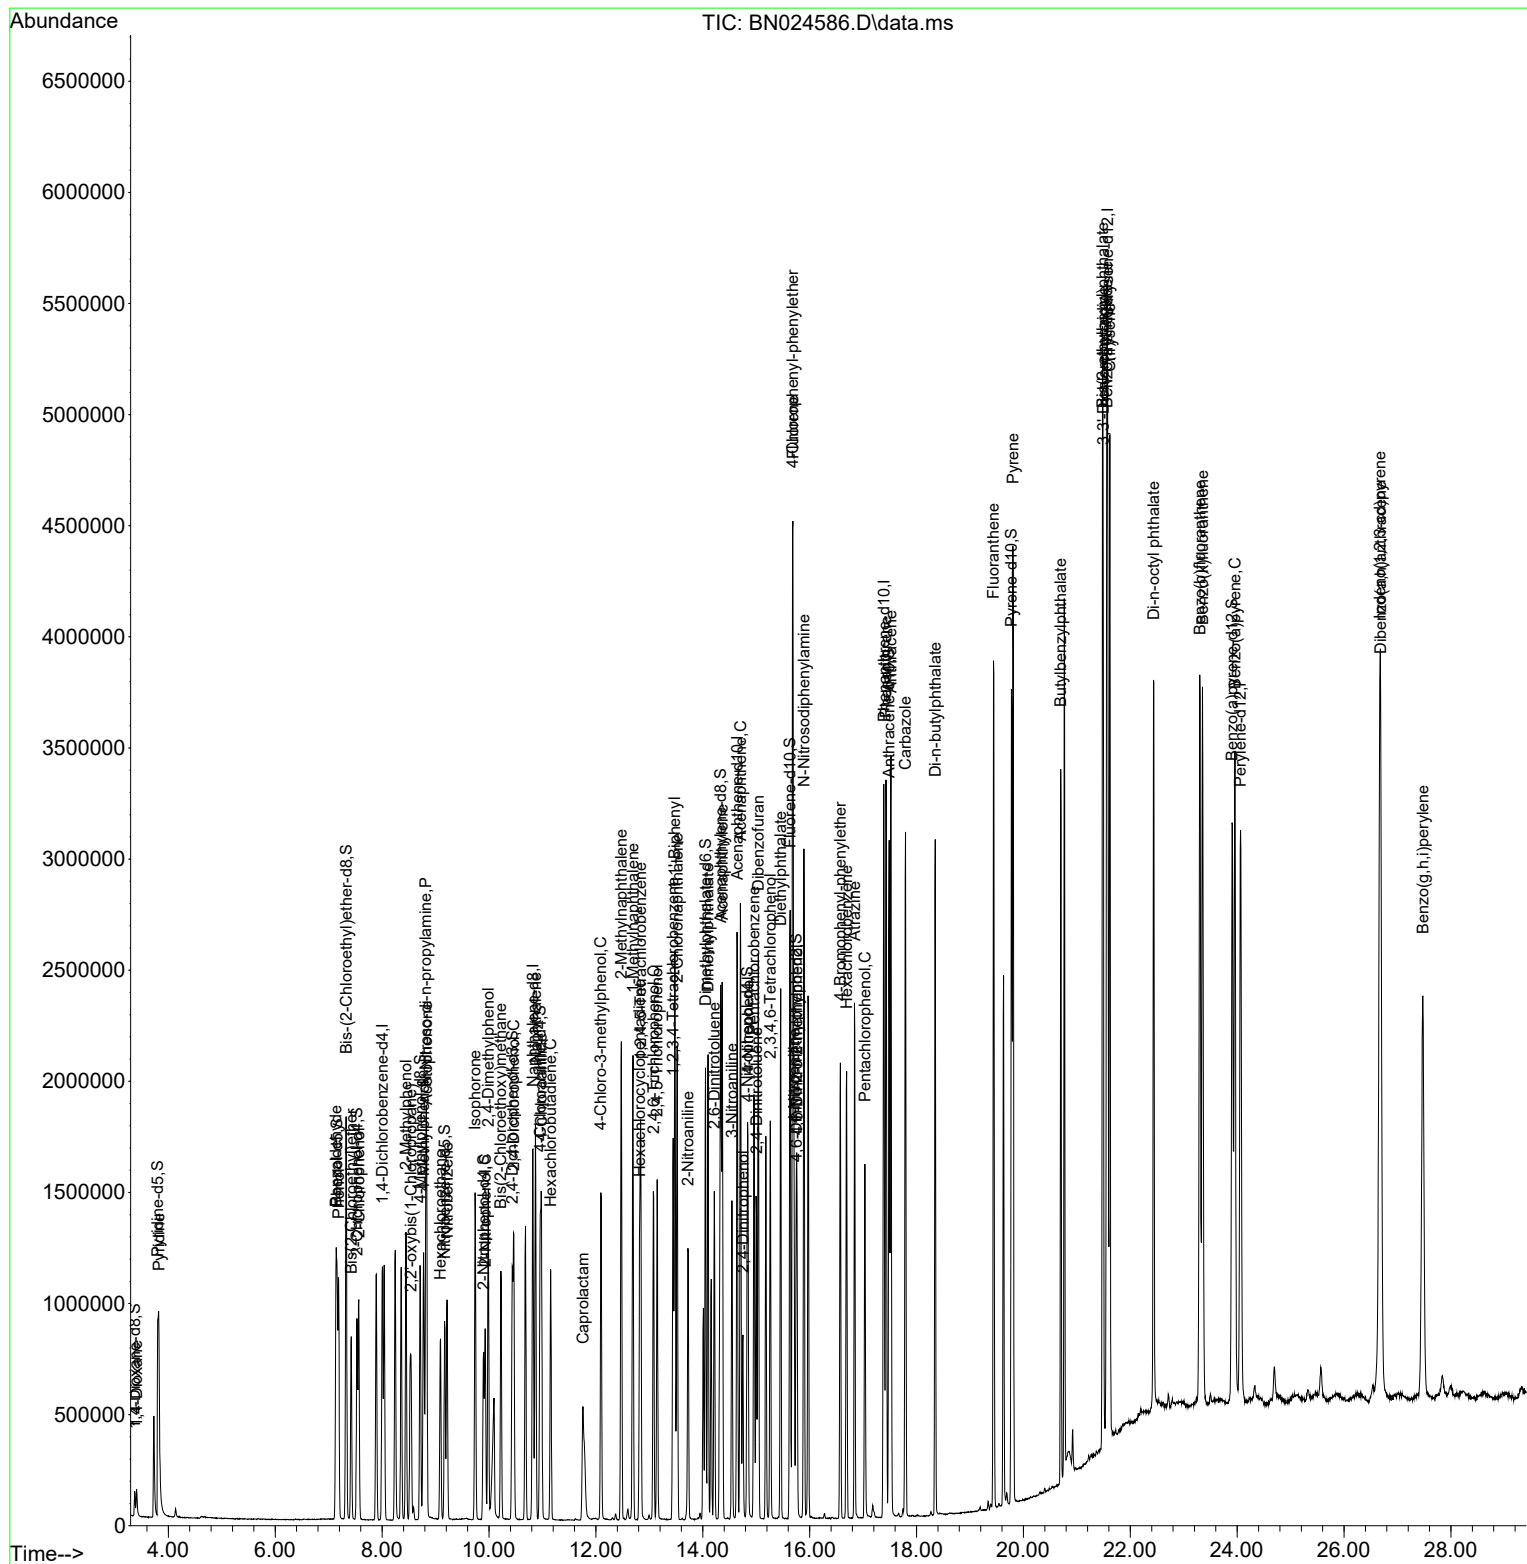




#2
 1,4-Dioxane
 Concen: 7.100 ng/uL
 RT: 3.405 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BN024586.D
 Acq: 28 Mar 2023 15:45




Instrument :
 BNA_N
 ClientSampleId :
 SICV210


Tgt Ion: 88 Resp: 58606
 Ion Ratio Lower Upper
 88 100
 43 37.0 29.0 43.6
 58 82.5 67.5 101.3

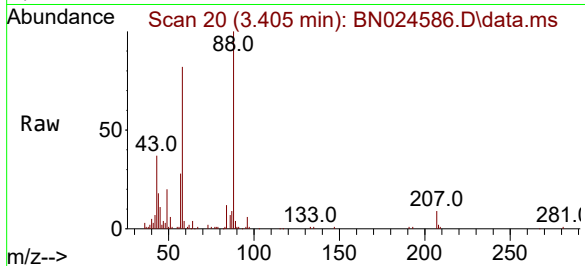

#5
 Pyridine
 Concen: 17.410 ng/uL
 RT: 3.822 min Scan# 91
 Delta R.T. 0.006 min
 Lab File: BN024586.D
 Acq: 28 Mar 2023 15:45

Tgt Ion: 79 Resp: 400872
 Ion Ratio Lower Upper
 79 100
 52 90.7 76.0 114.0
 51 44.6 35.0 52.4




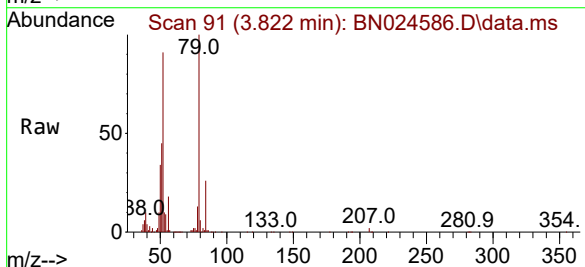




#6
Benzaldehyde
Concen: 27.259 ng/ul
RT: 7.134 min Scan# 610
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion: 77 Resp: 349731
Ion Ratio Lower Upper
77 100
105 93.1 74.0 111.0
106 92.8 71.7 107.5

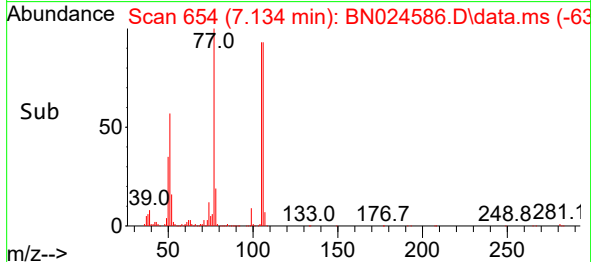

#8
Phenol
Concen: 18.299 ng/ul
RT: 7.187 min Scan# 663
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion: 94 Resp: 533913
Ion Ratio Lower Upper
94 100
65 30.0 23.7 35.5
66 38.8 29.9 44.9




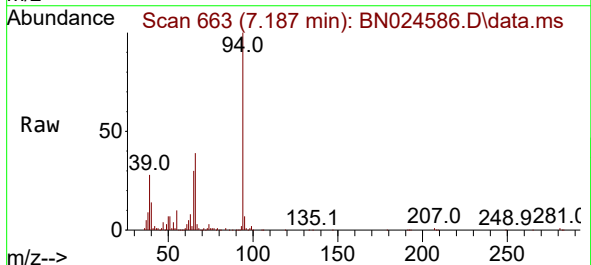




#10
Bis(2-Chloroethyl)ether
Concen: 18.509 ng/ul
RT: 7.422 min Scan# 703
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion: 93 Resp: 425864
Ion Ratio Lower Upper
93 100
63 82.3 64.9 97.3
95 31.4 25.2 37.8

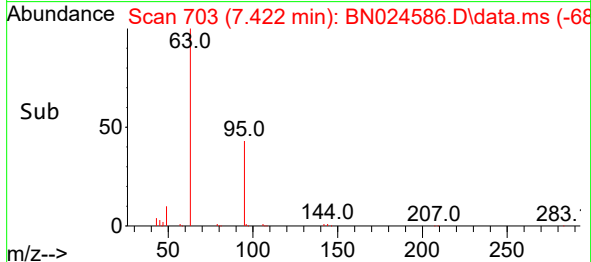

#12
2-Chlorophenol
Concen: 18.678 ng/ul
RT: 7.563 min Scan# 727
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:128 Resp: 406079
Ion Ratio Lower Upper
128 100
64 50.2 41.6 62.4
130 32.0 25.6 38.4

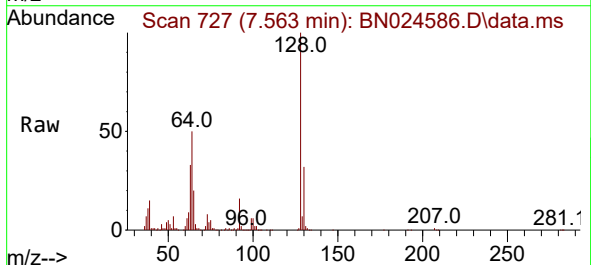



#13

2-Methylphenol

Concen: 18.482 ng/ul

RT: 8.446 min Scan# 81

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :





SICV210

Tgt Ion:108 Resp: 402706

Ion Ratio Lower Upper

108 100

107 88.0 70.9 106.3

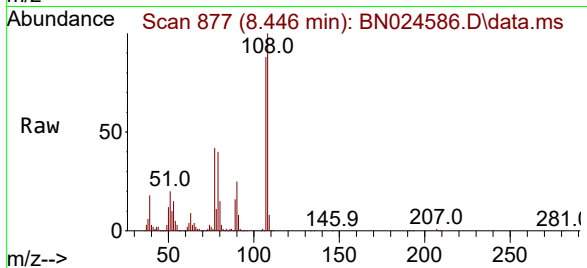

#14

2,2'-oxybis(1-Chloropropane)

Concen: 18.484 ng/ul

RT: 8.540 min Scan# 893

Delta R.T. 0.006 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion: 45 Resp: 755466


Ion Ratio Lower Upper

45 100

77 11.5 9.0 13.4

79 8.9 6.9 10.3




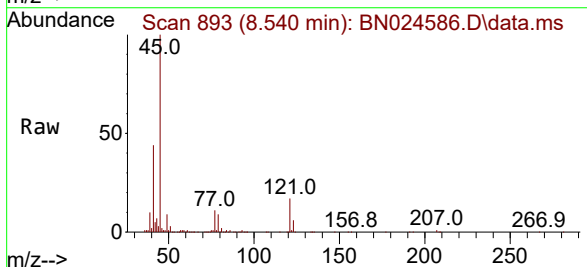




#16
Acetophenone
Concen: 19.346 ng/ul
RT: 8.834 min Scan# 943
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:105 Resp: 678875
Ion Ratio Lower Upper
105 100
77 78.7 64.3 96.5
51 32.5 27.3 40.9



#17
N-Nitroso-di-n-propylamine
Concen: 19.404 ng/ul
RT: 8.816 min Scan# 940
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion: 70 Resp: 358348
Ion Ratio Lower Upper
70 100
42 72.5 57.5 86.3
101 9.9 7.8 11.8
130 20.7 15.7 23.5









#18
4-Methylphenol
Concen: 18.371 ng/ul
RT: 8.775 min Scan# 911
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:108 Resp: 444412
Ion Ratio Lower Upper
108 100
107 112.4 87.7 131.5

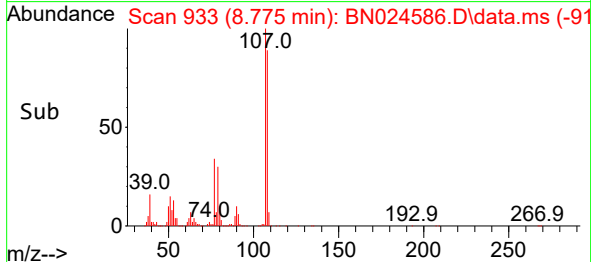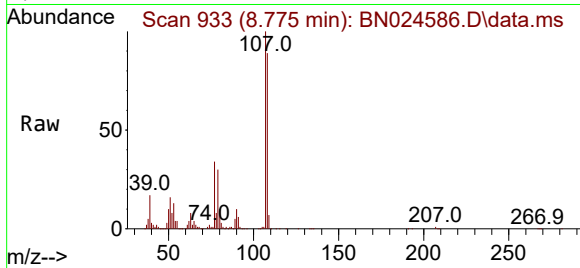

#19
Hexachloroethane
Concen: 18.025 ng/ul
RT: 9.087 min Scan# 986
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:117 Resp: 154778
Ion Ratio Lower Upper
117 100
201 92.3 71.9 107.9
199 57.0 45.2 67.8




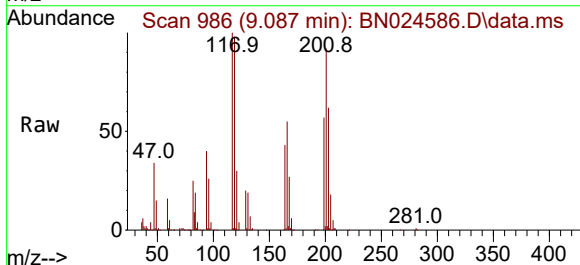




#22
Nitrobenzene
Concen: 18.448 ng/ul
RT: 9.216 min Scan# 1008
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion: 77 Resp: 514436
Ion Ratio Lower Upper
77 100
123 43.5 34.3 51.5
65 14.3 10.8 16.2

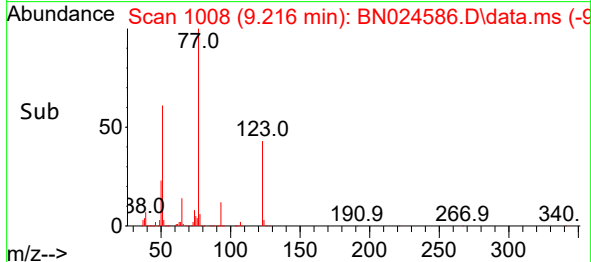

#23
Isophorone
Concen: 18.679 ng/ul
RT: 9.740 min Scan# 1097
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion: 82 Resp: 968182
Ion Ratio Lower Upper
82 100
95 6.6 5.4 8.0
138 16.4 12.6 18.8









#25
2-Nitrophenol
Concen: 18.865 ng/ul
RT: 9.928 min Scan# 1129
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:139 Resp: 238337
Ion Ratio Lower Upper
139 100
65 57.7 46.3 69.5
109 29.7 24.6 37.0

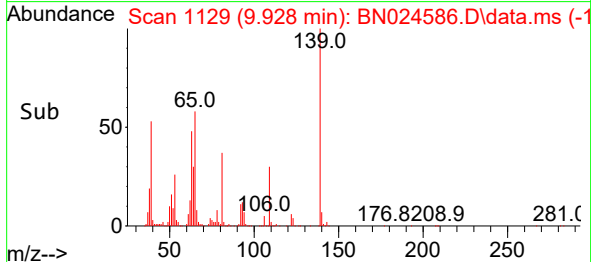

#26
2,4-Dimethylphenol
Concen: 18.578 ng/ul
RT: 9.987 min Scan# 1139
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:107 Resp: 487526
Ion Ratio Lower Upper
107 100
121 50.4 40.7 61.1
122 85.9 71.2 106.8

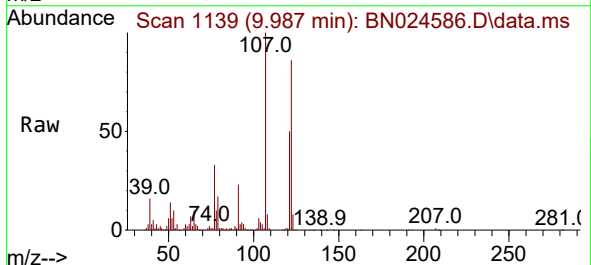



#27

Bis(2-Chloroethoxy)methane

Concen: 18.185 ng/ul

RT: 10.222 min Scan# 1179

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion: 93 Resp: 604893

Ion Ratio Lower Upper

93 100

95 32.1 26.4 39.6

123 10.6 8.9 13.3

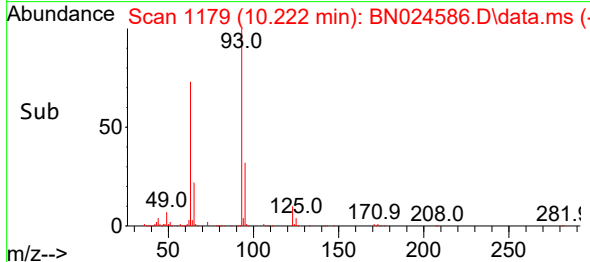

#29

2,4-Dichlorophenol

Concen: 18.672 ng/ul

RT: 10.463 min Scan# 1220

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:162 Resp: 399744


Ion Ratio Lower Upper

162 100

164 64.6 50.5 75.7

98 38.8 28.6 42.8

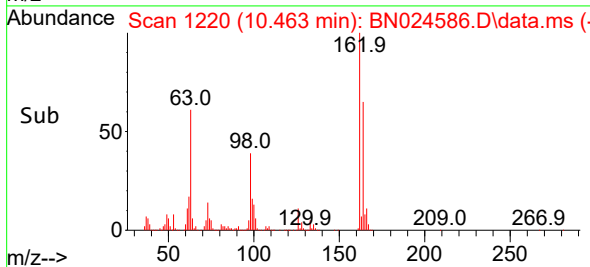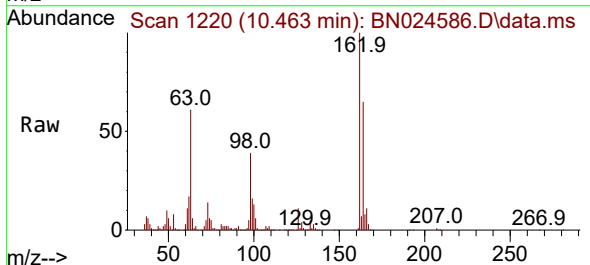



#30

Naphthalene

Concen: 18.224 ng/ul

RT: 10.869 min Scan# 1289

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:128 Resp: 1373713

Ion Ratio Lower Upper

128 100

129 11.0 8.5 12.7

127 12.8 10.4 15.6

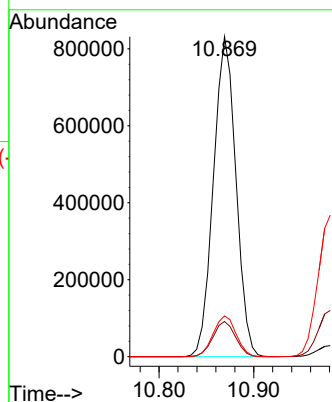

#32

4-Chloroaniline

Concen: 18.863 ng/ul

RT: 10.981 min Scan# 1308

Delta R.T. -0.000 min

Lab File: BN024586.D




Acq: 28 Mar 2023 15:45


Tgt Ion:127 Resp: 615176

Ion Ratio Lower Upper

127 100

129 32.7 25.5 38.3

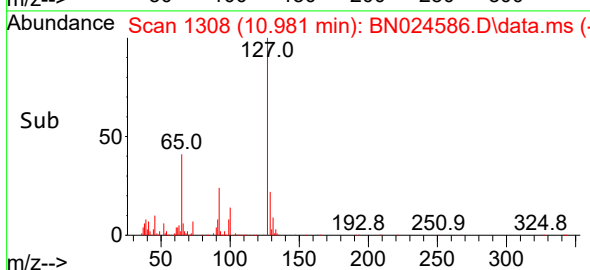



#33

Hexachlorobutadiene

Concen: 18.393 ng/ul

RT: 11.151 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:225 Resp: 226765

Ion Ratio Lower Upper

225 100

223 64.9 50.2 75.4

227 64.0 49.6 74.4

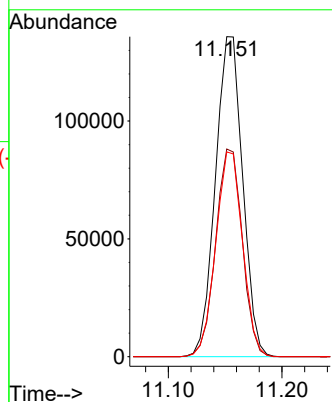

#34

Caprolactam

Concen: 19.456 ng/ul

RT: 11.757 min Scan# 1440

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:113 Resp: 144052


Ion Ratio Lower Upper

113 100

55 191.2 162.2 243.2

56 143.6 121.6 182.4









#35
4-Chloro-3-methylphenol
Concen: 18.850 ng/ul
RT: 12.092 min Scan# 1498
Delta R.T. -0.006 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:107 Resp: 461373
Ion Ratio Lower Upper
107 100
144 24.0 21.1 31.7
142 78.7 61.0 91.4

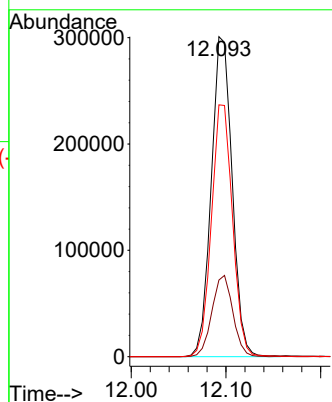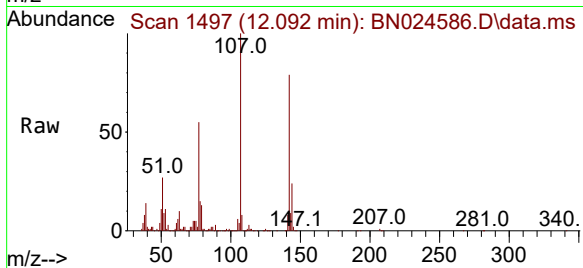

#36
2-Methylnaphthalene
Concen: 19.195 ng/ul
RT: 12.475 min Scan# 1562
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:142 Resp: 968677
Ion Ratio Lower Upper
142 100
141 89.7 70.2 105.4


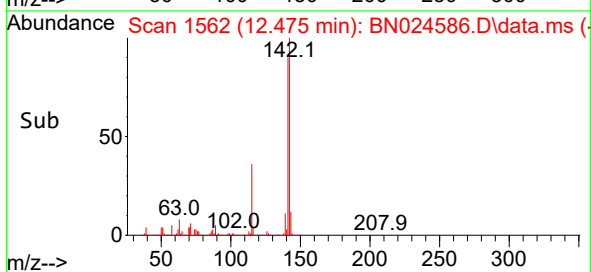
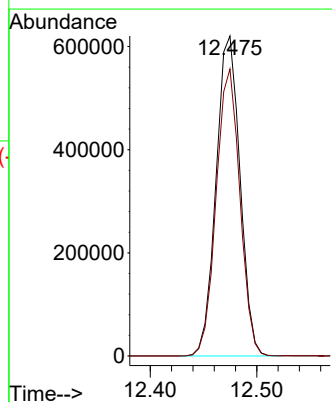
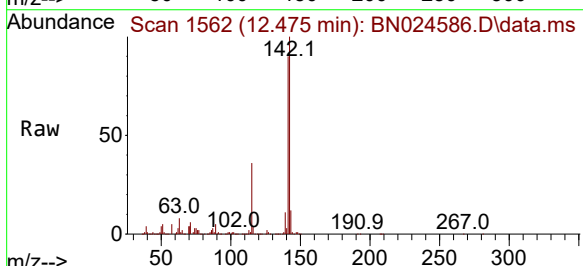




#37
1-Methylnaphthalene
Concen: 18.397 ng/ul
RT: 12.692 min Scan# 1599
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:142 Resp: 919859
Ion Ratio Lower Upper
142 100
141 92.3 74.2 111.4
116 3.7 3.0 4.6

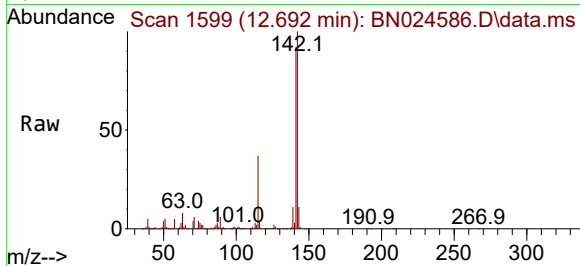

#39
1,2,4,5-Tetrachlorobenzene
Concen: 18.832 ng/ul
RT: 12.840 min Scan# 1624
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:216 Resp: 483079
Ion Ratio Lower Upper
216 100
214 75.9 61.0 91.4
179 21.5 15.7 23.5
108 19.0 14.0 21.0




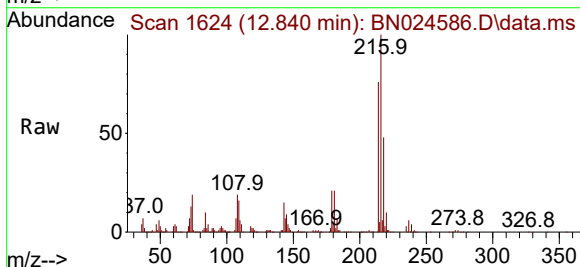




#40
Hexachlorocyclopentadiene
Concen: 17.644 ng/ul
RT: 12.816 min Scan# 1620
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:237 Resp: 284811
Ion Ratio Lower Upper
237 100
235 64.6 50.0 75.0
272 13.0 9.5 14.3



#41
2,4,6-Trichlorophenol
Concen: 18.647 ng/ul
RT: 13.081 min Scan# 1665
Delta R.T. 0.006 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:196 Resp: 318675
Ion Ratio Lower Upper
196 100
198 93.2 75.5 113.3
200 31.8 24.6 37.0





#42

2,4,5-Trichlorophenol

Concen: 18.797 ng/ul

RT: 13.145 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:196 Resp: 353074

Ion Ratio Lower Upper

196 100

198 91.2 75.4 113.0

200 29.2 24.6 37.0

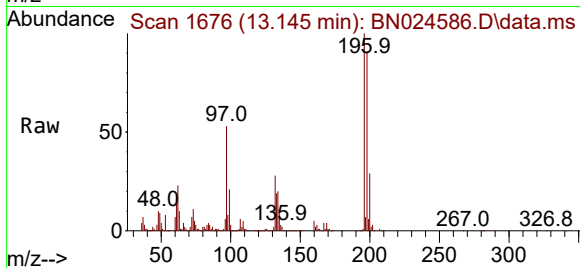

#43

1,1'-Biphenyl

Concen: 18.861 ng/ul

RT: 13.475 min Scan# 1732

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:154 Resp: 1296771


Ion Ratio Lower Upper

154 100

153 37.5 32.2 48.4

76 14.4 11.7 17.5

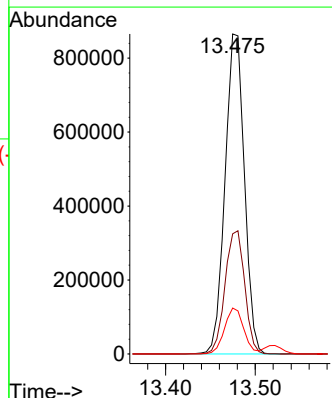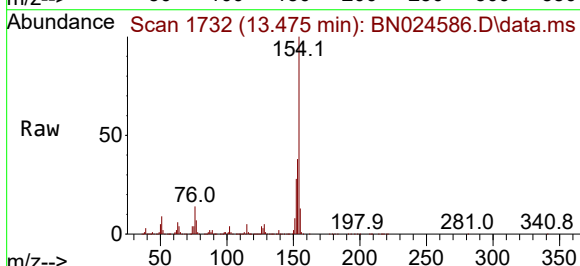



#44

2-Chloronaphthalene

Concen: 18.398 ng/ul

RT: 13.522 min Scan# 1740

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:162 Resp: 987481

Ion Ratio Lower Upper

162 100

164 32.4 26.1 39.1

127 39.6 31.1 46.7



#45

2-Nitroaniline

Concen: 19.533 ng/ul

RT: 13.722 min Scan# 1774

Delta R.T. -0.006 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion: 65 Resp: 325743


Ion Ratio Lower Upper

65 100

92 63.2 52.6 78.8

138 91.0 81.4 122.2





#47

Dimethylphthalate

Concen: 18.380 ng/ul

RT: 14.098 min Scan# 1838

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:163 Resp: 1242031

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.4 8.2 12.2

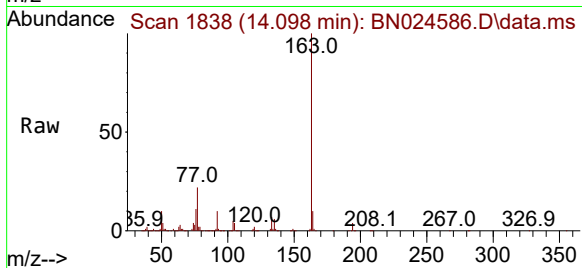

#48

2,6-Dinitrotoluene

Concen: 20.736 ng/ul

RT: 14.216 min Scan# 1858

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:165 Resp: 265432


Ion Ratio Lower Upper

165 100

89 62.4 47.8 71.6

121 23.2 17.3 25.9

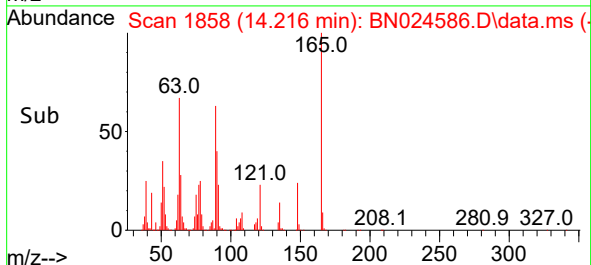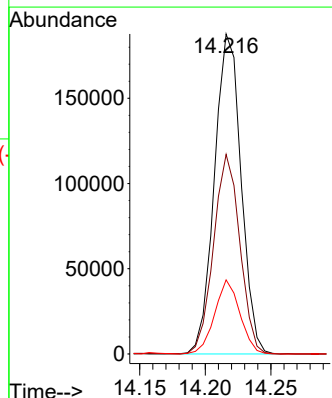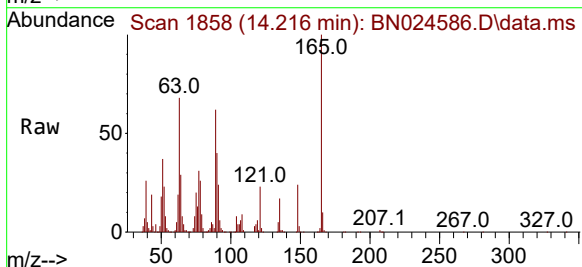



#50

Acenaphthylene

Concen: 19.125 ng/ul

RT: 14.363 min Scan# 1883

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:152 Resp: 1586675

Ion Ratio Lower Upper

152 100

151 19.9 15.5 23.3

153 13.2 10.3 15.5

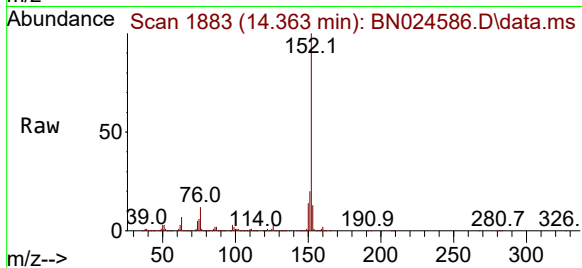

#51

3-Nitroaniline

Concen: 22.364 ng/ul

RT: 14.545 min Scan# 1914

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:138 Resp: 304286


Ion Ratio Lower Upper

138 100

108 10.6 8.8 13.2

92 117.8 96.1 144.1

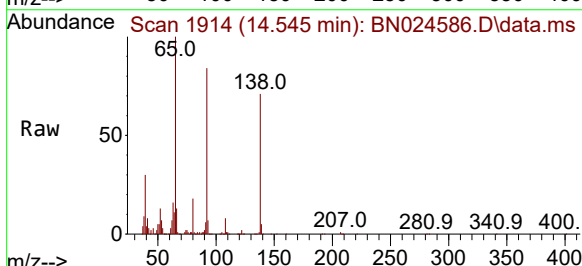



#52

Acenaphthene

Concen: 18.483 ng/ul

RT: 14.704 min Scan# 1941

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:153 Resp: 1068528

Ion Ratio Lower Upper

153 100

152 47.8 36.6 55.0

154 87.2 67.7 101.5



#53

2,4-Dinitrophenol

Concen: 16.892 ng/ul

RT: 14.751 min Scan# 1949

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:184 Resp: 146872


Ion Ratio Lower Upper

184 100

63 72.8 59.1 88.7

154 58.8 49.2 73.8









#55
4-Nitrophenol
Concen: 18.906 ng/ul
RT: 14.845 min Scan# 1965
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:109 Resp: 201469
Ion Ratio Lower Upper
109 100
139 140.3 108.4 162.6
65 143.6 121.1 181.7

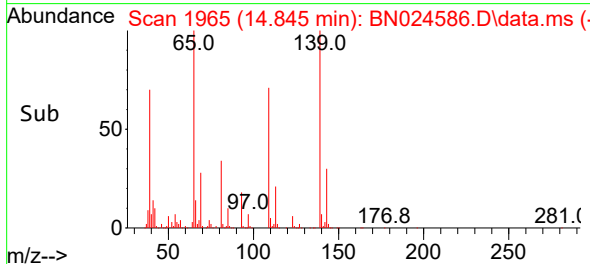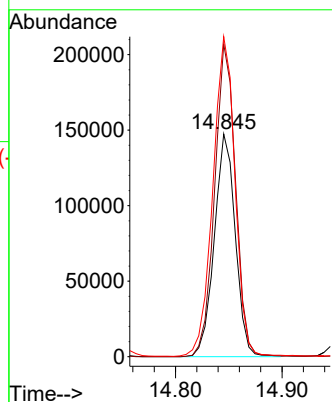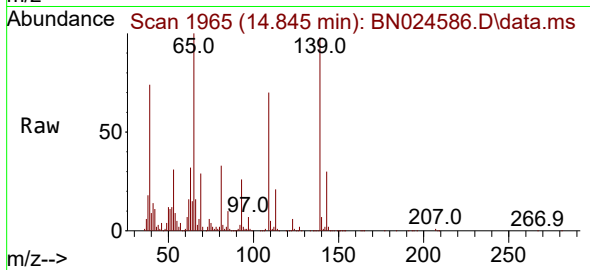

#56
Dibenzofuran
Concen: 19.109 ng/ul
RT: 15.039 min Scan# 1998
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:168 Resp: 1537238
Ion Ratio Lower Upper
168 100
139 37.2 30.0 45.0

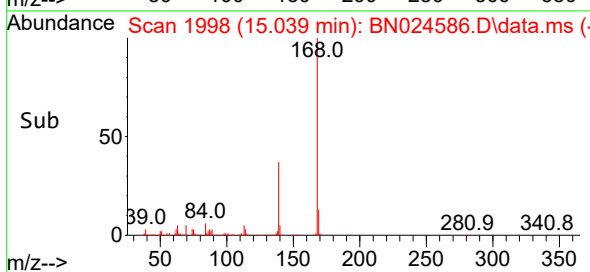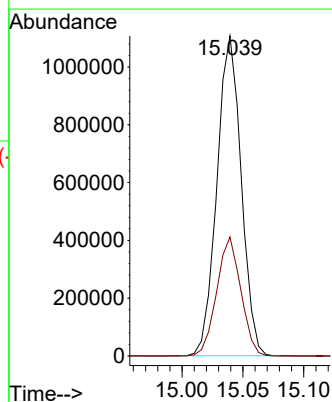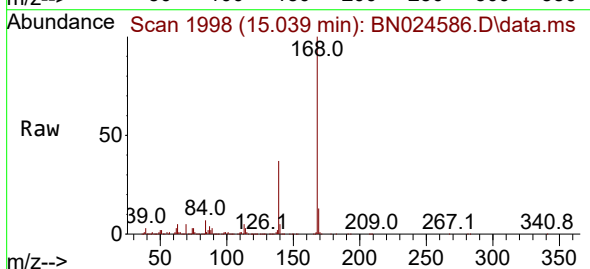



#57

2,4-Dinitrotoluene

Concen: 19.267 ng/ul

RT: 15.004 min Scan# 1992

Delta R.T. 0.006 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:165 Resp: 361300

Ion Ratio Lower Upper

165 100

63 47.1 42.2 63.4

182 2.9 2.3 3.5

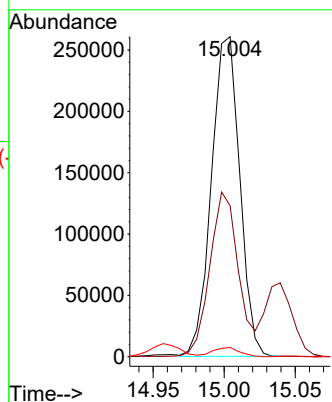

#58

2,3,4,6-Tetrachlorophenol

Concen: 20.273 ng/ul

RT: 15.263 min Scan# 2036

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Tgt Ion:232 Resp: 317332




Ion Ratio Lower Upper


232 100

131 46.6 36.5 54.7

130 2.3 1.8 2.8

166 32.3 24.4 36.6





#59

Diethylphthalate

Concen: 18.800 ng/ul

RT: 15.457 min Scan# 2069

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:149 Resp: 1243225

Ion Ratio Lower Upper

149 100

177 21.5 17.5 26.3

150 12.0 9.8 14.6

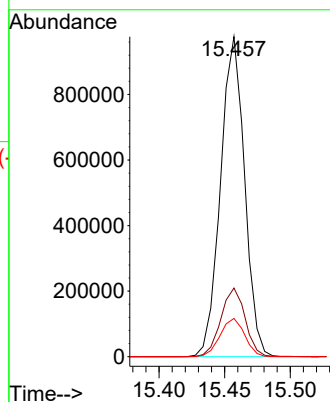

#61

Fluorene

Concen: 18.941 ng/ul

RT: 15.686 min Scan# 2108

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:166 Resp: 1221742


Ion Ratio Lower Upper

166 100

165 94.1 78.6 118.0

167 13.3 11.0 16.4









#62
4-Chlorophenyl-phenylether
Concen: 18.787 ng/ul
RT: 15.681 min Scan# 2107
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:204 Resp: 574972
Ion Ratio Lower Upper
204 100
206 33.1 25.9 38.9
141 58.5 49.9 74.9

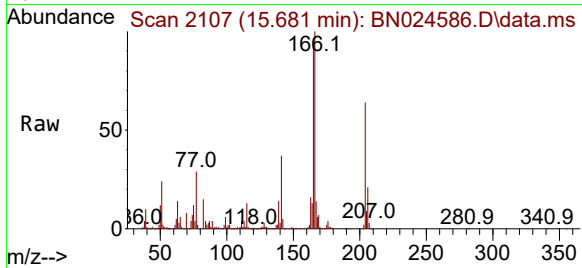

#63
4-Nitroaniline
Concen: 23.511 ng/ul
RT: 15.710 min Scan# 2112
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:138 Resp: 315137
Ion Ratio Lower Upper
138 100
92 52.4 41.5 62.3
108 78.4 63.0 94.4



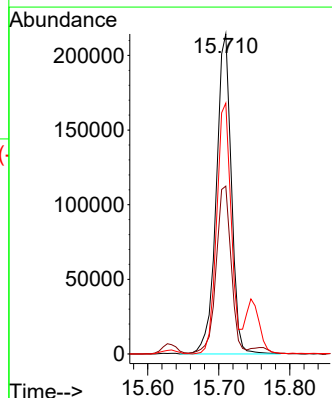
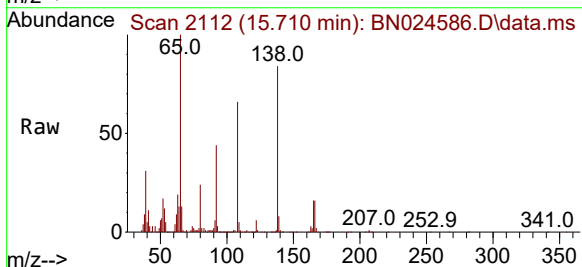




#66
 4,6-Dinitro-2-methylphenol
 Concen: 18.218 ng/ul
 RT: 15.763 min Scan# 2121
 Delta R.T. -0.000 min
 Lab File: BN024586.D
 Acq: 28 Mar 2023 15:45




Instrument :
 BNA_N
 ClientSampleId :
 SICV210


Tgt Ion:198 Resp: 221794
 Ion Ratio Lower Upper
 198 100
 182 4.7 3.9 5.9
 77 27.4 22.2 33.2

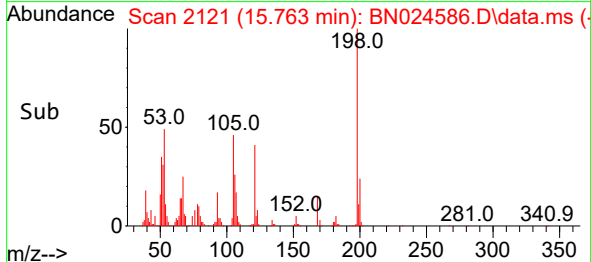

#67
 N-Nitrosodiphenylamine
 Concen: 19.352 ng/ul
 RT: 15.892 min Scan# 2143
 Delta R.T. -0.000 min
 Lab File: BN024586.D
 Acq: 28 Mar 2023 15:45

Tgt Ion:169 Resp: 1081665
 Ion Ratio Lower Upper
 169 100
 168 65.7 54.3 81.5
 167 34.9 29.4 44.0




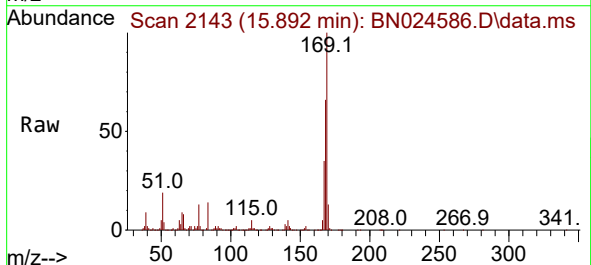




#68
4-Bromophenyl-phenylether
Concen: 18.942 ng/ul
RT: 16.575 min Scan# 2259
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:248 Resp: 353366
Ion Ratio Lower Upper
248 100
250 97.3 74.5 111.7
141 78.2 60.7 91.1



#69
Hexachlorobenzene
Concen: 18.110 ng/ul
RT: 16.692 min Scan# 2279
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:284 Resp: 397613
Ion Ratio Lower Upper
284 100
142 37.8 28.5 42.7
249 32.4 25.5 38.3

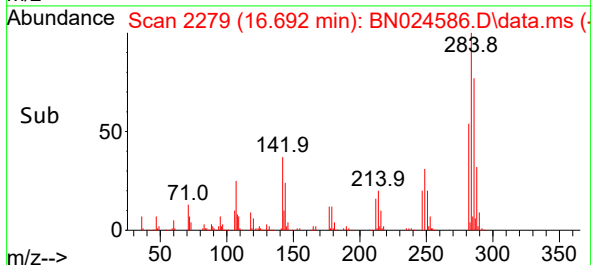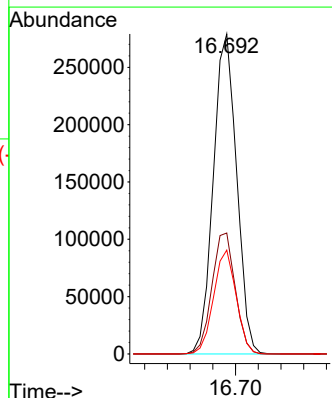



#70

Atrazine

Concen: 18.843 ng/ul

RT: 16.839 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:200 Resp: 359823

Ion Ratio Lower Upper

200 100

173 28.3 21.8 32.6

215 48.4 38.2 57.2



#71

Pentachlorophenol

Concen: 18.297 ng/ul

RT: 17.033 min Scan# 2337

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:266 Resp: 245571


Ion Ratio Lower Upper

266 100

264 60.9 52.5 78.7

268 62.0 54.4 81.6



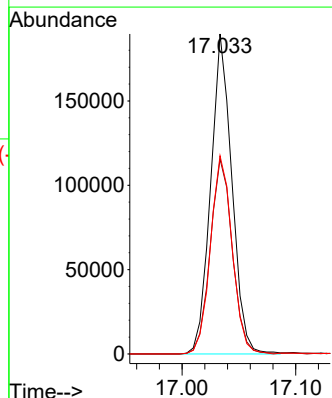





#72
Phenanthrene
Concen: 18.614 ng/ul
RT: 17.428 min Scan# 2404
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:178 Resp: 1949604
Ion Ratio Lower Upper
178 100
179 15.3 12.7 19.1
176 19.0 15.5 23.3



#74
Anthracene
Concen: 18.866 ng/ul
RT: 17.522 min Scan# 2420
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:178 Resp: 1985085
Ion Ratio Lower Upper
178 100
179 15.3 11.9 17.9
176 18.3 14.1 21.1









#75
1,2,3,4-Tetrachlorobenzene
Concen: 17.814 ng/uL
RT: 13.445 min Scan# 1727
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:216 Resp: 476039
Ion Ratio Lower Upper
216 100
214 78.3 62.7 94.1
218 50.4 38.0 57.0

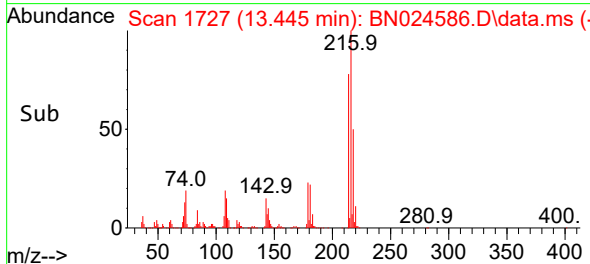

#76
Pentachlorobenzene
Concen: 17.737 ng/uL
RT: 14.957 min Scan# 1984
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:250 Resp: 460410
Ion Ratio Lower Upper
250 100
248 61.0 50.5 75.7
252 59.5 50.9 76.3

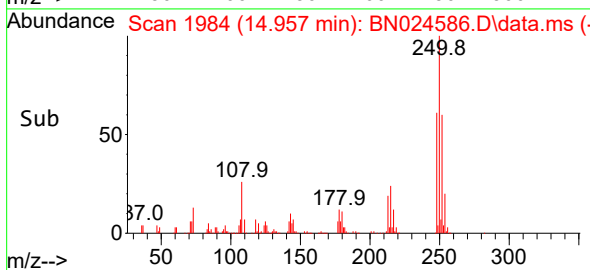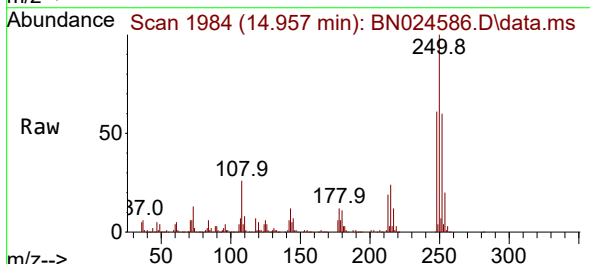



#77

Carbazole

Concen: 19.435 ng/ul

RT: 17.792 min Scan# 2466

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:167 Resp: 1838669

Ion Ratio Lower Upper

167 100

166 22.0 17.4 26.2

139 13.3 10.5 15.7

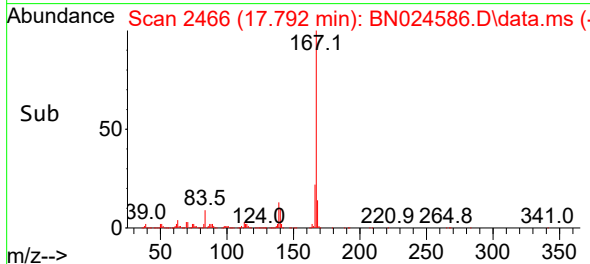

#78

Di-n-butylphthalate

Concen: 18.836 ng/ul

RT: 18.351 min Scan# 2561

Delta R.T. -0.000 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:149 Resp: 2019308


Ion Ratio Lower Upper

149 100

150 9.0 7.4 11.2

104 5.0 4.1 6.1


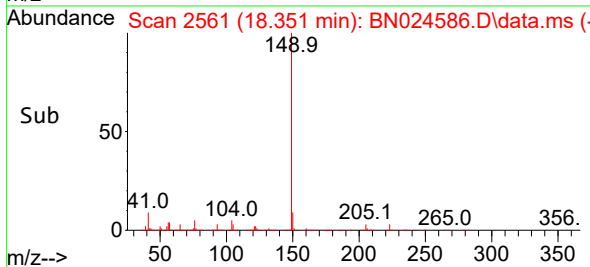

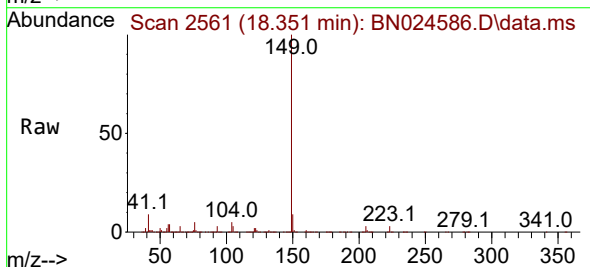




#80
Fluoranthene
Concen: 18.075 ng/ul
RT: 19.439 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:202 Resp: 2178468
Ion Ratio Lower Upper
202 100
101 12.9 10.3 15.5
100 9.7 8.2 12.2

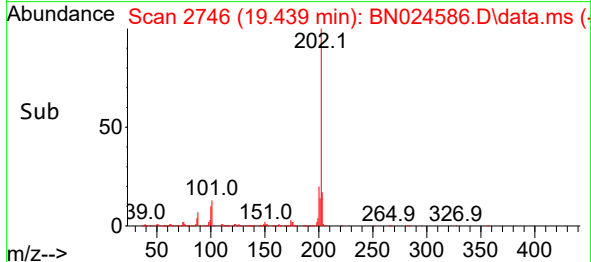

#82
Pyrene
Concen: 18.854 ng/ul
RT: 19.804 min Scan# 2808
Delta R.T. -0.000 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:202 Resp: 2395490
Ion Ratio Lower Upper
202 100
101 14.7 12.5 18.7
100 11.5 10.1 15.1




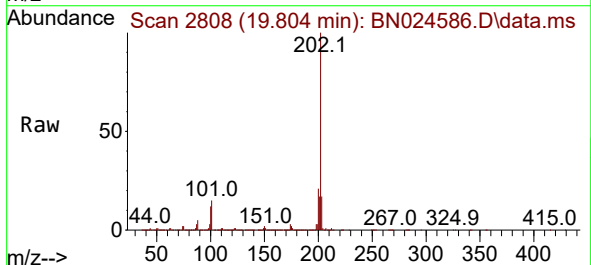




#83
Butylbenzylphthalate
Concen: 18.353 ng/ul
RT: 20.698 min Scan# 2959
Delta R.T. 0.006 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:149 Resp: 887850
Ion Ratio Lower Upper
149 100
91 78.0 59.7 89.5
206 19.1 15.4 23.2

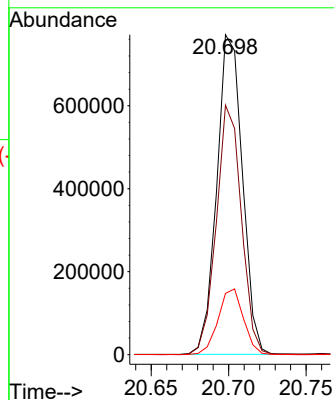

#84
3,3'-Dichlorobenzidine
Concen: 21.642 ng/ul
RT: 21.492 min Scan# 3095
Delta R.T. 0.006 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:252 Resp: 889190
Ion Ratio Lower Upper
252 100
254 67.3 50.0 75.0
126 12.2 9.8 14.8



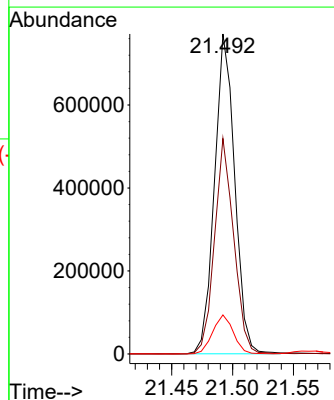





#85
Benzo(a)anthracene
Concen: 18.425 ng/ul
RT: 21.563 min Scan# 3106
Delta R.T. 0.006 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:228 Resp: 2287682
Ion Ratio Lower Upper
228 100
229 18.6 15.8 23.8
226 26.6 22.7 34.1

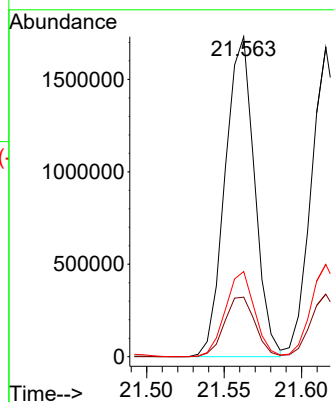

#86
Bis(2-ethylhexyl)phthalate
Concen: 18.896 ng/ul
RT: 21.480 min Scan# 3093
Delta R.T. 0.012 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:149 Resp: 1274558
Ion Ratio Lower Upper
149 100
167 27.8 21.6 32.4
279 3.8 2.7 4.1



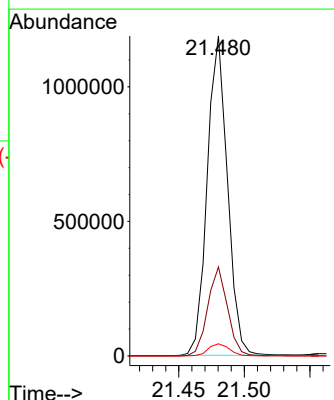





#87
Chrysene
Concen: 18.427 ng/ul
RT: 21.616 min Scan# 3115
Delta R.T. 0.006 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:228 Resp: 2164942
Ion Ratio Lower Upper
228 100
226 29.8 24.8 37.2
229 20.2 16.4 24.6

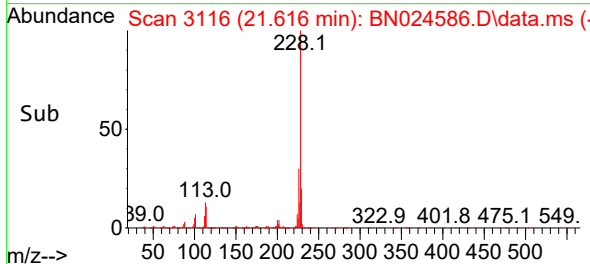

#89
Di-n-octyl phthalate
Concen: 18.142 ng/ul
RT: 22.439 min Scan# 3256
Delta R.T. 0.018 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:149 Resp: 2191255


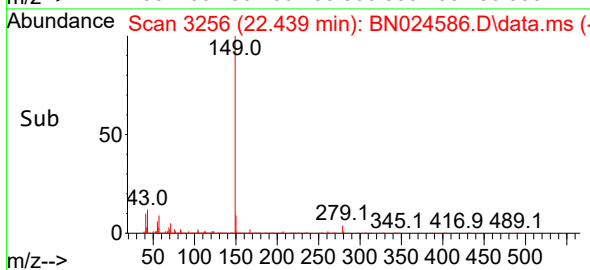

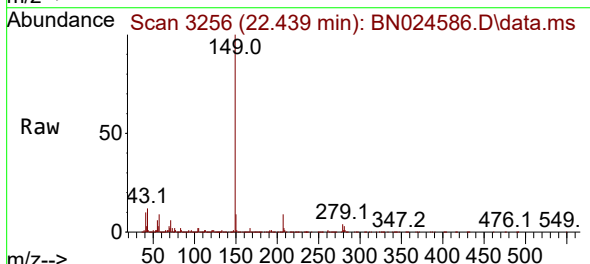




#90
Benzo(b)fluoranthene
Concen: 18.270 ng/ul
RT: 23.304 min Scan# 3400
Delta R.T. 0.018 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45




Instrument :
BNA_N
ClientSampleId :
SICV210


Tgt Ion:252 Resp: 2385315
Ion Ratio Lower Upper
252 100
253 21.8 15.8 23.8
125 11.0 8.6 13.0



#91
Benzo(k)fluoranthene
Concen: 18.383 ng/ul
RT: 23.351 min Scan# 3411
Delta R.T. 0.012 min
Lab File: BN024586.D
Acq: 28 Mar 2023 15:45

Tgt Ion:252 Resp: 2291300
Ion Ratio Lower Upper
252 100
253 21.0 17.5 26.3
125 11.4 9.2 13.8





#93

Benzo(a)pyrene

Concen: 18.261 ng/ul

RT: 23.957 min Scan# 31

Delta R.T. 0.018 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:252 Resp: 2087825

Ion Ratio Lower Upper

252 100

253 21.0 18.2 27.4

125 12.6 10.2 15.4



#94

Indeno(1,2,3-cd)pyrene

Concen: 18.004 ng/ul

RT: 26.668 min Scan# 3975

Delta R.T. 0.041 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45




Tgt Ion:276 Resp: 2623025


Ion Ratio Lower Upper

276 100

138 27.3 22.2 33.2

277 23.5 20.3 30.5





#95

Dibenzo(a,h)anthracene

Concen: 17.891 ng/ul

RT: 26.686 min Scan# 3971

Delta R.T. 0.041 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Instrument :

BNA_N

ClientSampleId :

SICV210





Tgt Ion:278 Resp: 2161732

Ion Ratio Lower Upper

278 100

139 18.2 14.2 21.4

279 24.3 19.6 29.4

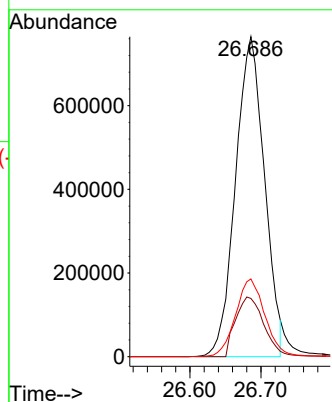

#96

Benzo(g,h,i)perylene

Concen: 17.275 ng/ul

RT: 27.474 min Scan# 4112

Delta R.T. 0.053 min

Lab File: BN024586.D

Acq: 28 Mar 2023 15:45

Tgt Ion:276 Resp: 2091181

Ion Ratio Lower Upper

276 100

138 23.5 19.5 29.3

277 21.7 18.4 27.6

