

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024595.D
 Acq On : 28 Mar 2023 21:13
 Operator : CG/JU
 Sample : 02086-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1




Instrument :
 BNA_N
 ClientSampleId :
 BFZ75

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/29/2023
 Supervised By :Jagrut Upadhyay 03/29/2023

Supervised By :Jagrut
 Upadhyay
 03/29/2023

Quant Time: Mar 29 05:04:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 29 03:32:05 2023
 Response via : Initial Calibration

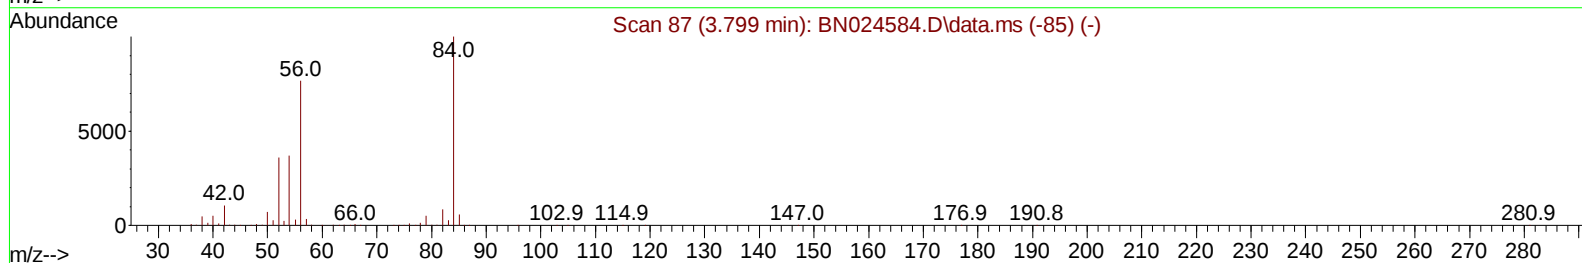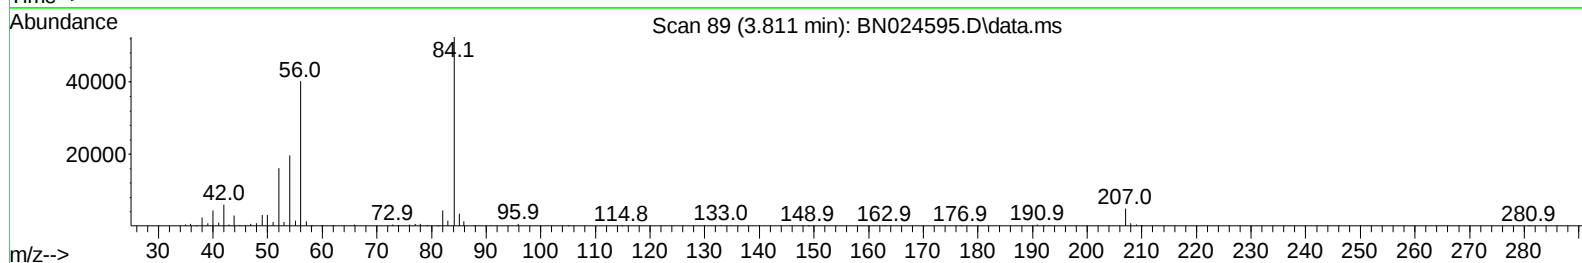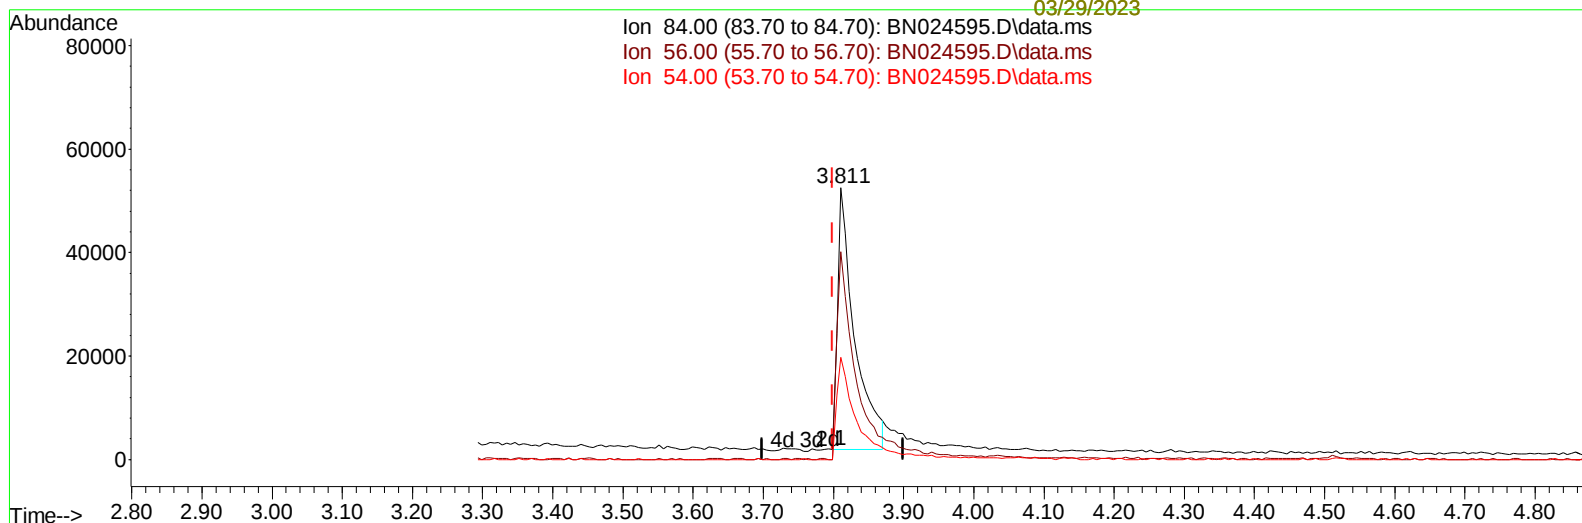

TIC: BN024595.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.012) 3.72 ng/u1

response 84632

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	75.10	76.56
54.00	36.20	37.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024595.D
Acq On : 28 Mar 2023 21:13
Operator : CG/JU
Sample : 02086-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ75


Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/29/2023
Supervised By :Jagrut Upadhyay 03/29/2023


Supervised By :Jagrut
Upadhyay
03/29/2023

Quant Time: Mar 29 05:04:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 29 03:32:05 2023
Response via : Initial Calibration


Ion 84.00 (83.70 to 84.70): BN024595.D\data.ms
Ion 56.00 (55.70 to 56.70): BN024595.D\data.ms
Ion 54.00 (53.70 to 54.70): BN024595.D\data.ms

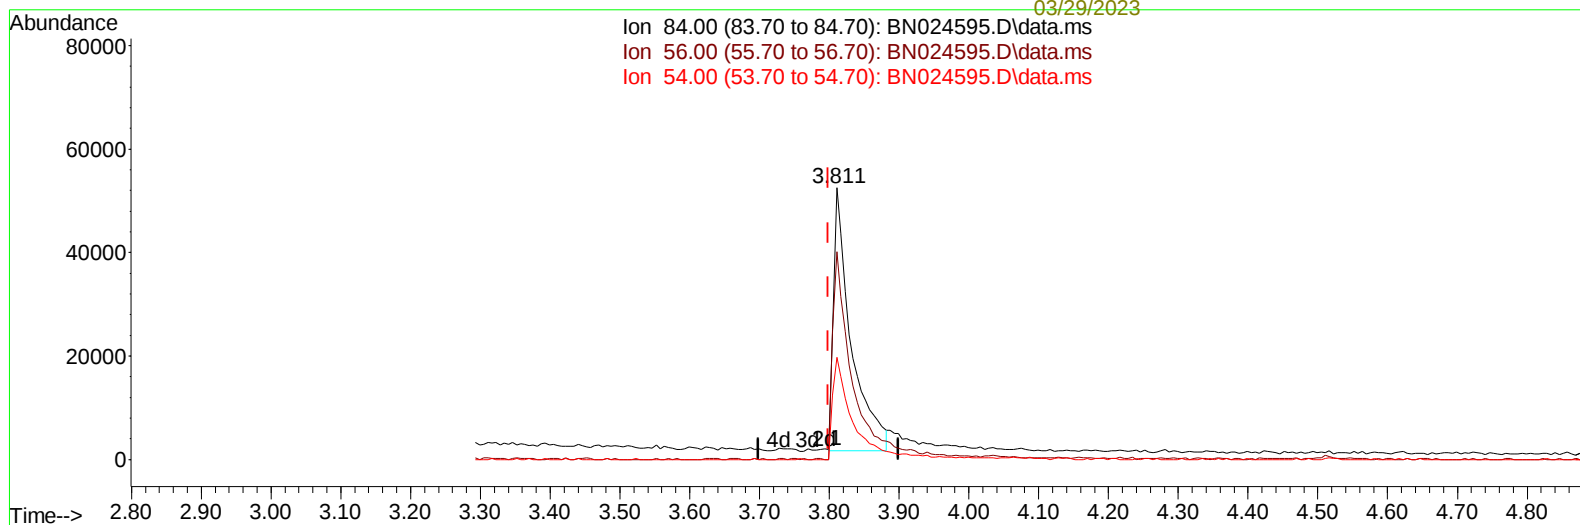

Scan 89 (3.811 min): BN024595.D\data.ms

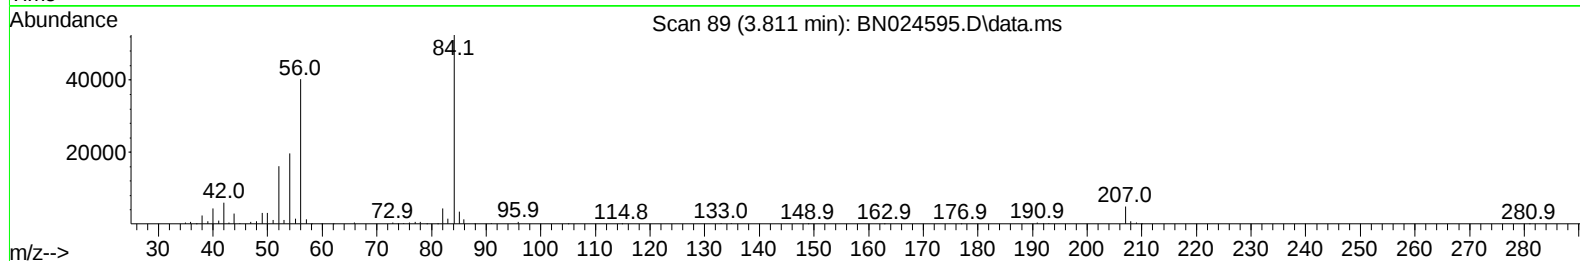

Scan 87 (3.799 min): BN024584.D\data.ms (-85) (-)

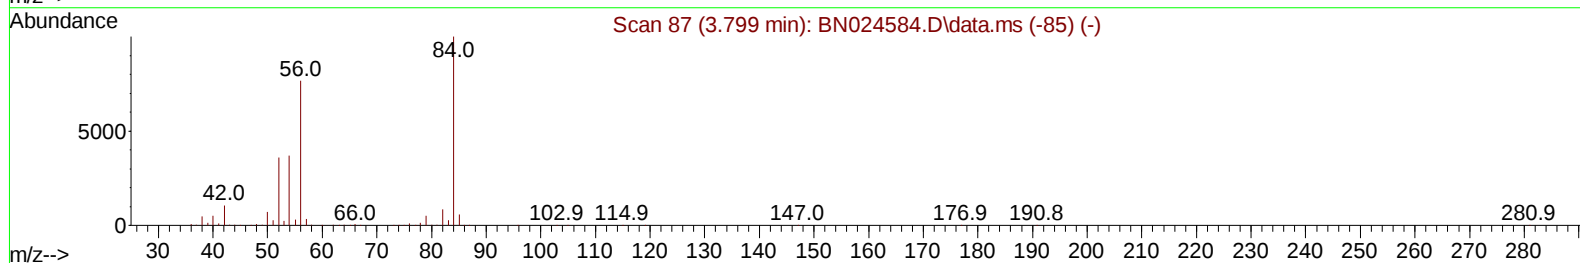

TIC: BN024595.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.012) 3.89 ng/u1 m

response 88523

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	75.10	76.56
54.00	36.20	37.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024595.D
 Acq On : 28 Mar 2023 21:13
 Operator : CG/JU
 Sample : 02086-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ75

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/29/2023
 Supervised By :Jagrut Upadhyay 03/29/2023

Supervised By :Jagrut
 Upadhyay
 03/29/2023

Quant Time: Mar 29 05:04:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 29 03:32:05 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.999	152		305545	20.000	ng/ul	0.00
20) Naphthalene-d8	10.816	136		1349701	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.639	164		878311	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188		1911021	20.000	ng/ul	0.00
79) Chrysene-d12	21.574	240		1772566	20.000	ng/ul	0.00
88) Perylene-d12	24.051	264		1934949	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.369	96		37980	4.819	ng/uL	0.00
4) Pyridine-d5	3.811	84		88523m	3.890	ng/ul	0.01
7) Phenol-d5	7.158	99		204248	7.064	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.322	67		555083	29.727	ng/ul	0.00
11) 2-Chlorophenol-d4	7.528	132		509233	23.754	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113		352432	15.240	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128		313694	29.368	ng/ul	0.00
24) 2-Nitrophenol-d4	9.893	143		322312	27.877	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165		548954	26.141	ng/ul	0.00
31) 4-Chloroaniline-d4	10.951	131		645379	20.141	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166		2040844	30.216	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160		2248543	29.237	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143		78198	5.532	ng/ul	0.00
60) Fluorene-d10	15.628	176		1790630	30.899	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200		298591	23.722	ng/ul	0.00
73) Anthracene-d10	17.486	188		3010661	33.496	ng/ul	0.00
81) Pyrene-d10	19.775	212		3566546	34.799	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.892	264		3463226	35.323	ng/ul	0.00
Target Compounds							
2) 1,4-Dioxane	3.411	88		13027	1.534	ng/uL	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024595.D
Acq On : 28 Mar 2023 21:13
Operator : CG/JU
Sample : 02086-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ75

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/29/2023
Supervised By :Jagrut Upadhyay 03/29/2023

Supervised By :Jagrut
Upadhyay
03/29/2023

Quant Time: Mar 29 05:04:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 29 03:32:05 2023
Response via : Initial Calibration

