

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024602.D
 Acq On : 29 Mar 2023 10:03
 Operator : CG/JU
 Sample : 01982-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EYGB1

Quant Time: Mar 30 02:29:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 02:26:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	325109	20.000	ng/u1	0.00
20) Naphthalene-d8	10.816	136	1440021	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.640	164	878802	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.386	188	1862168	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	1791117	20.000	ng/u1	0.00
88) Perylene-d12	24.068	264	1947823	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	32216	3.842	ng/uL	0.00
4) Pyridine-d5	3.793	84	436621	18.033	ng/u1	0.00
7) Phenol-d5	7.152	99	652805	21.217	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.322	67	418675	21.073	ng/u1	0.00
11) 2-Chlorophenol-d4	7.522	132	479644	21.028	ng/u1	0.00
15) 4-Methylphenol-d8	8.705	113	509013	20.687	ng/u1	0.00
21) Nitrobenzene-d5	9.163	128	223888	19.645	ng/u1	0.00
24) 2-Nitrophenol-d4	9.893	143	242155	19.630	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	457492	20.419	ng/u1	0.00
31) 4-Chloroaniline-d4	10.952	131	649965	19.012	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	1392777	20.610	ng/u1	0.00
49) Acenaphthylene-d8	14.334	160	1566022	20.351	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	221496	15.660	ng/u1	0.00
60) Fluorene-d10	15.628	176	1245214	21.475	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	161142	13.138	ng/u1	0.00
73) Anthracene-d10	17.486	188	1949243	22.256	ng/u1	0.00
81) Pyrene-d10	19.775	212	2247787	21.705	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.910	264	2164354	21.930	ng/u1	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.480	149	138514	2.015	ng/u1#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024602.D
Acq On : 29 Mar 2023 10:03
Operator : CG/JU
Sample : 01982-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYGB1

Quant Time: Mar 30 02:29:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 02:26:44 2023
Response via : Initial Calibration

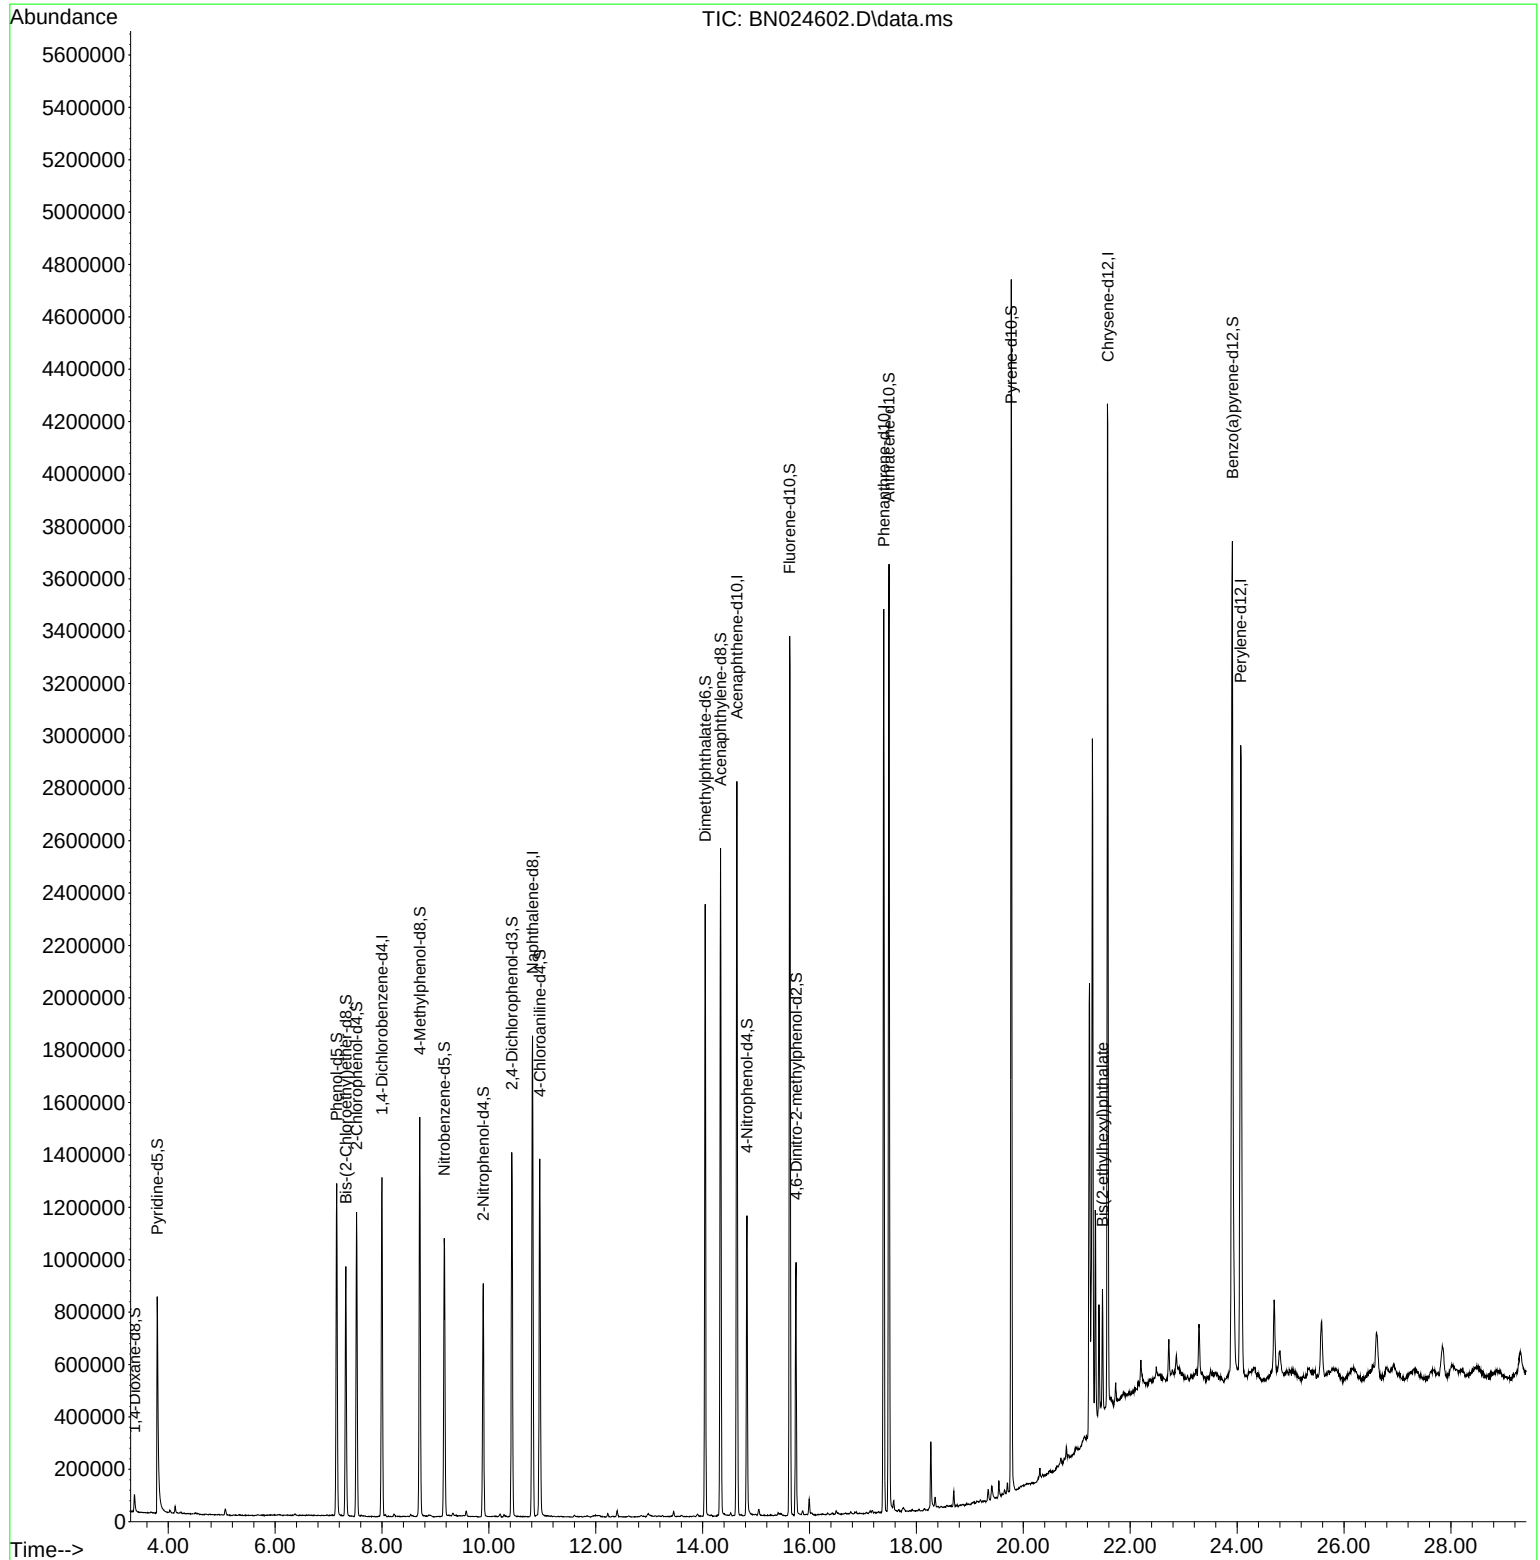

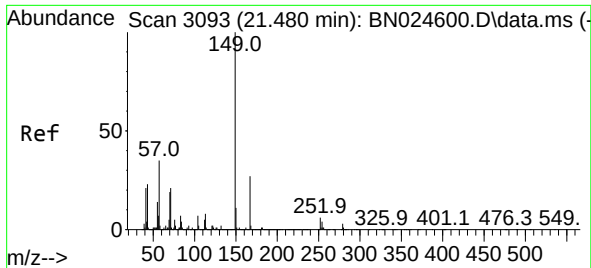

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.015 ng/ul
 RT: 21.480 min Scan# 3093
 Delta R.T. -0.000 min
 Lab File: BN024602.D
 Acq: 29 Mar 2023 10:03

Instrument :
 BNA_N
 ClientSampleId :
 EYGB1

Tgt Ion:149 Resp: 138514
 Ion Ratio Lower Upper
 149 100
 167 26.4 21.6 32.4
 279 4.1 2.7 4.1#

