

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024587.D
 Acq On : 28 Mar 2023 16:22
 Operator : CG/JU
 Sample : PB151699BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK699

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	23	rVB	86448	124862	1.35%	0.139%
2	3.799	84	87	111	rBV	1111454	1838686	19.82%	2.049%
3	4.134	140	144	152	rVB	20363	32556	0.35%	0.036%
4	7.158	649	658	669	rBV	1487424	2318469	25.00%	2.583%
5	7.328	679	687	698	rVB	1195696	1849679	19.94%	2.061%
6	7.528	713	721	729	rBV	1430367	2258887	24.35%	2.517%
7	8.005	794	802	809	rBV	1005513	1635050	17.63%	1.822%
8	8.710	914	922	931	rBV	1802632	2817960	30.38%	3.140%
9	9.169	993	1000	1011	rBV	1421062	2306090	24.86%	2.570%
10	9.899	1113	1124	1132	rBV	1162238	1922387	20.73%	2.142%
11	10.434	1208	1215	1226	rBV	1691934	2759169	29.75%	3.075%
12	10.816	1272	1280	1289	rVB	1510201	2510784	27.07%	2.798%
13	10.957	1294	1304	1315	rBV	1847415	3129275	33.74%	3.487%
14	11.604	1410	1414	1419	rBV5	6747	11824	0.13%	0.013%
15	12.398	1543	1549	1557	rVB	31266	53603	0.58%	0.060%
16	12.998	1645	1651	1655	rBV6	6815	12142	0.13%	0.014%
17	13.910	1802	1806	1814	rBV6	7899	14909	0.16%	0.017%
18	14.045	1823	1829	1840	rVB	3270321	4603624	49.63%	5.130%
19	14.334	1871	1878	1890	rBV	3595729	5231101	56.40%	5.829%
20	14.640	1923	1930	1938	rBV	2351651	3456249	37.26%	3.851%
21	14.728	1942	1945	1951	rVB7	5685	10172	0.11%	0.011%
22	14.828	1956	1962	1975	rBV	1877652	2609261	28.13%	2.908%
23	15.416	2057	2062	2064	rBV4	7575	9749	0.11%	0.011%
24	15.634	2090	2099	2106	rBV	4541707	6549039	70.61%	7.298%
25	15.745	2111	2118	2132	rVV	1924134	2439031	26.30%	2.718%
26	15.869	2136	2139	2146	rVB4	22915	38705	0.42%	0.043%
27	17.063	2339	2342	2348	rVB6	7303	10730	0.12%	0.012%
28	17.386	2390	2397	2406	rBV	3015738	4205347	45.34%	4.686%
29	17.486	2407	2414	2428	rVV	5251124	7387145	79.64%	8.232%
30	19.339	2725	2729	2735	rBV2	55365	81225	0.88%	0.091%
31	19.410	2737	2741	2747	rVV	59828	82411	0.89%	0.092%
32	19.775	2797	2803	2816	rBV	6302338	8569552	92.39%	9.549%
33	21.574	3104	3109	3117	rBV2	3478071	4608531	49.69%	5.135%
34	23.915	3499	3507	3518	rBV	4554436	9275291	100.00%	10.335%
35	24.063	3525	3532	3545	rVB2	2360678	4978689	53.68%	5.548%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024587.D
Acq On : 28 Mar 2023 16:22
Operator : CG/JU
Sample : PB151699BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK699

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Title : SVOA CALIBRATION




Sum of corrected areas: 89742184

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024587.D
Acq On : 28 Mar 2023 16:22
Operator : CG/JU
Sample : PB151699BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK699

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

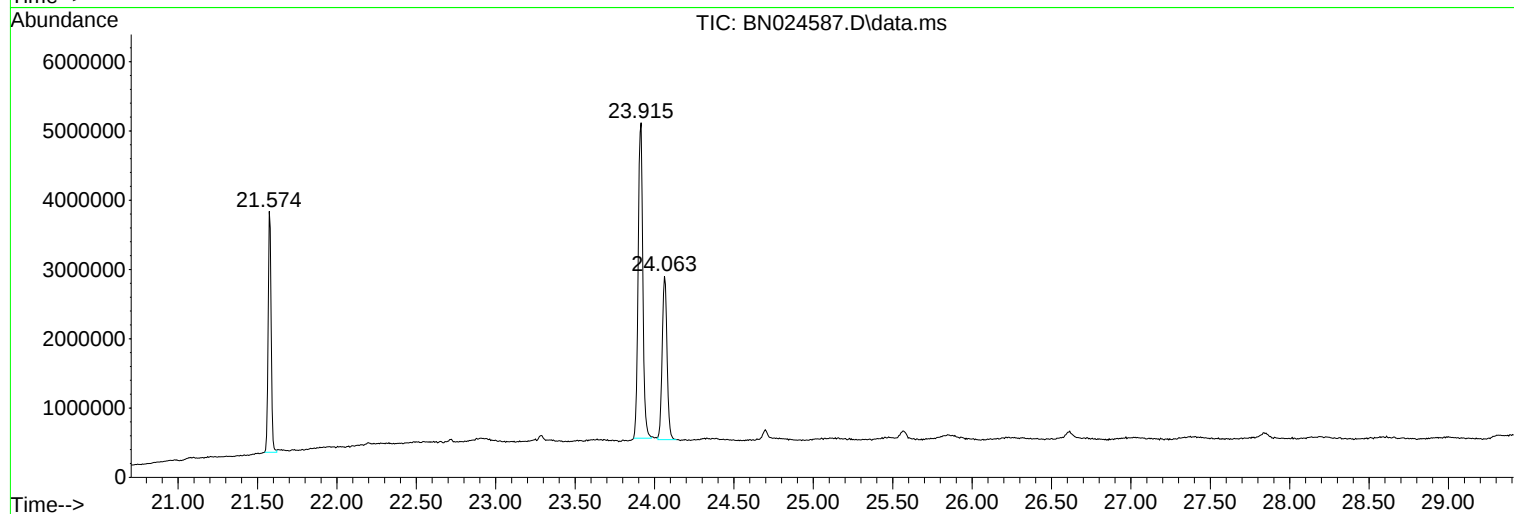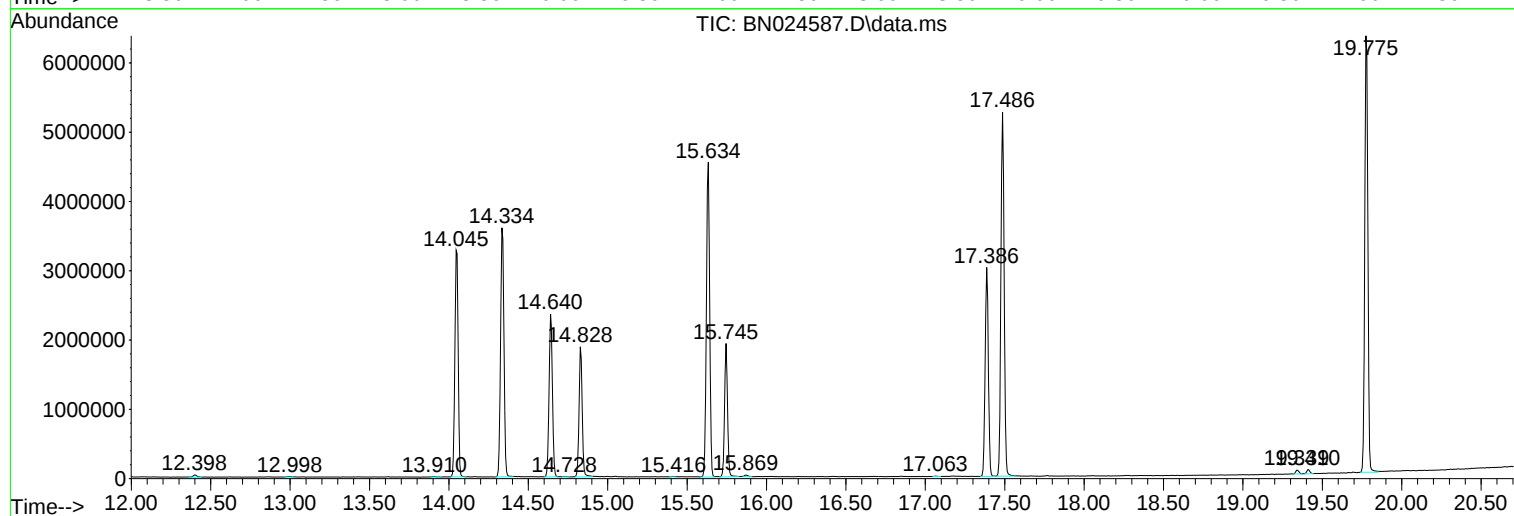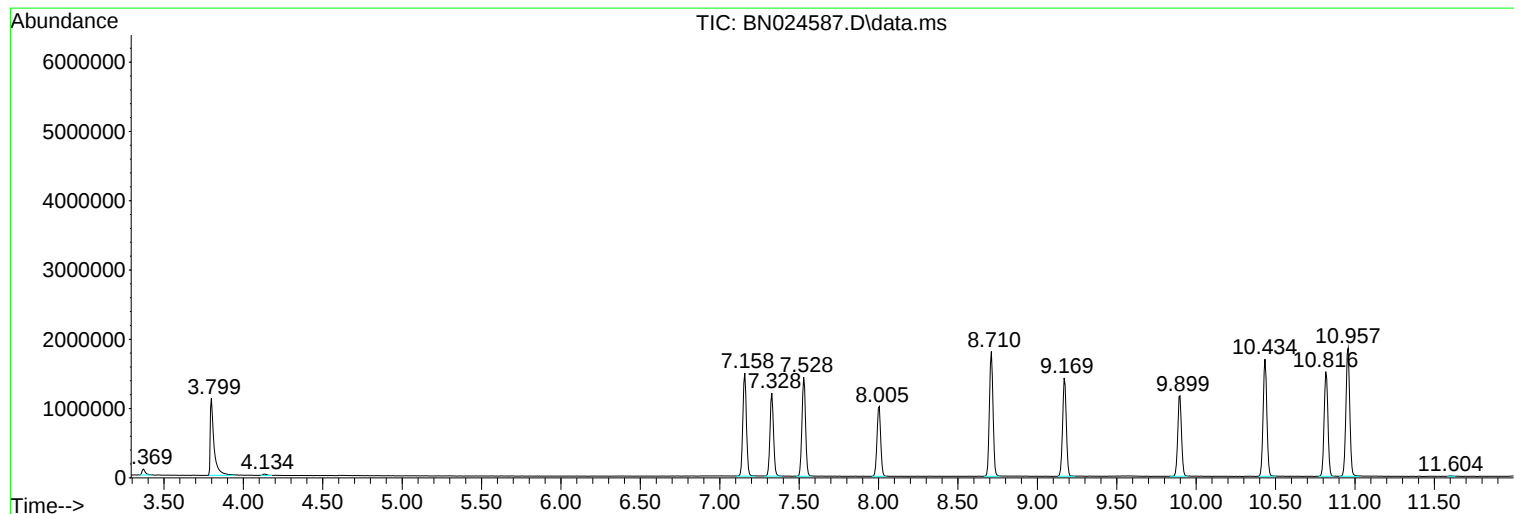

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024587.D
Acq On : 28 Mar 2023 16:22
Operator : CG/JU
Sample : PB151699BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK699

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024587.D
Acq On : 28 Mar 2023 16:22
Operator : CG/JU
Sample : PB151699BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK699

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc