

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024590.D
 Acq On : 28 Mar 2023 18:11
 Operator : CG/JU
 Sample : PB151705BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK705

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	27	rVB	97636	160924	1.59%	0.167%
2	3.799	84	87	109	rBV	1204239	1963020	19.36%	2.041%
3	4.134	140	144	152	rVB	21877	32852	0.32%	0.034%
4	7.158	649	658	675	rBV	1563580	2480806	24.47%	2.579%
5	7.328	679	687	701	rVB	1268464	1982018	19.55%	2.061%
6	7.528	714	721	733	rBV	1516775	2383127	23.50%	2.478%
7	7.999	794	801	812	rBV	1129805	1860633	18.35%	1.934%
8	8.710	913	922	933	rBV	1853024	2980181	29.39%	3.098%
9	9.169	992	1000	1008	rBV	1529264	2456095	24.22%	2.553%
10	9.893	1115	1123	1133	rBV	1215714	2030910	20.03%	2.111%
11	10.434	1205	1215	1225	rBV	1778742	2929396	28.89%	3.046%
12	10.816	1272	1280	1290	rBV	1702078	2805950	27.68%	2.917%
13	10.951	1295	1303	1315	rBV	1880563	3267874	32.23%	3.397%
14	11.604	1408	1414	1418	rBV9	6509	11837	0.12%	0.012%
15	12.398	1543	1549	1556	rBV2	32116	55549	0.55%	0.058%
16	12.993	1645	1650	1654	rBV6	7463	14034	0.14%	0.015%
17	13.534	1734	1742	1745	rBV6	6457	11811	0.12%	0.012%
18	13.910	1802	1806	1811	rBV6	7303	10767	0.11%	0.011%
19	14.045	1822	1829	1842	rBV	3526458	4780597	47.15%	4.970%
20	14.334	1871	1878	1892	rBV	3641709	5442646	53.68%	5.658%
21	14.640	1922	1930	1939	rBV	2608582	3822135	37.70%	3.974%
22	14.828	1955	1962	1977	rBV	2013885	2784479	27.46%	2.895%
23	15.039	1996	1998	2004	rVB6	7477	11101	0.11%	0.012%
24	15.634	2090	2099	2105	rBV	4728189	6887173	67.93%	7.160%
25	15.745	2112	2118	2127	rBV	1976729	2536706	25.02%	2.637%
26	15.869	2135	2139	2144	rVB3	22643	31567	0.31%	0.033%
27	17.175	2357	2361	2366	rBV4	6753	11142	0.11%	0.012%
28	17.386	2390	2397	2407	rBV	3259535	4607594	45.44%	4.790%
29	17.486	2407	2414	2425	rBV	5425357	7718087	76.12%	8.024%
30	17.763	2458	2461	2468	rVB4	7238	11132	0.11%	0.012%
31	18.263	2543	2546	2551	rBV6	9079	13201	0.13%	0.014%
32	19.339	2725	2729	2735	rBV2	62494	87347	0.86%	0.091%
33	19.410	2737	2741	2745	rBV	63900	88316	0.87%	0.092%
34	19.775	2797	2803	2815	rBV	6719280	9040894	89.17%	9.399%
35	21.574	3104	3109	3119	rBV	3950664	5083967	50.14%	5.286%
36	23.904	3498	3505	3520	rBV2	5243314	10138933	100.00%	10.541%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024590.D
Acq On : 28 Mar 2023 18:11
Operator : CG/JU
Sample : PB151705BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK705

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Title : SVOA CALIBRATION

37	24.063	3525	3532	3545	rVB2	2565519	5652083	55.75%	5.876%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 96186884

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024590.D
Acq On : 28 Mar 2023 18:11
Operator : CG/JU
Sample : PB151705BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK705

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

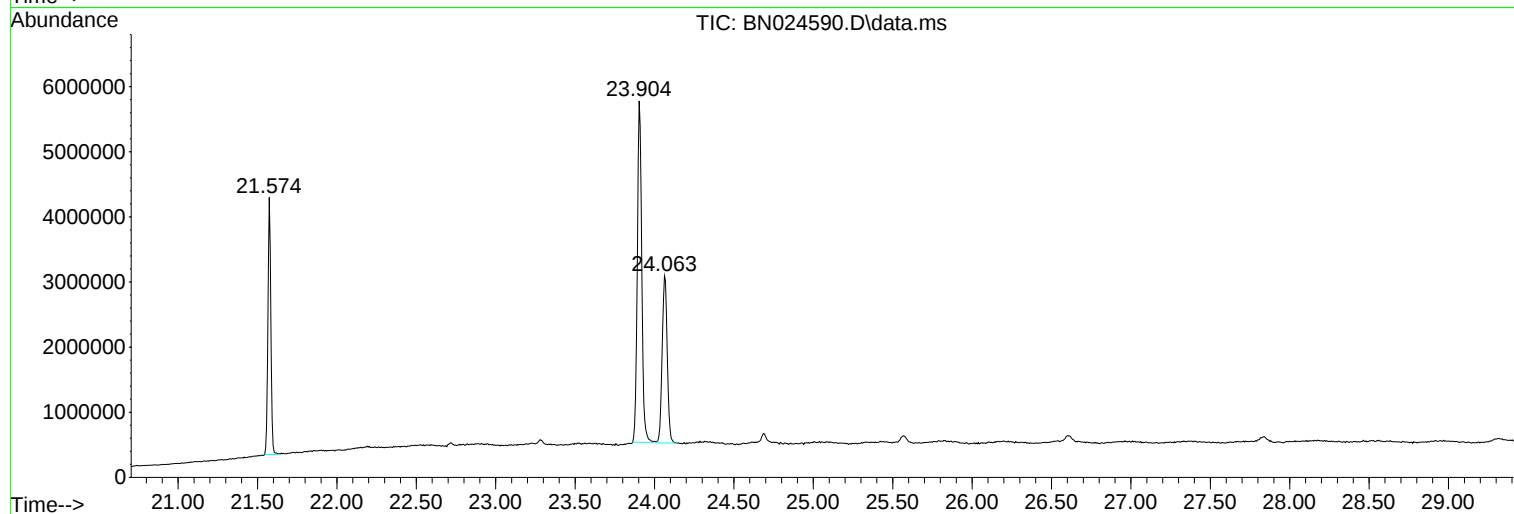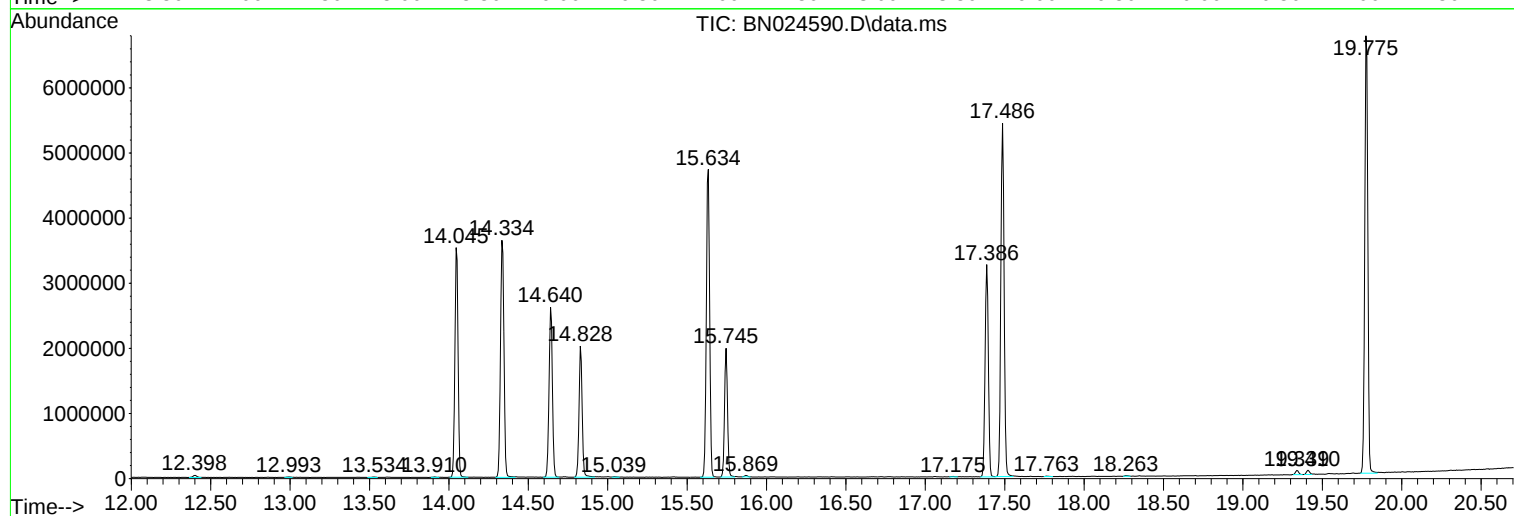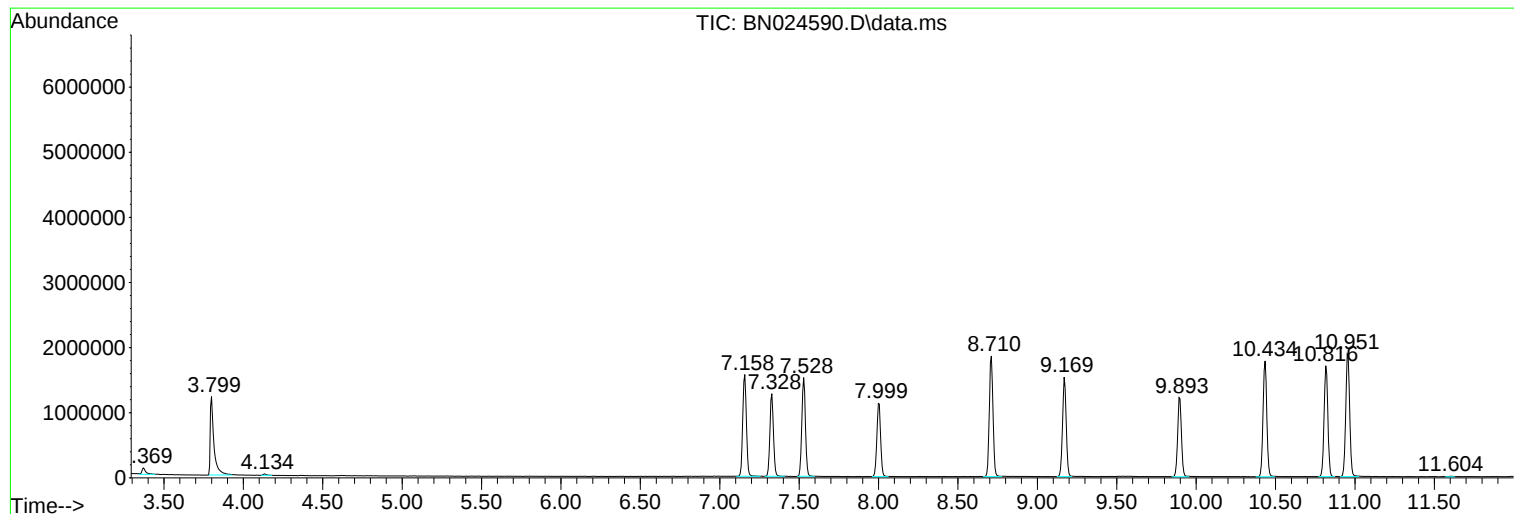

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024590.D
Acq On : 28 Mar 2023 18:11
Operator : CG/JU
Sample : PB151705BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK705

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024590.D
Acq On : 28 Mar 2023 18:11
Operator : CG/JU
Sample : PB151705BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK705

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc