

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024591.D
 Acq On : 28 Mar 2023 18:47
 Operator : CG/JU
 Sample : 02086-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024591.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	27	rVB	71013	104122	1.03%	0.123%
2	3.805	86	88	106	rBV	249160	427977	4.22%	0.506%
3	4.034	123	127	133	rVB	29719	43016	0.42%	0.051%
4	4.134	139	144	152	rVB	23415	32405	0.32%	0.038%
5	4.240	158	162	166	rBV3	16175	22832	0.23%	0.027%
6	4.799	252	257	261	rBV7	7283	11713	0.12%	0.014%
7	5.069	298	303	312	rVB	25325	44763	0.44%	0.053%
8	6.375	520	525	531	rVB4	16065	27486	0.27%	0.033%
9	6.669	572	575	580	rVB6	10272	15886	0.16%	0.019%
10	6.987	621	629	635	rBV7	12145	31196	0.31%	0.037%
11	7.157	651	658	668	rVB	245856	426830	4.21%	0.505%
12	7.328	679	687	697	rBV	1053534	1693943	16.71%	2.004%
13	7.528	714	721	731	rBV	903973	1413534	13.94%	1.672%
14	7.999	794	801	808	rBV	1088604	1777633	17.54%	2.103%
15	8.063	808	812	818	rVB	53353	83365	0.82%	0.099%
16	8.710	912	922	930	rBV	716372	1155585	11.40%	1.367%
17	9.169	991	1000	1009	rBV	1333036	2126373	20.98%	2.515%
18	9.575	1063	1069	1073	rVB3	11595	21456	0.21%	0.025%
19	9.893	1115	1123	1135	rBV	891549	1463939	14.44%	1.732%
20	10.434	1206	1215	1228	rBV	1282332	2082591	20.54%	2.463%
21	10.816	1270	1280	1287	rBV	1637922	2735425	26.98%	3.236%
22	10.875	1287	1290	1295	rVV6	9940	13936	0.14%	0.016%
23	10.951	1295	1303	1321	rVV	1447161	2476878	24.43%	2.930%
24	11.346	1364	1370	1376	rBV7	7771	15269	0.15%	0.018%
25	11.593	1408	1412	1418	rBV8	11347	20085	0.20%	0.024%
26	12.222	1513	1519	1525	rBV3	19668	32091	0.32%	0.038%
27	12.316	1530	1535	1539	rVV2	11843	20342	0.20%	0.024%
28	12.398	1542	1549	1556	rVV2	25843	44702	0.44%	0.053%
29	13.481	1726	1733	1738	rBV2	52421	91011	0.90%	0.108%
30	13.528	1738	1741	1748	rVB2	22878	35768	0.35%	0.042%
31	13.910	1802	1806	1811	rBV5	5278	10453	0.10%	0.012%
32	14.045	1822	1829	1840	rBV	3170566	4400390	43.41%	5.205%
33	14.334	1871	1878	1890	rBV	3393245	4847804	47.82%	5.734%
34	14.522	1907	1910	1917	rVB9	6183	12395	0.12%	0.015%
35	14.639	1922	1930	1938	rBV	2584531	3754300	37.04%	4.441%
36	14.728	1942	1945	1953	rVB9	7383	12122	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024591.D
 Acq On : 28 Mar 2023 18:47
 Operator : CG/JU
 Sample : 02086-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

37	14.828	1956	1962	1973	rBV	269788	412681	4.07%	0.488%
38	15.051	1995	2000	2006	rVB10	12410	20723	0.20%	0.025%
39	15.204	2022	2026	2029	rBV3	7430	10562	0.10%	0.012%
40	15.410	2057	2061	2065	rBV6	7253	10633	0.10%	0.013%
41	15.581	2084	2090	2092	rBV3	33578	51296	0.51%	0.061%
42	15.634	2092	2099	2107	rVV	4427556	6565352	64.77%	7.766%
43	15.745	2111	2118	2130	rBV	1605862	2126591	20.98%	2.516%
44	15.869	2134	2139	2144	rVB3	23354	37346	0.37%	0.044%
45	15.992	2155	2160	2166	rBV	125472	173777	1.71%	0.206%
46	16.251	2200	2204	2208	rVB	7717	10778	0.11%	0.013%
47	16.333	2213	2218	2225	rVB10	11722	22089	0.22%	0.026%
48	17.057	2339	2341	2347	rVB6	6409	10220	0.10%	0.012%
49	17.386	2390	2397	2406	rBV	3208031	4511921	44.51%	5.337%
50	17.486	2407	2414	2432	rVV	5740024	8006663	78.99%	9.471%
51	17.775	2457	2463	2466	rBV4	8924	18599	0.18%	0.022%
52	18.269	2542	2547	2554	rBV	180063	251230	2.48%	0.297%
53	18.345	2557	2560	2563	rVV	20311	23667	0.23%	0.028%
54	18.616	2603	2606	2610	rBV6	8985	12917	0.13%	0.015%
55	19.345	2725	2730	2735	rBV	66059	94423	0.93%	0.112%
56	19.410	2737	2741	2746	rVV	72451	107019	1.06%	0.127%
57	19.498	2752	2756	2758	rBV4	22903	27774	0.27%	0.033%
58	19.539	2759	2763	2769	rBV	147519	203093	2.00%	0.240%
59	19.774	2797	2803	2814	rBV	6815037	9334593	92.09%	11.042%
60	21.269	3053	3057	3067	rBV	228730	413033	4.07%	0.489%
61	21.574	3104	3109	3118	rBV2	3754606	4974377	49.07%	5.884%
62	23.910	3499	3506	3522	rVV2	5019253	10136839	100.00%	11.991%
63	24.062	3525	3532	3550	rVB2	2648520	5440891	53.67%	6.436%




Sum of corrected areas: 84538703

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024591.D
Acq On : 28 Mar 2023 18:47
Operator : CG/JU
Sample : 02086-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ70

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

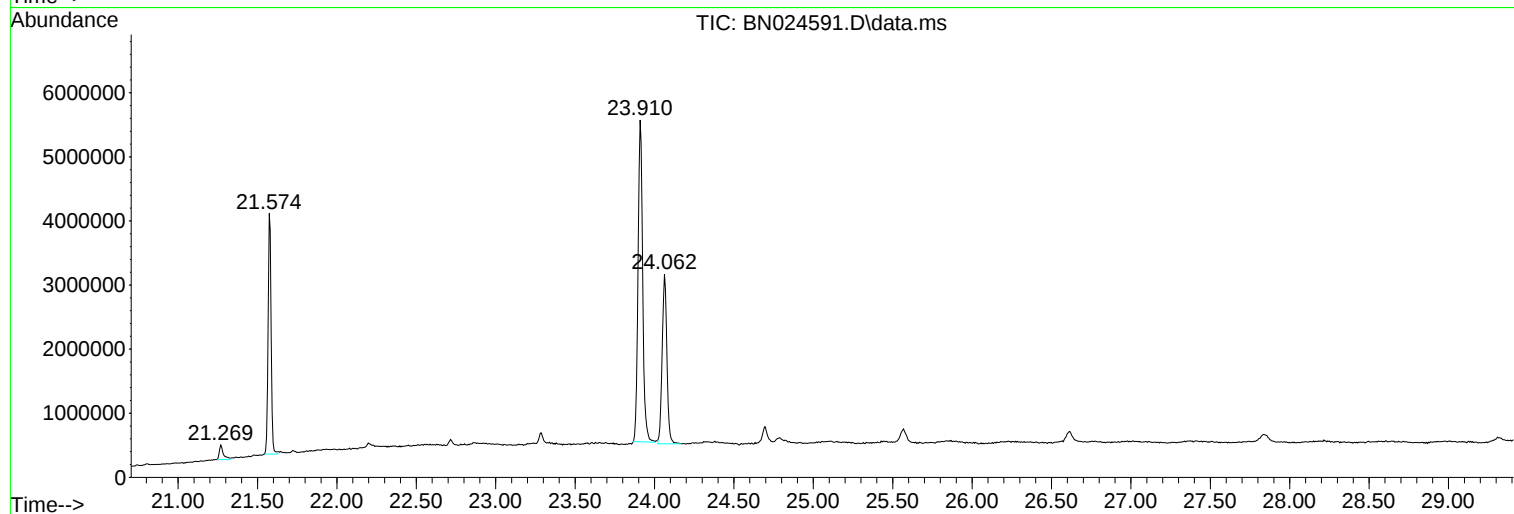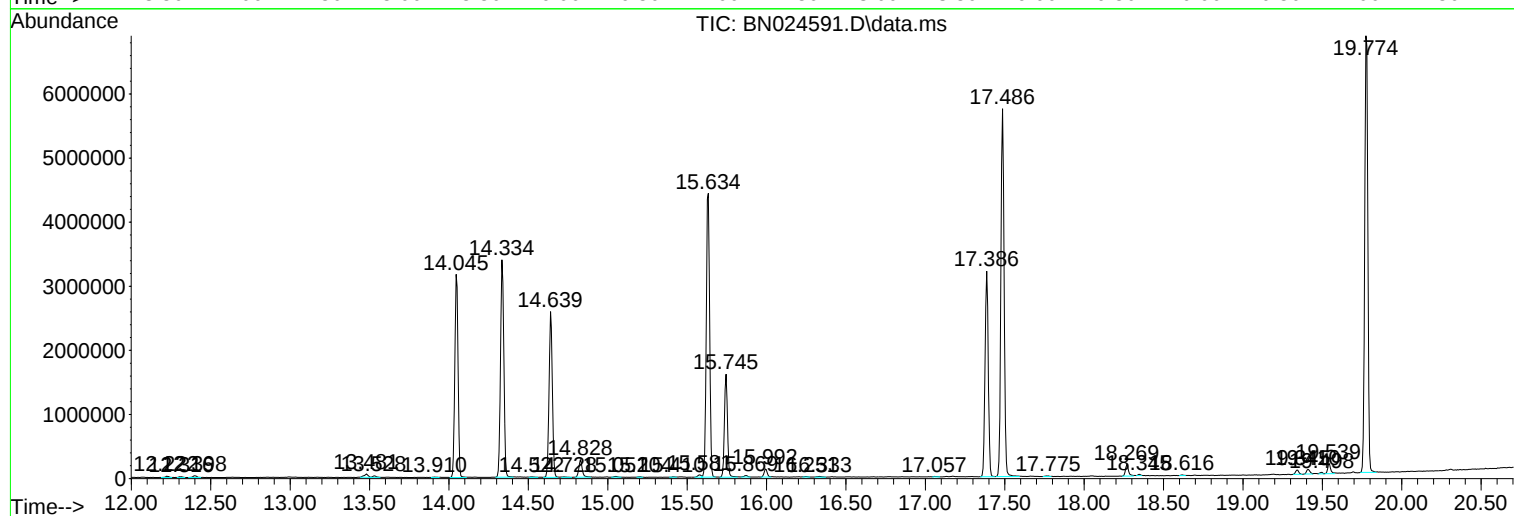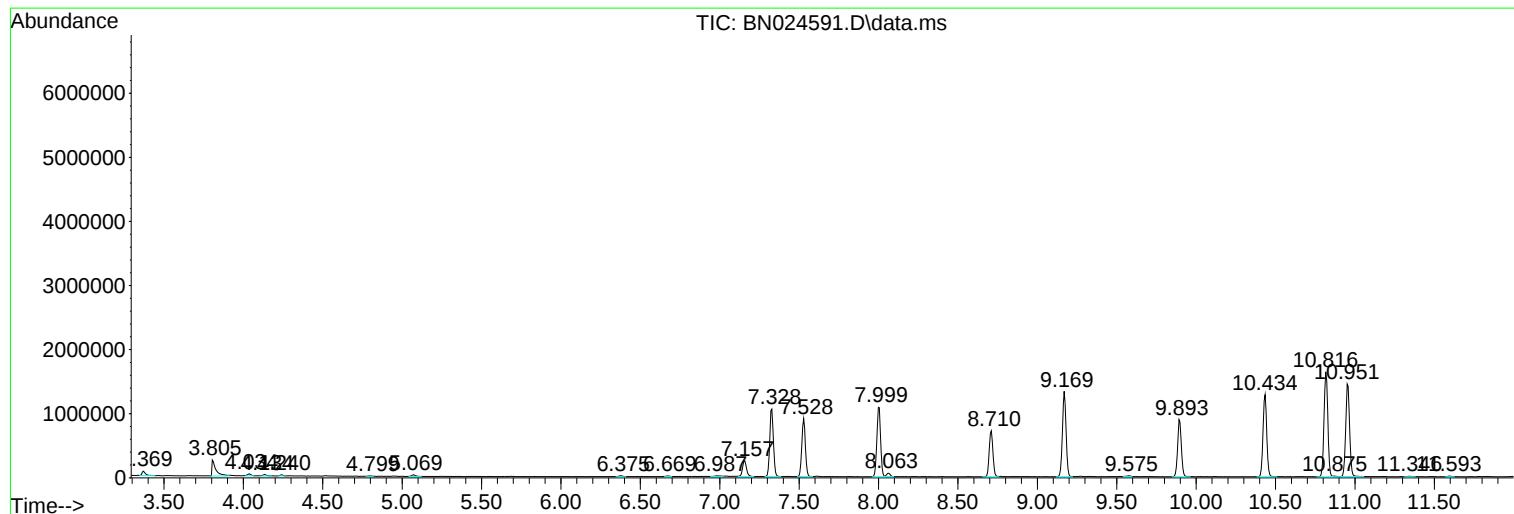

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024591.D
Acq On : 28 Mar 2023 18:47
Operator : CG/JU
Sample : 02086-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ70

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024591.D
Acq On : 28 Mar 2023 18:47
Operator : CG/JU
Sample : 02086-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ70

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
