

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024592.D
 Acq On : 28 Mar 2023 19:24
 Operator : CG/JU
 Sample : 02086-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	27	rVB	66663	105899	0.99%	0.119%
2	3.805	86	88	114	rBV	336741	625913	5.88%	0.705%
3	4.034	122	127	135	rVB	28355	50664	0.48%	0.057%
4	4.134	140	144	150	rVB2	20769	31239	0.29%	0.035%
5	4.240	157	162	169	rVB7	18334	32332	0.30%	0.036%
6	5.070	299	303	312	rBV	25675	41250	0.39%	0.046%
7	6.375	521	525	532	rVB2	17391	26902	0.25%	0.030%
8	7.158	648	658	668	rVB	260139	426478	4.01%	0.480%
9	7.328	680	687	697	rBV	1147395	1864572	17.51%	2.100%
10	7.528	713	721	731	rBV	1013744	1601126	15.04%	1.803%
11	7.611	732	735	741	rVB4	7886	12419	0.12%	0.014%
12	7.999	792	801	809	rBV	1125596	1829258	17.18%	2.060%
13	8.711	915	922	933	rBV	791013	1274006	11.97%	1.435%
14	9.169	992	1000	1008	rBV	1485145	2366192	22.23%	2.665%
15	9.269	1012	1017	1023	rVV6	8859	17028	0.16%	0.019%
16	9.334	1023	1028	1032	rVB7	6801	11936	0.11%	0.013%
17	9.575	1065	1069	1078	rVB3	12564	24462	0.23%	0.028%
18	9.893	1115	1123	1139	rBV	1086039	1785332	16.77%	2.010%
19	10.116	1157	1161	1169	rVB9	8754	15564	0.15%	0.018%
20	10.434	1207	1215	1224	rBV	1511881	2453991	23.05%	2.763%
21	10.816	1269	1280	1290	rBV	1663442	2775953	26.08%	3.126%
22	10.952	1295	1303	1324	rBV	1585146	2759194	25.92%	3.107%
23	11.599	1407	1413	1418	rBV4	18105	33974	0.32%	0.038%
24	12.075	1487	1494	1499	rVB4	7572	14533	0.14%	0.016%
25	12.228	1513	1520	1525	rBV2	17539	29622	0.28%	0.033%
26	12.399	1543	1549	1555	rBV	30525	49949	0.47%	0.056%
27	13.251	1689	1694	1701	rVB9	6542	10949	0.10%	0.012%
28	13.457	1725	1729	1733	rVB4	13659	18605	0.17%	0.021%
29	14.046	1822	1829	1845	rBV	3452123	4837833	45.44%	5.448%
30	14.334	1871	1878	1889	rVV	3804785	5410296	50.82%	6.092%
31	14.640	1923	1930	1941	rBV	2586912	3808348	35.77%	4.288%
32	14.728	1943	1945	1951	rVB7	7702	11846	0.11%	0.013%
33	14.828	1955	1962	1976	rBV	269447	419501	3.94%	0.472%
34	15.046	1995	1999	2003	rBV6	15120	25516	0.24%	0.029%
35	15.198	2021	2025	2029	rVB5	8477	10656	0.10%	0.012%
36	15.422	2058	2063	2066	rBV6	8468	17083	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024592.D
 Acq On : 28 Mar 2023 19:24
 Operator : CG/JU
 Sample : 02086-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

37	15.451	2066	2068	2076	rVB3	12270	20544	0.19%	0.023%
38	15.575	2084	2089	2092	rBV2	37684	57760	0.54%	0.065%
39	15.634	2092	2099	2109	rVV	4851653	7110654	66.79%	8.007%
40	15.745	2111	2118	2134	rVV	1837966	2428240	22.81%	2.734%
41	15.869	2134	2139	2144	rVB3	27042	39748	0.37%	0.045%
42	15.934	2146	2150	2155	rBV5	8302	11059	0.10%	0.012%
43	15.993	2155	2160	2165	rBV	88094	125661	1.18%	0.142%
44	17.169	2357	2360	2365	rBV2	8434	11959	0.11%	0.013%
45	17.292	2377	2381	2385	rBV6	7167	11119	0.10%	0.013%
46	17.387	2391	2397	2406	rBV	3305056	4588569	43.10%	5.167%
47	17.487	2407	2414	2425	rBV	5792778	8229281	77.30%	9.267%
48	17.669	2440	2445	2451	rBV4	9268	17662	0.17%	0.020%
49	17.757	2458	2460	2467	rVB3	8868	12616	0.12%	0.014%
50	18.269	2543	2547	2552	rBV2	91570	123485	1.16%	0.139%
51	18.345	2557	2560	2566	rVB	21069	32254	0.30%	0.036%
52	19.339	2725	2729	2734	rBV2	71588	99720	0.94%	0.112%
53	19.410	2737	2741	2747	rVV	72539	107326	1.01%	0.121%
54	19.539	2760	2763	2767	rBV4	35021	42804	0.40%	0.048%
55	19.692	2787	2789	2794	rVB5	14022	16471	0.15%	0.019%
56	19.775	2797	2803	2815	rBV2	6959142	9600919	90.18%	10.811%
57	21.269	3053	3057	3063	rBV3	138453	225239	2.12%	0.254%
58	21.575	3104	3109	3115	rBV2	3736633	4965644	46.64%	5.592%
59	23.904	3497	3505	3523	rVB2	5389540	10645966	100.00%	11.988%
60	24.069	3525	3533	3545	rVB	2420680	5449008	51.18%	6.136%




Sum of corrected areas: 88804129

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024592.D
Acq On : 28 Mar 2023 19:24
Operator : CG/JU
Sample : 02086-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ76

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

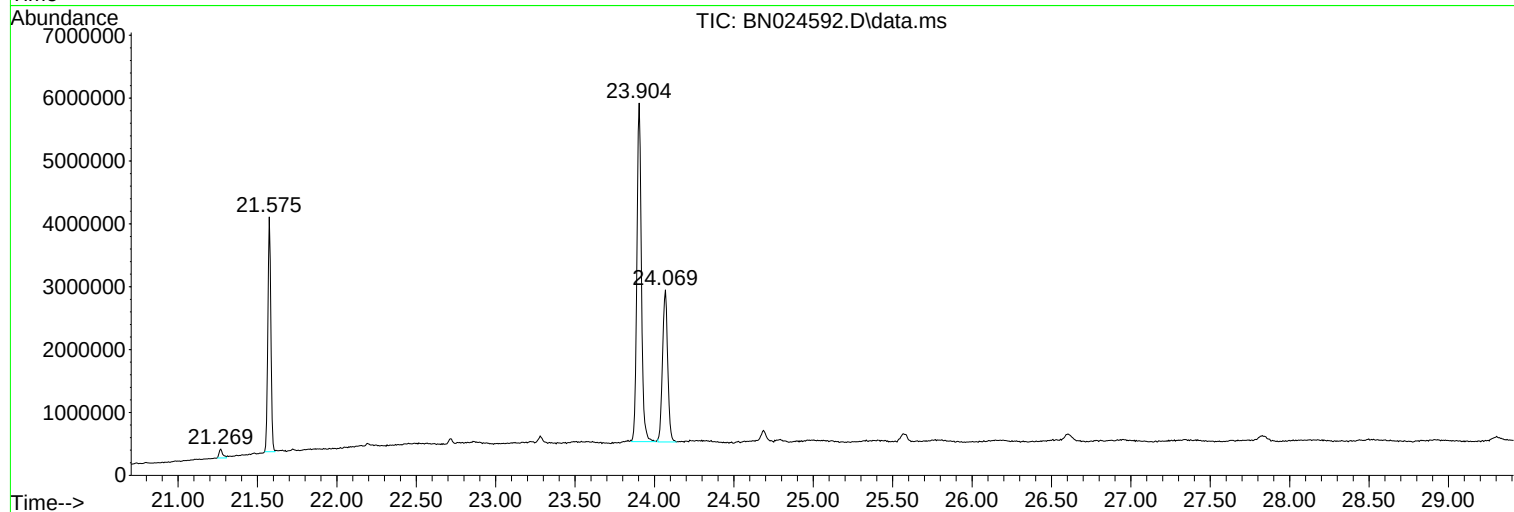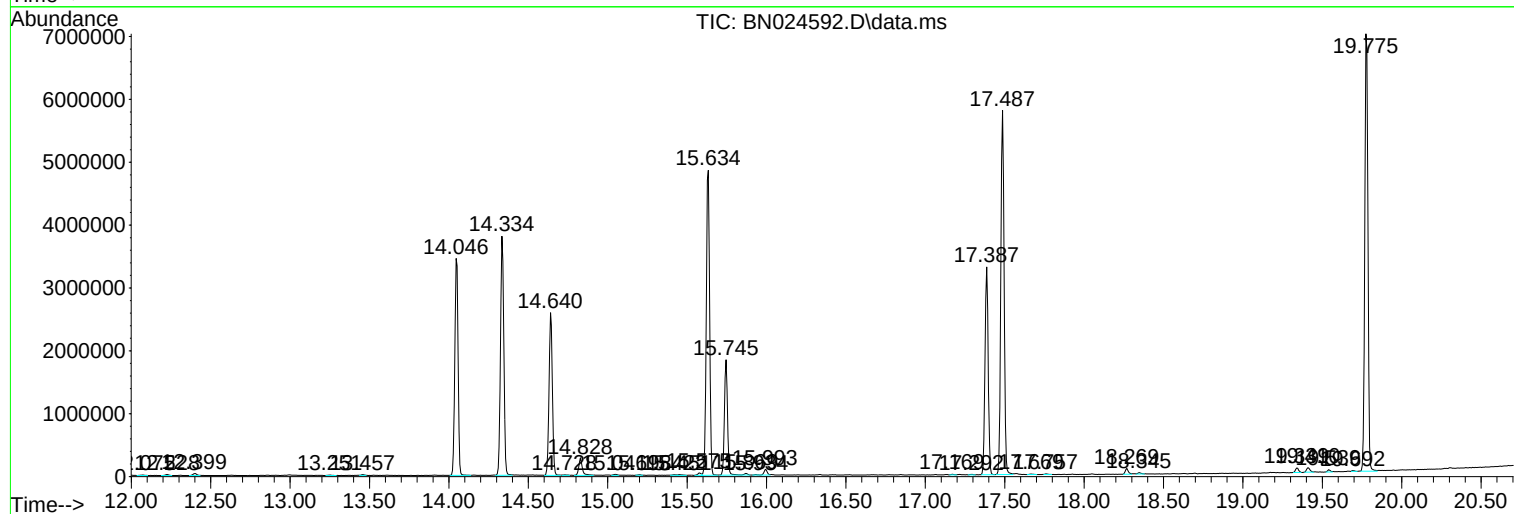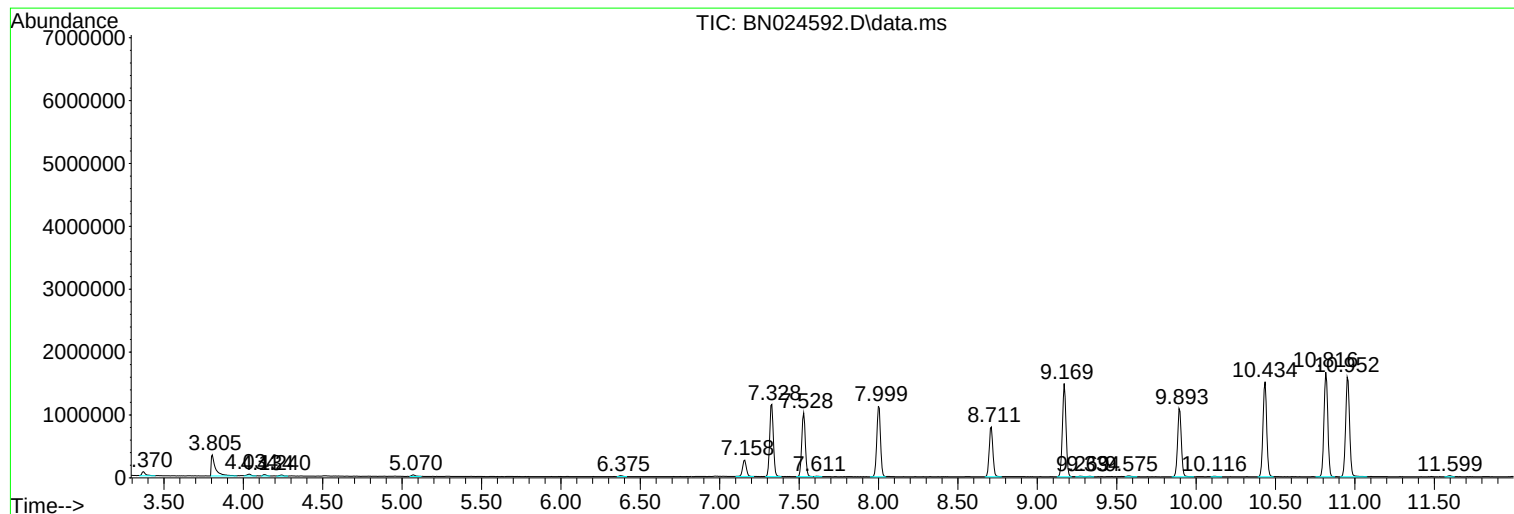

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024592.D
Acq On : 28 Mar 2023 19:24
Operator : CG/JU
Sample : 02086-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ76

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024592.D
Acq On : 28 Mar 2023 19:24
Operator : CG/JU
Sample : 02086-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ76

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc