

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024593.D
 Acq On : 28 Mar 2023 20:00
 Operator : CG/JU
 Sample : 02086-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	11	14	27	rVB	69382	127903	1.22%	0.148%
2	3.805	85	88	105	rBV	326087	594845	5.69%	0.689%
3	4.034	123	127	135	rVB	30536	48820	0.47%	0.057%
4	4.134	140	144	151	rVB	20512	33719	0.32%	0.039%
5	4.240	157	162	169	rVB5	18218	31488	0.30%	0.036%
6	4.511	204	208	216	rVB6	9936	17473	0.17%	0.020%
7	5.069	299	303	310	rVV	24272	38728	0.37%	0.045%
8	5.164	314	319	326	rVB2	16469	28019	0.27%	0.032%
9	5.281	334	339	343	rVB2	19119	29326	0.28%	0.034%
10	5.681	405	407	417	rVB10	5235	13143	0.13%	0.015%
11	6.375	521	525	534	rVB3	17669	30884	0.30%	0.036%
12	7.158	647	658	666	rBV2	291995	526671	5.03%	0.610%
13	7.328	678	687	699	rBV	1231264	1975000	18.88%	2.288%
14	7.422	699	703	708	rVB4	11316	18219	0.17%	0.021%
15	7.528	713	721	731	rVV	1114585	1775088	16.97%	2.057%
16	7.616	731	736	741	rVB2	8262	14803	0.14%	0.017%
17	7.999	794	801	810	rBV	1061840	1753424	16.76%	2.031%
18	8.710	914	922	930	rBV	843246	1342234	12.83%	1.555%
19	9.169	991	1000	1011	rBV	1509702	2438796	23.31%	2.825%
20	9.269	1011	1017	1024	rVV6	10604	21789	0.21%	0.025%
21	9.328	1024	1027	1033	rVB7	7282	11468	0.11%	0.013%
22	9.575	1066	1069	1076	rVB4	11414	23886	0.23%	0.028%
23	9.893	1116	1123	1137	rBV	1112514	1866161	17.84%	2.162%
24	10.434	1207	1215	1227	rBV	1600621	2573988	24.61%	2.982%
25	10.816	1272	1280	1287	rBV	1549137	2605540	24.91%	3.019%
26	10.869	1287	1289	1295	rVB	22310	30506	0.29%	0.035%
27	10.952	1295	1303	1318	rBV	1510524	2610301	24.95%	3.024%
28	11.599	1407	1413	1417	rBV3	15819	29353	0.28%	0.034%
29	12.222	1515	1519	1524	rBV2	10251	13572	0.13%	0.016%
30	12.398	1544	1549	1555	rBV	31080	50079	0.48%	0.058%
31	12.987	1642	1649	1655	rBV9	6954	18644	0.18%	0.022%
32	13.457	1725	1729	1733	rVB4	9599	13835	0.13%	0.016%
33	13.528	1737	1741	1748	rVB	27839	46988	0.45%	0.054%
34	14.045	1822	1829	1838	rBV	3311734	4529155	43.30%	5.247%
35	14.334	1871	1878	1889	rBV	3648722	5271773	50.40%	6.108%
36	14.640	1923	1930	1938	rBV	2402621	3529790	33.74%	4.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024593.D
 Acq On : 28 Mar 2023 20:00
 Operator : CG/JU
 Sample : 02086-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

37	14.828	1954	1962	1971	rBV	253714	398148	3.81%	0.461%
38	14.916	1973	1977	1983	rVB4	13903	22591	0.22%	0.026%
39	15.045	1995	1999	2006	rVB8	11004	19131	0.18%	0.022%
40	15.634	2091	2099	2110	rBV	4612315	6684541	63.90%	7.744%
41	15.745	2111	2118	2129	rBV	1753838	2279210	21.79%	2.641%
42	15.869	2134	2139	2145	rVB2	23542	38788	0.37%	0.045%
43	15.992	2155	2160	2164	rBV	65659	87311	0.83%	0.101%
44	16.416	2228	2232	2236	rBV6	6780	11947	0.11%	0.014%
45	17.386	2390	2397	2404	rBV	3142413	4330105	41.39%	5.017%
46	17.486	2407	2414	2427	rBV	5420737	7690154	73.52%	8.909%
47	18.269	2542	2547	2553	rBV3	70466	105695	1.01%	0.122%
48	18.345	2557	2560	2568	rVB	22640	32533	0.31%	0.038%
49	19.339	2725	2729	2735	rBV2	67659	95148	0.91%	0.110%
50	19.410	2736	2741	2747	rBV	71659	118327	1.13%	0.137%
51	19.539	2760	2763	2767	rBV2	30814	37063	0.35%	0.043%
52	19.692	2787	2789	2792	rVB3	13024	10828	0.10%	0.013%
53	19.775	2797	2803	2814	rBV	6823298	9256160	88.49%	10.724%
54	21.269	3054	3057	3063	rBV4	105530	146872	1.40%	0.170%
55	21.574	3104	3109	3116	rBV	3805265	4917578	47.01%	5.697%
56	23.910	3499	3506	3521	rBV2	4911956	10460496	100.00%	12.119%
57	24.063	3525	3532	3545	rVB2	2688866	5487831	52.46%	6.358%




Sum of corrected areas: 86315868

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024593.D
Acq On : 28 Mar 2023 20:00
Operator : CG/JU
Sample : 02086-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

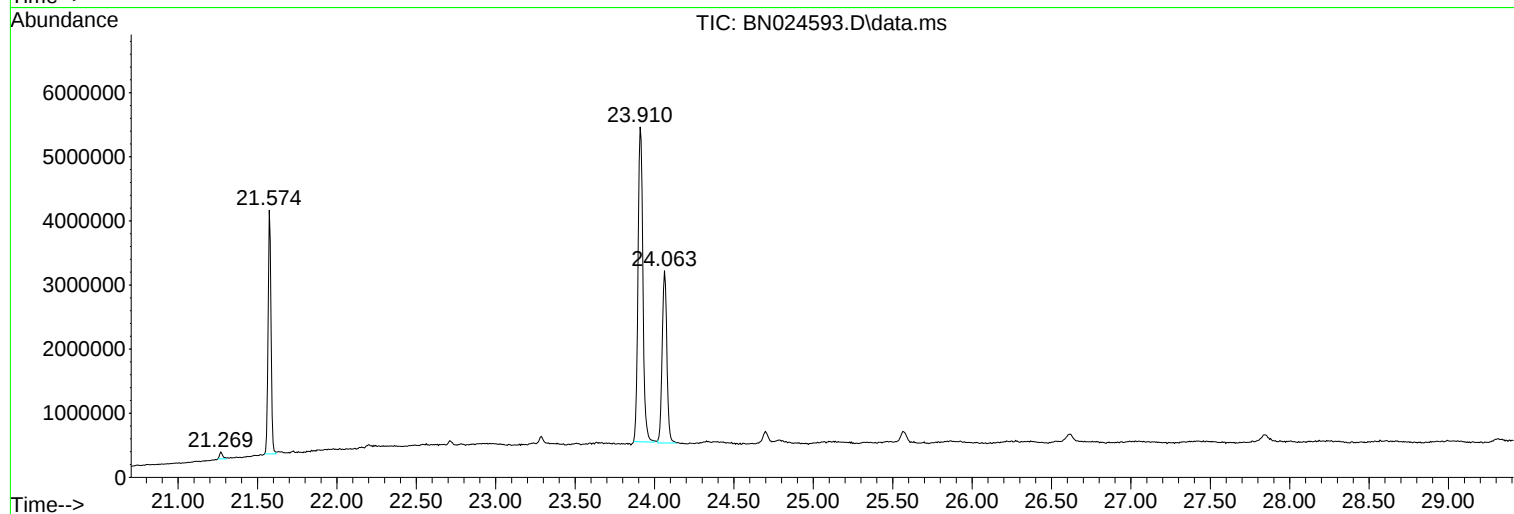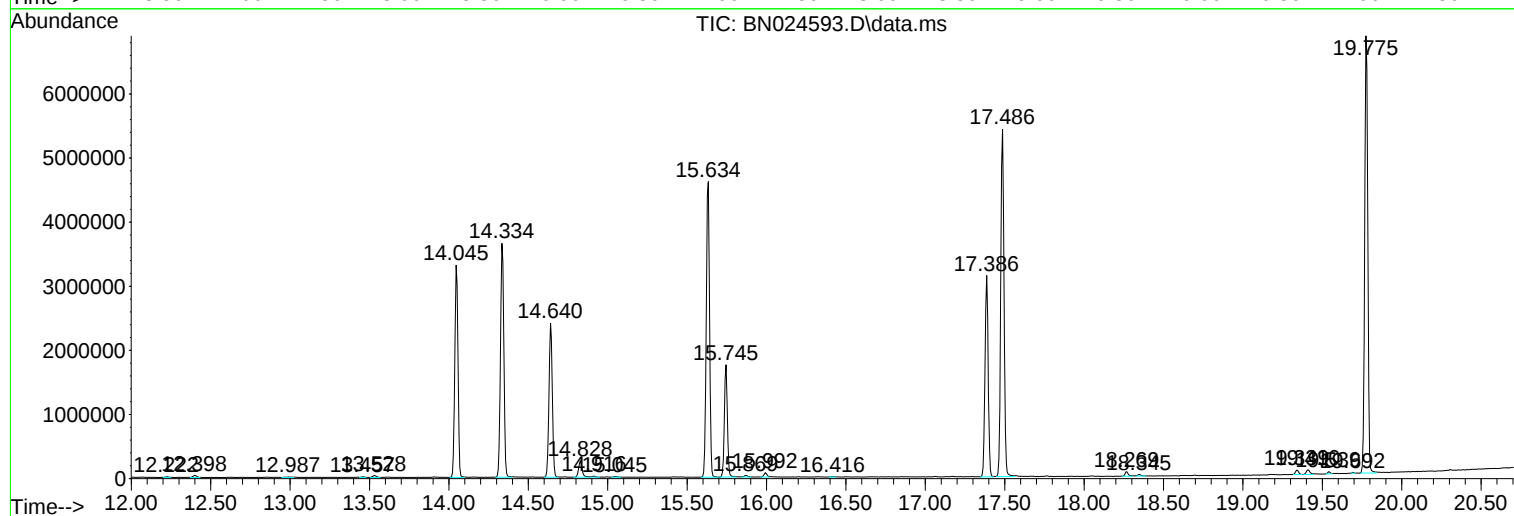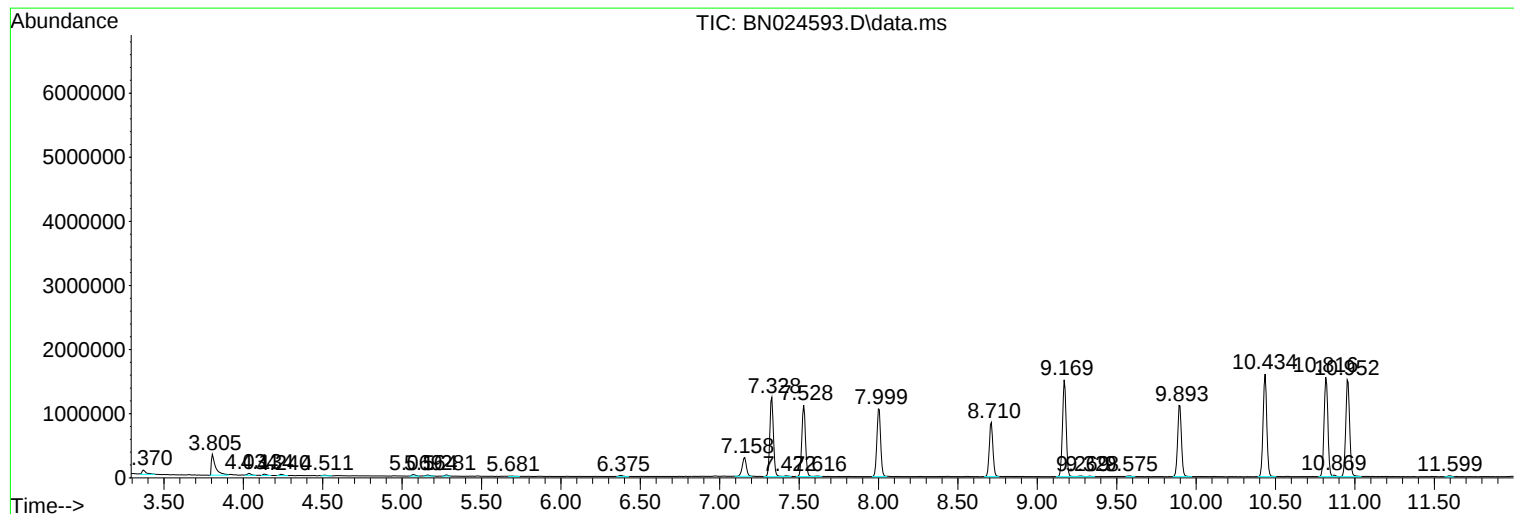

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024593.D
Acq On : 28 Mar 2023 20:00
Operator : CG/JU
Sample : 02086-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024593.D
Acq On : 28 Mar 2023 20:00
Operator : CG/JU
Sample : 02086-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
