

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024601.D
 Acq On : 29 Mar 2023 09:16
 Operator : CG/JU
 Sample : PB151624BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	28	rVB	121805	196966	1.74%	0.174%
2	3.799	83	87	114	rBV	1004558	1886086	16.70%	1.671%
3	4.128	139	143	148	rVB	21702	30675	0.27%	0.027%
4	5.246	328	333	340	rBV5	12004	22803	0.20%	0.020%
5	7.151	650	657	669	rBV	2062988	3214922	28.46%	2.848%
6	7.322	679	686	698	rVB	1635343	2542259	22.50%	2.252%
7	7.522	712	720	728	rBV	1941292	3085115	27.31%	2.733%
8	7.998	793	801	808	rBV	1242430	2058782	18.22%	1.824%
9	8.704	913	921	937	rBV	2431509	3864429	34.21%	3.424%
10	9.169	991	1000	1011	rBV	1880989	3134048	27.74%	2.777%
11	9.892	1114	1123	1133	rBV	1600746	2596047	22.98%	2.300%
12	10.428	1207	1214	1227	rBV	2317903	3763280	33.31%	3.334%
13	10.816	1272	1280	1288	rBV	1834396	3124168	27.65%	2.768%
14	10.951	1293	1303	1315	rBV	1673247	2849059	25.22%	2.524%
15	11.598	1407	1413	1418	rBV8	7682	14155	0.13%	0.013%
16	12.398	1542	1549	1556	rVB2	41523	69024	0.61%	0.061%
17	12.986	1642	1649	1654	rBV5	10895	24219	0.21%	0.021%
18	13.528	1737	1741	1745	rBV3	12292	18452	0.16%	0.016%
19	13.898	1798	1804	1811	rBV4	9206	17820	0.16%	0.016%
20	14.045	1822	1829	1840	rBV	4238632	5843858	51.73%	5.177%
21	14.333	1871	1878	1887	rBV	4832553	6817099	60.34%	6.039%
22	14.639	1922	1930	1939	rBV	2959069	4247695	37.60%	3.763%
23	14.728	1942	1945	1951	rVB6	9152	14394	0.13%	0.013%
24	14.828	1955	1962	1979	rBV	2450716	3461793	30.64%	3.067%
25	14.992	1987	1990	1995	rVV6	7924	13413	0.12%	0.012%
26	15.045	1995	1999	2004	rVB7	9901	16061	0.14%	0.014%
27	15.404	2057	2060	2067	rBV4	8620	15735	0.14%	0.014%
28	15.633	2088	2099	2111	rBV	5828662	8560889	75.78%	7.584%
29	15.745	2111	2118	2133	rVV	2374727	3124332	27.66%	2.768%
30	15.869	2134	2139	2145	rVB3	29278	49447	0.44%	0.044%
31	16.851	2301	2306	2311	rBV7	5664	12349	0.11%	0.011%
32	17.386	2390	2397	2407	rBV	3637434	5077184	44.94%	4.498%
33	17.486	2407	2414	2428	rBV	6633113	9523181	84.30%	8.437%
34	18.051	2504	2510	2515	rVB9	9770	17866	0.16%	0.016%
35	18.269	2543	2547	2552	rBV8	9852	14740	0.13%	0.013%
36	19.345	2725	2730	2734	rBV2	76703	116699	1.03%	0.103%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024601.D
Acq On : 29 Mar 2023 09:16
Operator : CG/JU
Sample : PB151624BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK624

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Title : SVOA CALIBRATION

37	19.410	2737	2741	2746	rVV	80006	102272	0.91%	0.091%
38	19.780	2797	2804	2814	rBV	7704887	10770808	95.34%	9.542%
39	21.580	3104	3110	3122	rBV	4034662	5439983	48.15%	4.819%
40	23.909	3499	3506	3520	rBV2	5623228	11297158	100.00%	10.008%
41	24.068	3526	3533	3546	rVB	2593126	5826560	51.58%	5.162%




Sum of corrected areas: 112875825

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024601.D
Acq On : 29 Mar 2023 09:16
Operator : CG/JU
Sample : PB151624BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

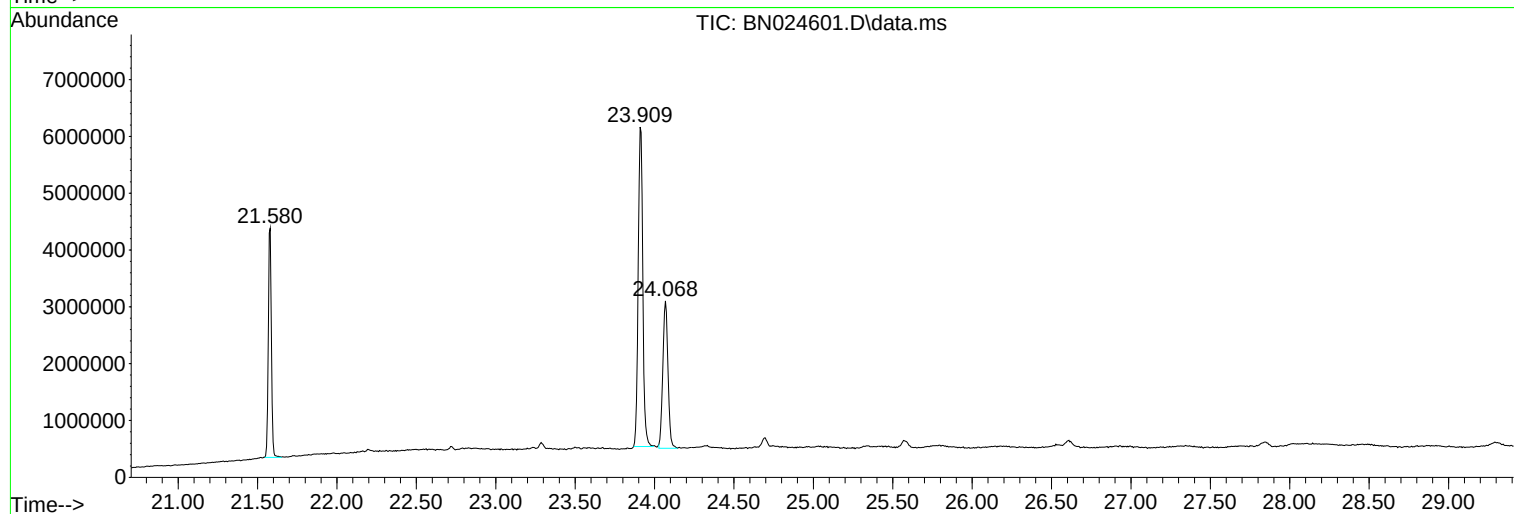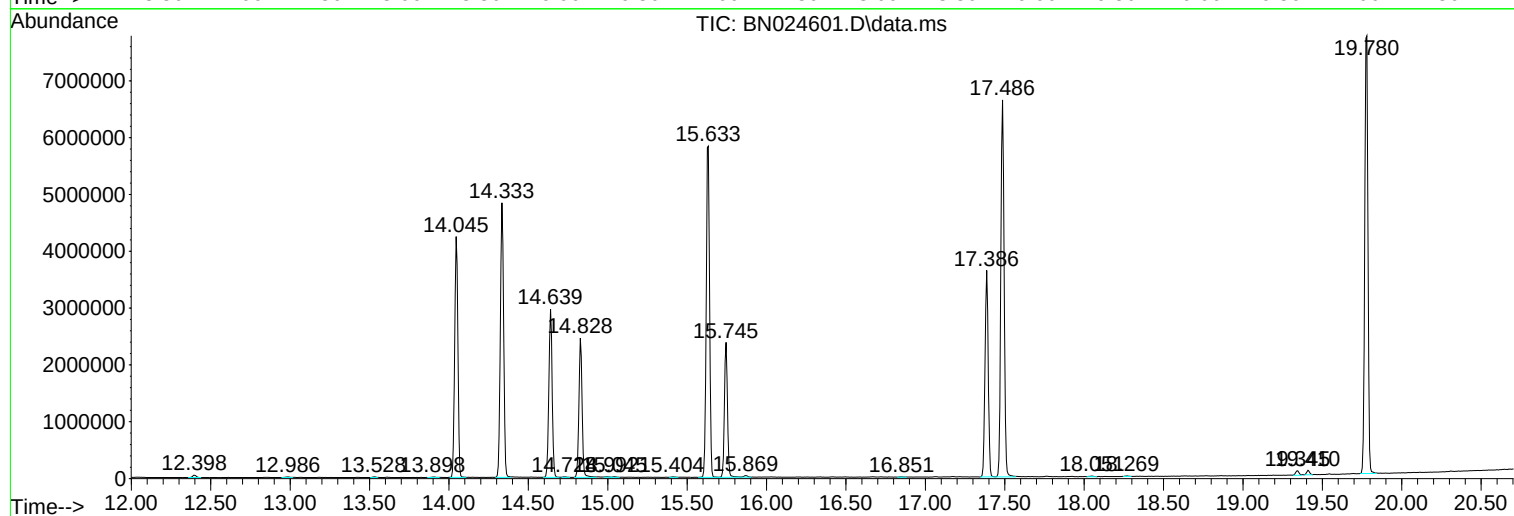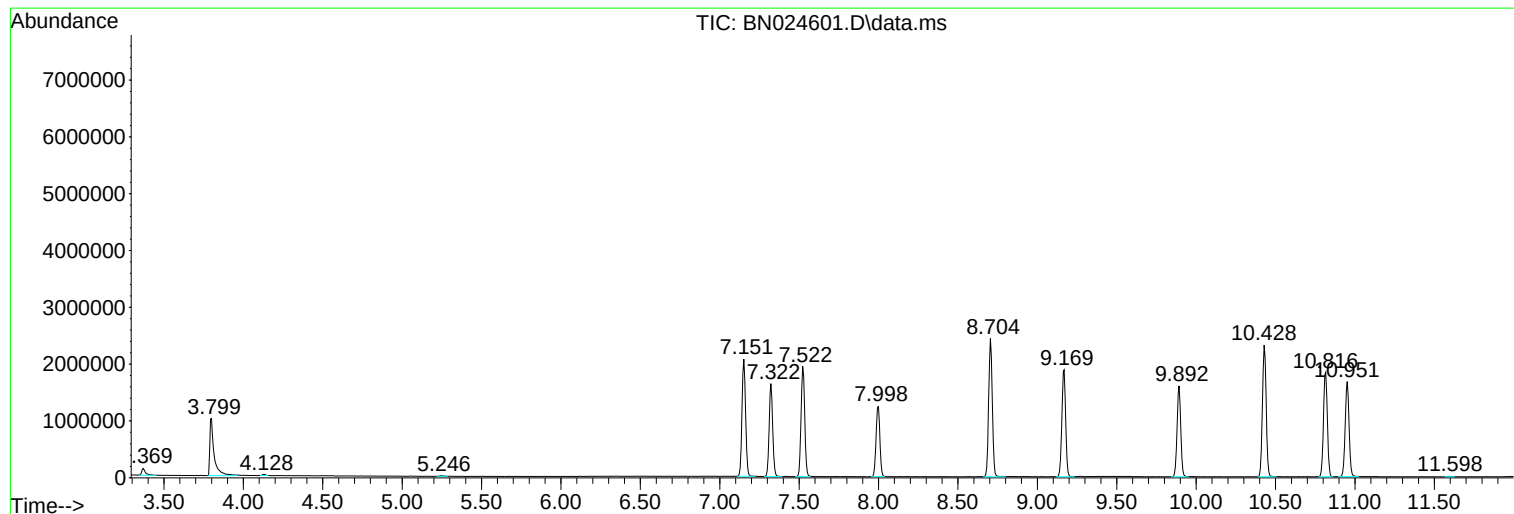

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024601.D
Acq On : 29 Mar 2023 09:16
Operator : CG/JU
Sample : PB151624BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024601.D
Acq On : 29 Mar 2023 09:16
Operator : CG/JU
Sample : PB151624BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc