

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024607.D
 Acq On : 29 Mar 2023 13:04
 Operator : CG/JU
 Sample : 01982-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EYGB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	27	rVB	74091	114141	1.89%	0.157%
2	3.669	63	65	71	rVB5	6331	8599	0.14%	0.012%
3	3.799	84	87	108	rBV	868651	1420888	23.51%	1.956%
4	4.034	124	127	131	rVB3	11477	15560	0.26%	0.021%
5	4.134	140	144	150	rVB	22446	34655	0.57%	0.048%
6	4.240	159	162	168	rVB6	8059	11833	0.20%	0.016%
7	5.069	299	303	309	rVB	27239	41640	0.69%	0.057%
8	7.158	650	658	670	rVB	1148747	1844848	30.53%	2.540%
9	7.328	680	687	696	rVB	900883	1437237	23.78%	1.979%
10	7.528	714	721	730	rBV	1120426	1767753	29.25%	2.434%
11	7.999	794	801	809	rBV	1217064	1909127	31.59%	2.628%
12	8.069	809	813	817	rVB6	6489	9044	0.15%	0.012%
13	8.705	914	921	931	rBV	1325641	2135773	35.34%	2.941%
14	9.169	992	1000	1007	rBV	1070131	1736432	28.73%	2.391%
15	9.328	1023	1027	1031	rVB6	8786	11128	0.18%	0.015%
16	9.581	1062	1070	1075	rVB2	15695	28241	0.47%	0.039%
17	9.893	1115	1123	1132	rBV	855987	1399215	23.15%	1.926%
18	10.434	1206	1215	1223	rBV	1281256	2157656	35.70%	2.971%
19	10.816	1271	1280	1289	rVB	1734472	2880942	47.67%	3.966%
20	10.951	1296	1303	1319	rVB	1354768	2275344	37.65%	3.133%
21	11.598	1409	1413	1418	rVB6	9356	13806	0.23%	0.019%
22	11.987	1473	1479	1481	rBV6	4449	8146	0.13%	0.011%
23	12.069	1488	1493	1500	rVB5	4807	9418	0.16%	0.013%
24	12.228	1515	1520	1527	rVB4	14246	26308	0.44%	0.036%
25	12.304	1530	1533	1539	rBV8	5673	11489	0.19%	0.016%
26	12.398	1543	1549	1556	rVB2	22856	37165	0.61%	0.051%
27	12.851	1622	1626	1631	rBV7	3714	6964	0.12%	0.010%
28	12.993	1646	1650	1654	rVV4	4417	7064	0.12%	0.010%
29	13.034	1654	1657	1662	rVB6	5110	7049	0.12%	0.010%
30	13.175	1676	1681	1690	rVB10	4097	10225	0.17%	0.014%
31	13.457	1720	1729	1734	rVB	23035	34574	0.57%	0.048%
32	13.534	1737	1742	1749	rBV7	7568	13345	0.22%	0.018%
33	13.604	1749	1754	1761	rVB9	6419	12445	0.21%	0.017%
34	13.904	1803	1805	1808	rBV3	6176	7046	0.12%	0.010%
35	14.045	1822	1829	1843	rBV	2347361	3142561	52.00%	4.327%
36	14.169	1843	1850	1853	rVB9	5322	10026	0.17%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024607.D
 Acq On : 29 Mar 2023 13:04
 Operator : CG/JU
 Sample : 01982-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EYGB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

37	14.334	1871	1878	1889	rBV2	2664192	3761791	62.25%	5.179%
38	14.528	1905	1911	1914	rVB8	8379	13807	0.23%	0.019%
39	14.639	1922	1930	1939	rBV	2656779	3914494	64.77%	5.389%
40	14.828	1955	1962	1979	rBV	1011482	1456794	24.11%	2.006%
41	14.934	1979	1980	1986	rVB6	5695	6850	0.11%	0.009%
42	15.051	1995	2000	2003	rVB6	17862	27407	0.45%	0.038%
43	15.416	2058	2062	2067	rBV8	7289	13034	0.22%	0.018%
44	15.628	2091	2098	2108	rBV	3398468	4838217	80.06%	6.661%
45	15.745	2112	2118	2130	rVV	824222	1120269	18.54%	1.542%
46	15.869	2135	2139	2145	rVV4	16627	25682	0.42%	0.035%
47	15.992	2155	2160	2164	rBV	41091	58141	0.96%	0.080%
48	16.028	2164	2166	2172	rVB6	6848	9870	0.16%	0.014%
49	16.339	2215	2219	2224	rBV7	5300	8992	0.15%	0.012%
50	16.410	2226	2231	2234	rBV7	5693	9413	0.16%	0.013%
51	16.669	2270	2275	2279	rBV8	6169	11677	0.19%	0.016%
52	16.775	2288	2293	2297	rBV7	5398	10472	0.17%	0.014%
53	17.057	2340	2341	2346	rVB5	6793	6340	0.10%	0.009%
54	17.133	2351	2354	2356	rBV4	7191	9038	0.15%	0.012%
55	17.169	2357	2360	2365	rVV3	7244	9447	0.16%	0.013%
56	17.386	2390	2397	2404	rBV	3273682	4615868	76.38%	6.355%
57	17.486	2407	2414	2426	rVV	3590990	5070995	83.91%	6.982%
58	17.575	2426	2429	2434	rVB4	35576	47207	0.78%	0.065%
59	17.763	2453	2461	2465	rBV9	10446	23942	0.40%	0.033%
60	18.269	2542	2547	2555	rBV	230591	326838	5.41%	0.450%
61	18.345	2558	2560	2565	rVB4	13148	19457	0.32%	0.027%
62	18.692	2617	2619	2624	rVB4	24665	28162	0.47%	0.039%
63	19.339	2725	2729	2734	rBV2	40981	58043	0.96%	0.080%
64	19.410	2736	2741	2749	rBV	55111	126665	2.10%	0.174%
65	19.539	2760	2763	2769	rBV3	55681	65559	1.08%	0.090%
66	19.775	2797	2803	2815	rVB	4439917	5810101	96.14%	7.999%
67	20.304	2891	2893	2897	rVB2	39389	39764	0.66%	0.055%
68	20.798	2975	2977	2981	rVB2	47923	46645	0.77%	0.064%
69	21.263	3052	3056	3064	rBV	377633	590479	9.77%	0.813%
70	21.569	3103	3108	3115	rBV	3604444	4832519	79.96%	6.653%
71	23.880	3494	3501	3519	rVB2	2832743	6043360	100.00%	8.320%
72	24.045	3522	3529	3542	rVB2	2362667	4977175	82.36%	6.853%




Sum of corrected areas: 72632201

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024607.D
Acq On : 29 Mar 2023 13:04
Operator : CG/JU
Sample : 01982-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYGB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

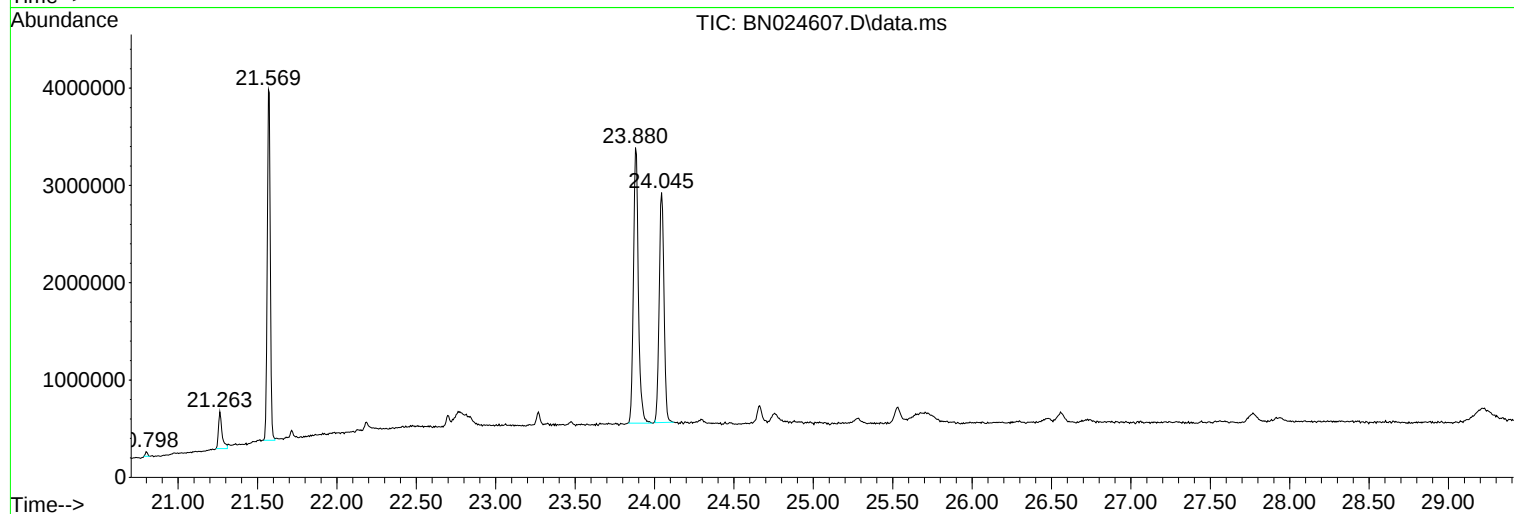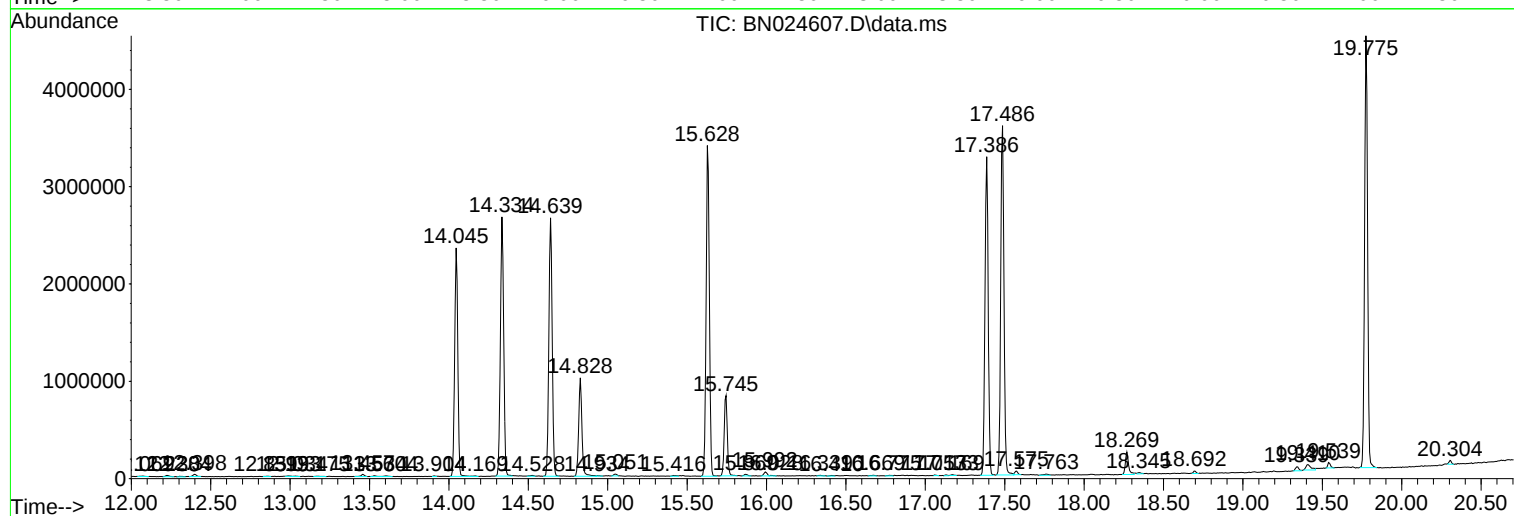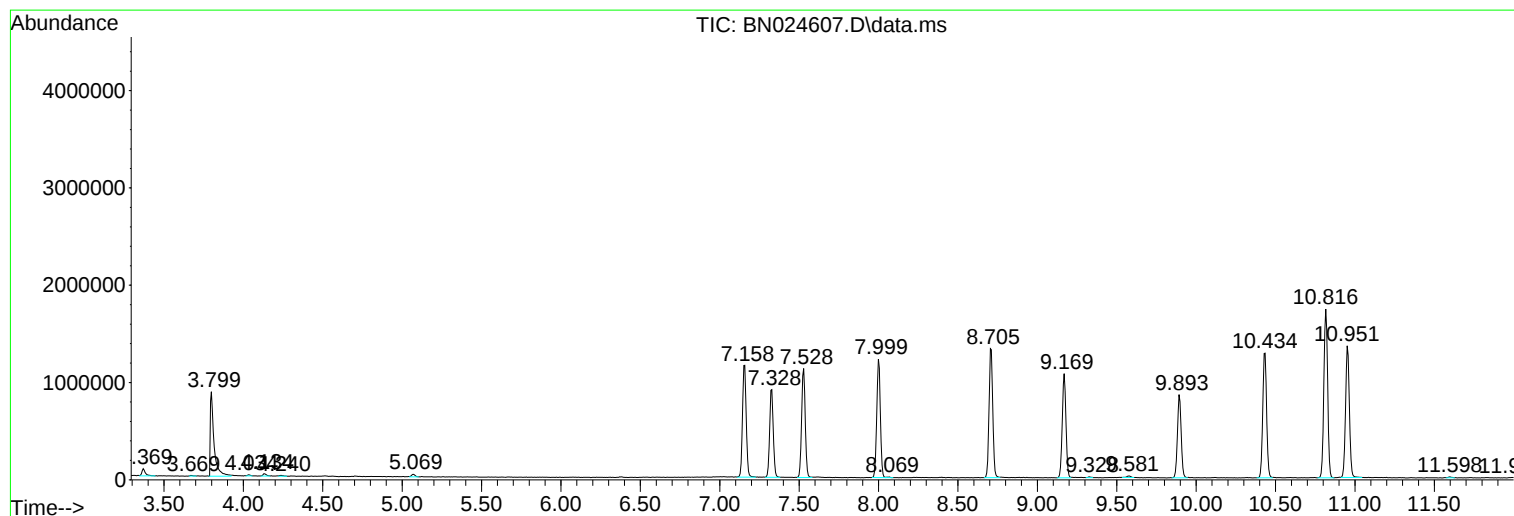

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024607.D
Acq On : 29 Mar 2023 13:04
Operator : CG/JU
Sample : 01982-06
Misc :
ALS Vial : 9 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
EYGB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.263	2.44 ng/ul	590479	Chrysene-d12		21.574	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	17-Pentatriacontene		491	C35H70	006971-40-0	91
2	1-Octadecene		252	C18H36	000112-88-9	91
3	Heneicosyl heptafluorobutyrate		508	C25H43F7O2	1000351-83-8	90
4	Octacosyl trifluoroacetate		506	C30H57F3O2	1000351-74-9	90
5	Tetracosyl trifluoroacetate		450	C26H49F3O2	1000351-76-4	90

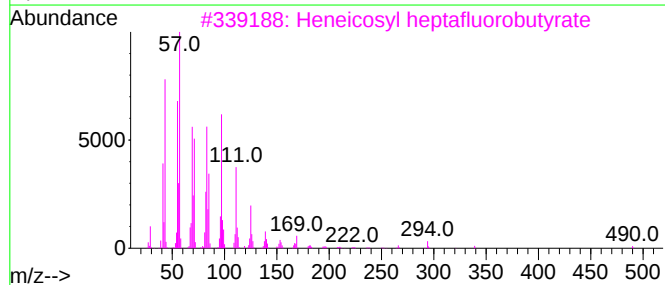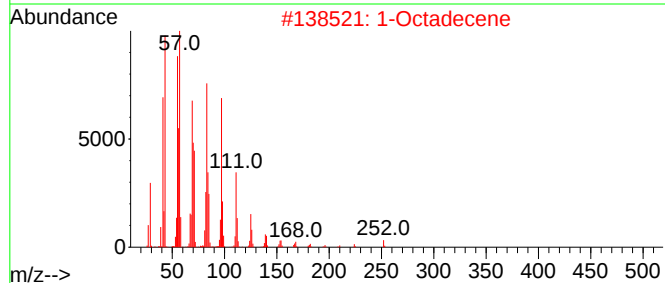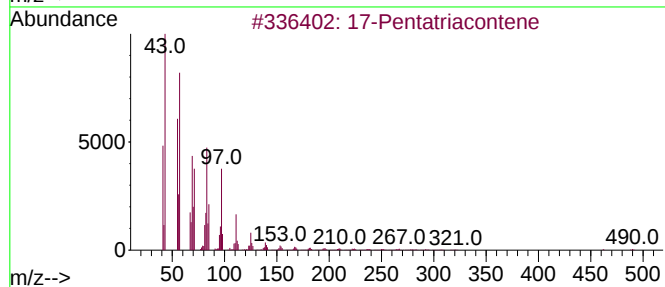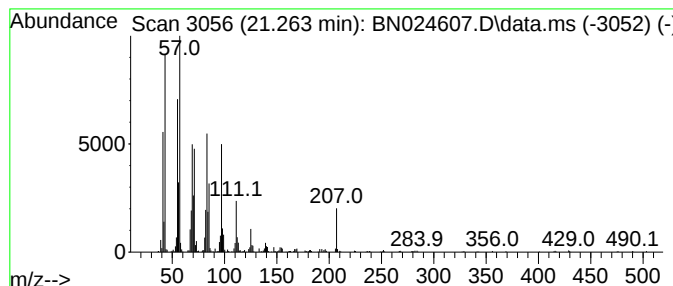

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024607.D
Acq On : 29 Mar 2023 13:04
Operator : CG/JU
Sample : 01982-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYGB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.263	2.4	ng/u1	590479	5	21.574	4832520	20.0