

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024608.D
 Acq On : 29 Mar 2023 13:40
 Operator : CG/JU
 Sample : 01982-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EYG98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	24	rVB	62055	96101	1.52%	0.135%
2	3.799	84	87	111	rBV	797489	1345403	21.23%	1.895%
3	4.128	139	143	148	rBV2	21454	31065	0.49%	0.044%
4	5.069	299	303	311	rVB	27087	42908	0.68%	0.060%
5	6.963	622	625	628	rBV5	4492	6767	0.11%	0.010%
6	7.152	648	657	669	rVB	1096195	1760151	27.77%	2.479%
7	7.322	678	686	697	rBV	861888	1378190	21.74%	1.941%
8	7.528	712	721	728	rBV	1045020	1672681	26.39%	2.356%
9	7.722	750	754	755	rBV4	5155	6690	0.11%	0.009%
10	7.757	756	760	764	rVB5	8685	13639	0.22%	0.019%
11	7.952	788	793	794	rBV5	5046	7031	0.11%	0.010%
12	7.999	794	801	809	rVV	1138870	1792710	28.28%	2.525%
13	8.075	809	814	821	rVB2	29163	56877	0.90%	0.080%
14	8.704	914	921	932	rBV	1296274	2072202	32.69%	2.919%
15	8.793	934	936	940	rVB5	6580	6537	0.10%	0.009%
16	9.169	991	1000	1008	rBV	1021340	1662846	26.23%	2.342%
17	9.328	1022	1027	1032	rVB8	11560	16690	0.26%	0.024%
18	9.575	1063	1069	1075	rVB3	18140	32570	0.51%	0.046%
19	9.893	1115	1123	1132	rBV	826697	1338870	21.12%	1.886%
20	10.322	1192	1196	1202	rVB9	5182	9083	0.14%	0.013%
21	10.434	1206	1215	1224	rBV	1238777	2060159	32.50%	2.902%
22	10.593	1236	1242	1247	rBV4	17183	33629	0.53%	0.047%
23	10.816	1270	1280	1289	rBV	1631432	2703450	42.65%	3.808%
24	10.951	1296	1303	1314	rVB	1309777	2172412	34.27%	3.060%
25	11.593	1405	1412	1417	rBV10	6203	11394	0.18%	0.016%
26	11.828	1447	1452	1458	rBV8	10860	22348	0.35%	0.031%
27	12.222	1514	1519	1524	rBV2	14575	23923	0.38%	0.034%
28	12.398	1543	1549	1555	rVB3	23042	36535	0.58%	0.051%
29	13.175	1677	1681	1689	rBV10	5526	8940	0.14%	0.013%
30	13.457	1725	1729	1736	rVB2	23103	30824	0.49%	0.043%
31	13.528	1736	1741	1747	rBV	16736	26037	0.41%	0.037%
32	13.904	1802	1805	1812	rBV8	4267	7875	0.12%	0.011%
33	14.045	1822	1829	1835	rBV	2233044	3000850	47.34%	4.227%
34	14.157	1845	1848	1853	rVB6	5078	7074	0.11%	0.010%
35	14.334	1871	1878	1887	rBV	2468173	3560740	56.17%	5.016%
36	14.528	1906	1911	1914	rVB6	9349	10968	0.17%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024608.D
 Acq On : 29 Mar 2023 13:40
 Operator : CG/JU
 Sample : 01982-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EYG98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

37	14.639	1921	1930	1941	rBV	2502609	3652421	57.62%	5.145%
38	14.828	1953	1962	1982	rBV	1048095	1483230	23.40%	2.089%
39	15.045	1994	1999	2006	rVB7	22381	38633	0.61%	0.054%
40	15.416	2056	2062	2063	rBV5	5873	8163	0.13%	0.011%
41	15.628	2091	2098	2109	rBV	3296926	4631067	73.06%	6.524%
42	15.745	2112	2118	2130	rVB	797733	1097036	17.31%	1.545%
43	15.869	2135	2139	2144	rVB4	16415	26159	0.41%	0.037%
44	15.992	2155	2160	2164	rBV	42427	60625	0.96%	0.085%
45	16.028	2164	2166	2173	rVB6	6133	11880	0.19%	0.017%
46	16.334	2213	2218	2224	rBV9	8182	18176	0.29%	0.026%
47	16.775	2289	2293	2294	rBV3	6862	7474	0.12%	0.011%
48	16.845	2302	2305	2307	rBV4	5743	6768	0.11%	0.010%
49	17.169	2357	2360	2364	rVV4	7986	11217	0.18%	0.016%
50	17.275	2374	2378	2379	rBV4	5250	7010	0.11%	0.010%
51	17.386	2390	2397	2404	rBV	3054839	4355801	68.72%	6.136%
52	17.486	2407	2414	2425	rVV	3458180	4912274	77.50%	6.920%
53	17.569	2425	2428	2438	rVB5	37630	62286	0.98%	0.088%
54	18.045	2507	2509	2513	rVB5	6412	8071	0.13%	0.011%
55	18.269	2542	2547	2555	rBV	245404	346169	5.46%	0.488%
56	18.692	2616	2619	2624	rBV3	22916	26510	0.42%	0.037%
57	19.339	2725	2729	2734	rVB2	40202	52819	0.83%	0.074%
58	19.410	2736	2741	2746	rBV2	53752	106232	1.68%	0.150%
59	19.539	2760	2763	2768	rBV3	53313	68230	1.08%	0.096%
60	19.774	2797	2803	2813	rBV2	4367451	5794020	91.41%	8.162%
61	20.304	2890	2893	2896	rBV2	36638	36173	0.57%	0.051%
62	20.804	2975	2978	2981	rVB2	50537	54303	0.86%	0.076%
63	21.263	3052	3056	3065	rBV2	404401	666492	10.51%	0.939%
64	21.574	3104	3109	3116	rVB	3601501	4740006	74.78%	6.677%
65	21.716	3131	3133	3139	rVB2	87226	102053	1.61%	0.144%
66	23.892	3495	3503	3517	rBV2	2842835	6338730	100.00%	8.929%
67	24.051	3523	3530	3540	rVB2	2593166	5193700	81.94%	7.316%




Sum of corrected areas: 70989897

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024608.D
Acq On : 29 Mar 2023 13:40
Operator : CG/JU
Sample : 01982-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYG98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

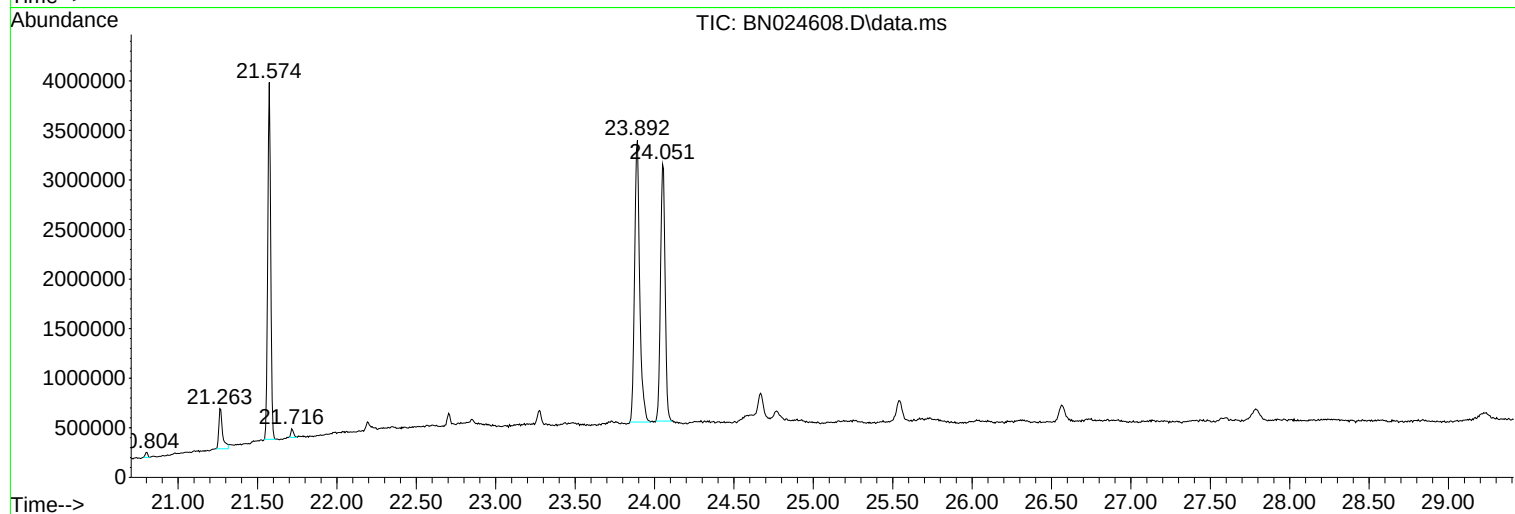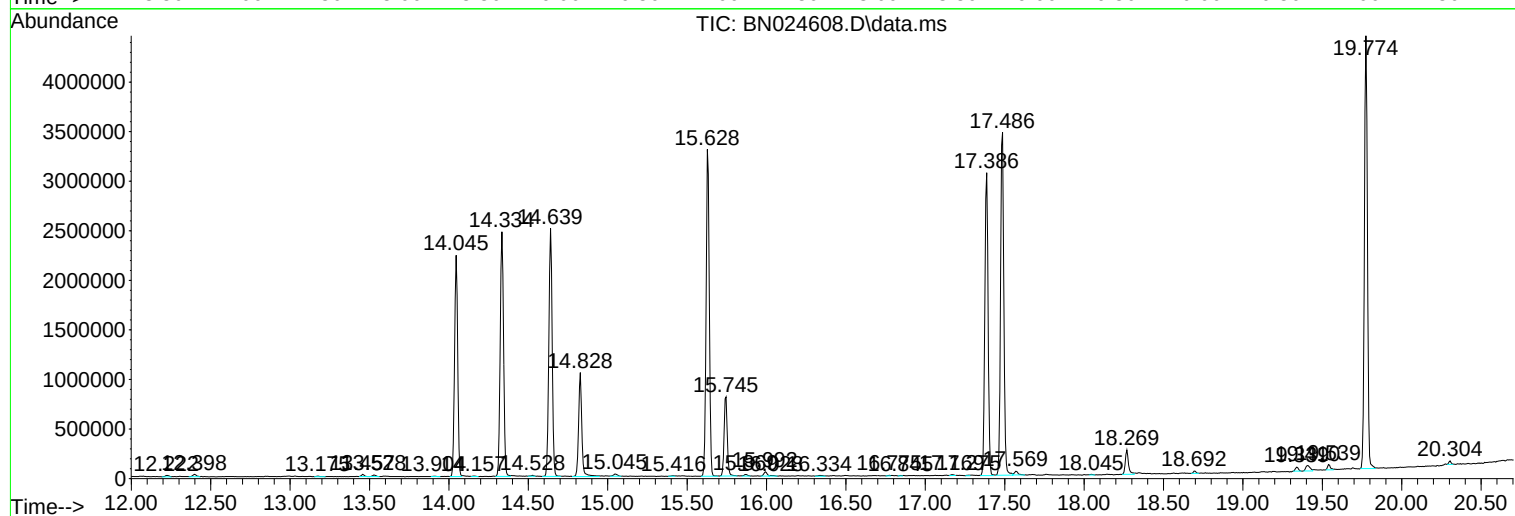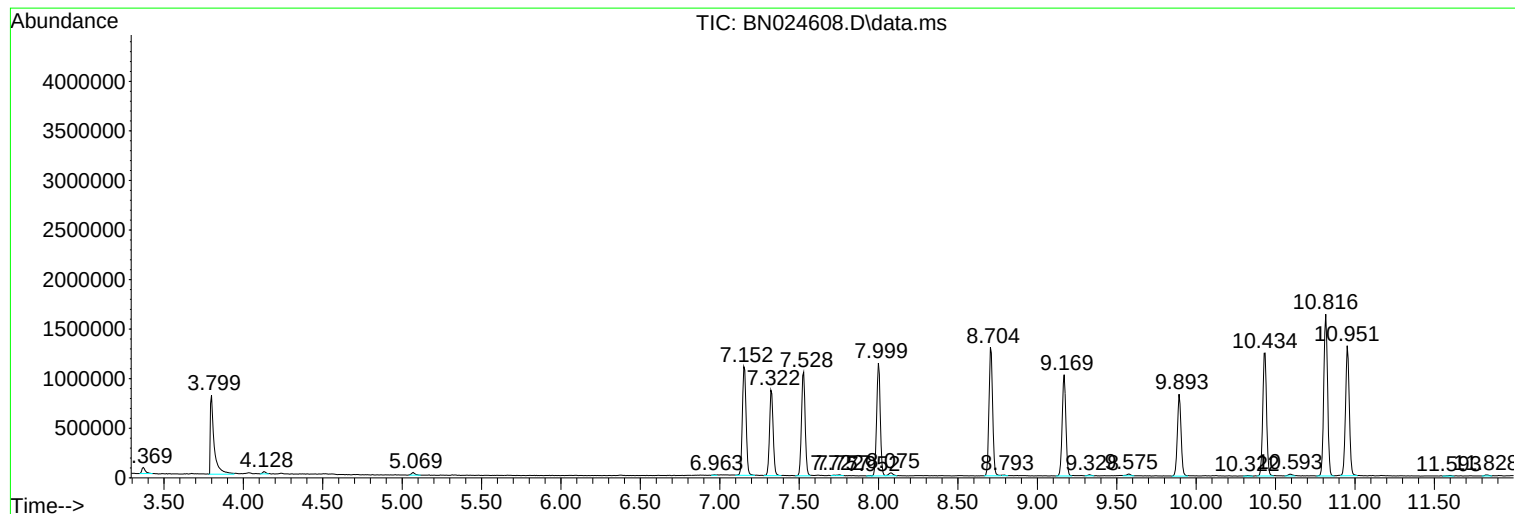

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024608.D
Acq On : 29 Mar 2023 13:40
Operator : CG/JU
Sample : 01982-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYG98










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Nonadecyl pentafluoropropio... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.263	2.81 ng/ul	666492	Chrysene-d12	21.574

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	91
2			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	91
3			17-Pentatriacontene	491	C35H70	006971-40-0	91
4			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91
5			1-Tricosene	322	C23H46	018835-32-0	91

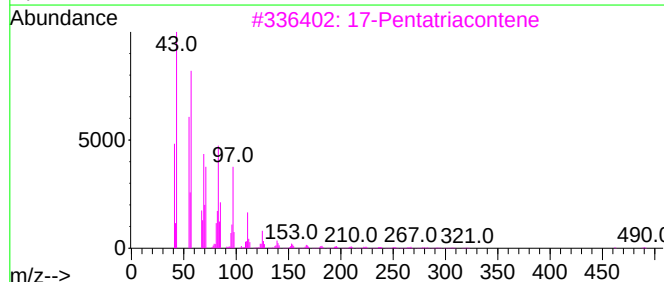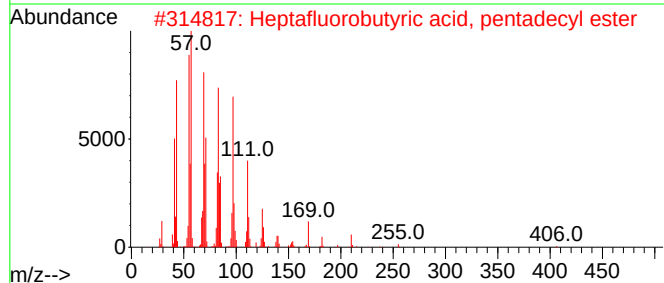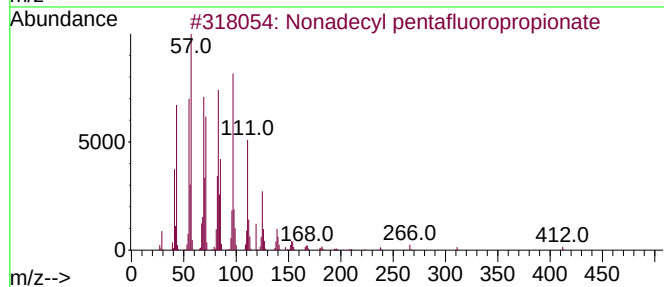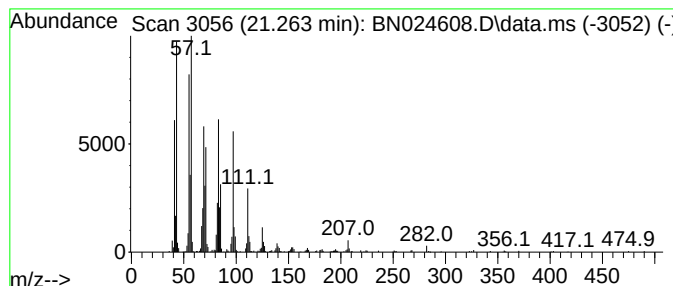

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024608.D
Acq On : 29 Mar 2023 13:40
Operator : CG/JU
Sample : 01982-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYG98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Nonadecyl penta...	21.263	2.8	ng/u1	666492	5	21.574	4740010	20.0