

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024615.D
 Acq On : 29 Mar 2023 18:32
 Operator : CG/JU
 Sample : PB151642BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	24	rVB	109850	155516	1.67%	0.155%
2	3.799	84	87	104	rBV	922650	1471392	15.80%	1.468%
3	4.134	139	144	148	rBV	29217	43305	0.47%	0.043%
4	5.246	328	333	341	rVB8	13050	31378	0.34%	0.031%
5	7.157	650	658	668	rBV	1729636	2776551	29.82%	2.771%
6	7.328	679	687	699	rVB	1351540	2155311	23.15%	2.151%
7	7.528	714	721	730	rBV	1666614	2637618	28.33%	2.632%
8	7.998	793	801	813	rBV	1357170	2161181	23.21%	2.157%
9	8.710	913	922	935	rBV	2025051	3312256	35.57%	3.305%
10	9.169	992	1000	1012	rBV	1654883	2662778	28.60%	2.657%
11	9.892	1112	1123	1131	rBV	1361821	2206613	23.70%	2.202%
12	10.434	1206	1215	1224	rBV	1945292	3258111	34.99%	3.251%
13	10.816	1271	1280	1289	rBV	1996583	3274014	35.16%	3.267%
14	10.951	1294	1303	1315	rBV	1653336	2785669	29.92%	2.780%
15	11.604	1406	1414	1416	rBV7	8504	14916	0.16%	0.015%
16	12.398	1540	1549	1555	rBV3	36532	60513	0.65%	0.060%
17	12.986	1645	1649	1653	rBV7	6028	10930	0.12%	0.011%
18	13.533	1736	1742	1748	rVB7	8104	15365	0.17%	0.015%
19	14.045	1822	1829	1839	rBV	3586180	4876661	52.37%	4.867%
20	14.333	1870	1878	1890	rBV2	3979209	5788199	62.16%	5.776%
21	14.639	1922	1930	1940	rBV	3087731	4433026	47.61%	4.424%
22	14.827	1954	1962	1975	rBV	2128107	2881143	30.94%	2.875%
23	14.992	1987	1990	1995	rVB5	7333	10241	0.11%	0.010%
24	15.045	1995	1999	2004	rVB6	5976	10544	0.11%	0.011%
25	15.633	2090	2099	2107	rBV	4947379	7286485	78.26%	7.271%
26	15.745	2110	2118	2130	rBV	1897603	2506277	26.92%	2.501%
27	15.869	2135	2139	2145	rVB2	24935	42204	0.45%	0.042%
28	17.169	2356	2360	2363	rBV4	6510	10309	0.11%	0.010%
29	17.386	2389	2397	2406	rBV	3702097	5287010	56.78%	5.276%
30	17.486	2407	2414	2430	rBV2	5590508	7909150	84.94%	7.893%
31	17.769	2458	2462	2466	rVB5	8597	13934	0.15%	0.014%
32	18.045	2506	2509	2516	rBV9	11393	17254	0.19%	0.017%
33	19.339	2725	2729	2734	rBV2	64380	88651	0.95%	0.088%
34	19.410	2737	2741	2745	rVV2	60740	78889	0.85%	0.079%
35	19.774	2797	2803	2815	rBV	6846206	9194718	98.75%	9.176%
36	21.574	3104	3109	3117	rBV2	4309243	5576144	59.89%	5.565%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024615.D
Acq On : 29 Mar 2023 18:32
Operator : CG/JU
Sample : PB151642BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK642

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Title : SVOA CALIBRATION

37	23.909	3499	3506	3520	rBV	4653148	9311104	100.00%	9.292%
38	24.062	3525	3532	3543	rVB2	2856691	5852719	62.86%	5.841%




Sum of corrected areas: 100208079

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024615.D
Acq On : 29 Mar 2023 18:32
Operator : CG/JU
Sample : PB151642BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK642

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

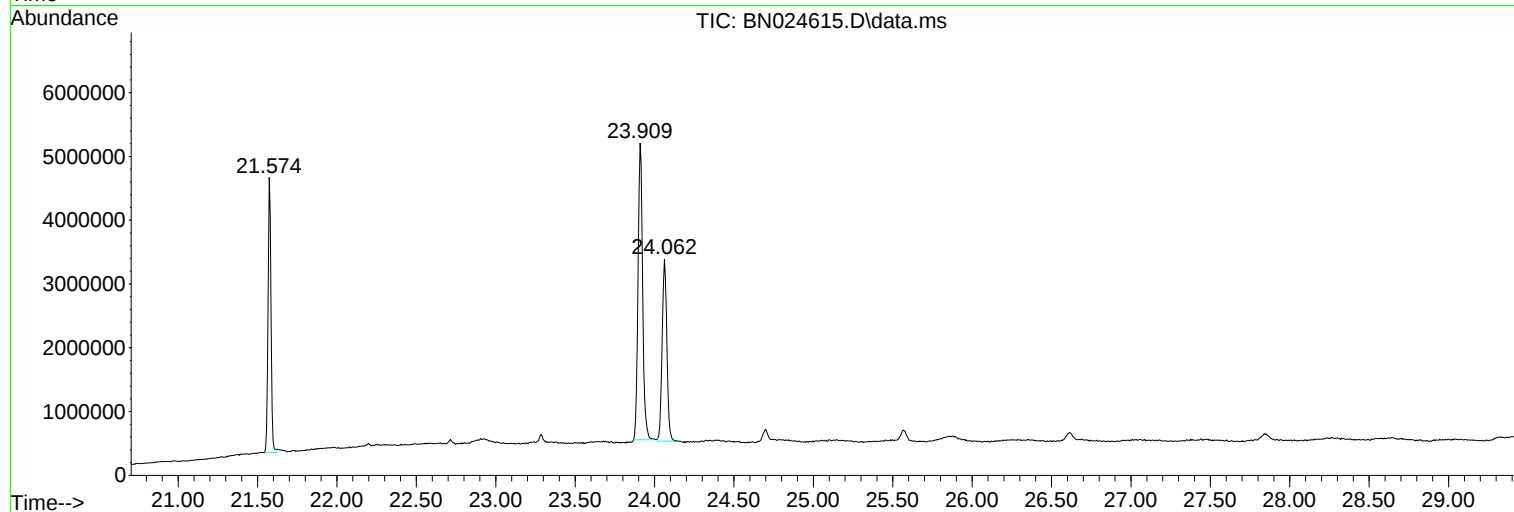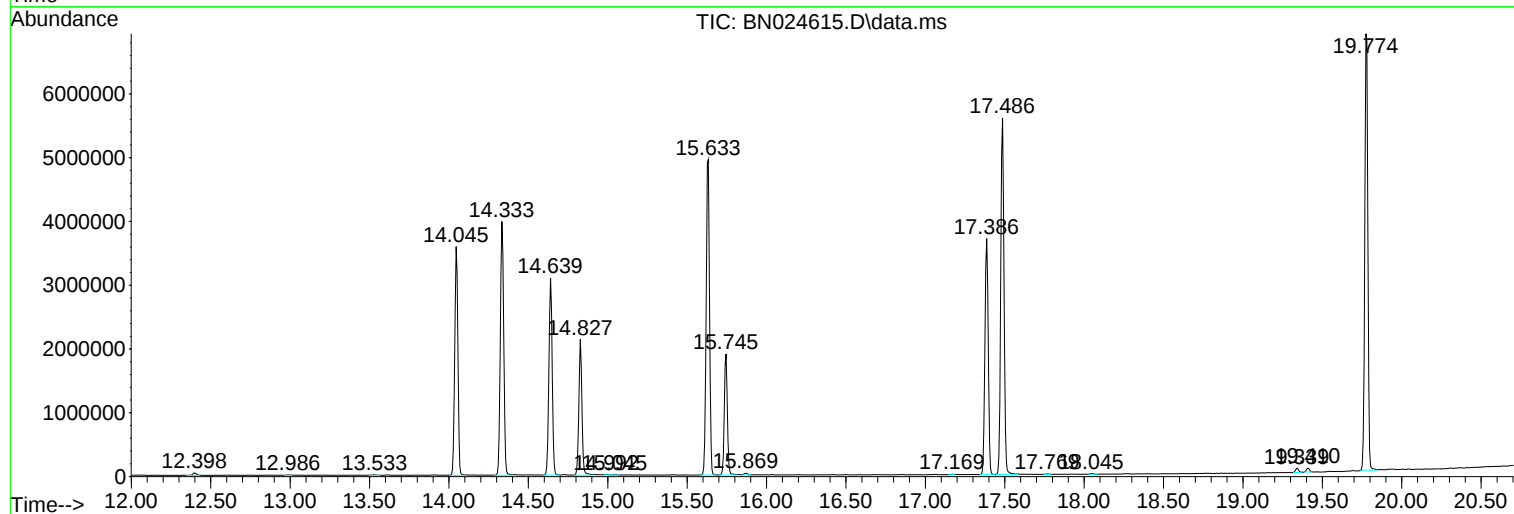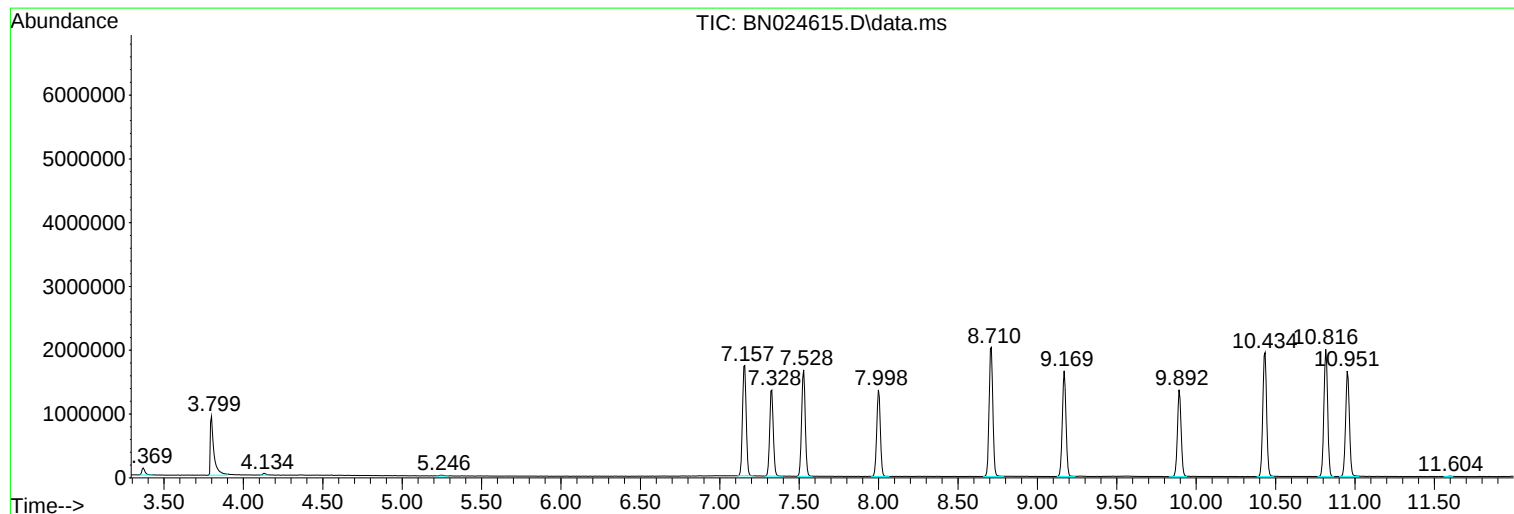

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024615.D
Acq On : 29 Mar 2023 18:32
Operator : CG/JU
Sample : PB151642BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK642

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024615.D
Acq On : 29 Mar 2023 18:32
Operator : CG/JU
Sample : PB151642BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK642

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc