

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024623.D
 Acq On : 29 Mar 2023 23:24
 Operator : CG/JU
 Sample : 02085-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	19	rBV	72911	98422	1.01%	0.111%
2	3.805	86	88	109	rBV	218541	371630	3.80%	0.418%
3	4.034	122	127	133	rVB2	29306	52372	0.54%	0.059%
4	4.128	140	143	151	rVB	28884	46142	0.47%	0.052%
5	4.240	158	162	167	rVB2	19460	29290	0.30%	0.033%
6	4.517	205	209	214	rVB7	6850	11264	0.12%	0.013%
7	5.070	299	303	308	rVB	22870	35437	0.36%	0.040%
8	6.375	520	525	530	rVB2	18098	30172	0.31%	0.034%
9	7.152	649	657	665	rVB	309494	493138	5.05%	0.555%
10	7.322	678	686	696	rBV	1196095	1884946	19.28%	2.121%
11	7.528	714	721	731	rBV	1098789	1778065	18.19%	2.000%
12	7.611	731	735	739	rVB6	8615	11435	0.12%	0.013%
13	7.999	792	801	808	rBV	1228404	1952197	19.97%	2.196%
14	8.605	901	904	907	rBV4	7224	10908	0.11%	0.012%
15	8.705	912	921	930	rBV	873834	1387539	14.20%	1.561%
16	9.169	992	1000	1010	rBV	1469956	2379829	24.35%	2.677%
17	9.575	1063	1069	1075	rBV2	35017	62766	0.64%	0.071%
18	9.893	1114	1123	1134	rBV	1158262	1882095	19.25%	2.117%
19	10.428	1206	1214	1223	rBV	1611343	2622832	26.83%	2.951%
20	10.681	1251	1257	1262	rVB9	7668	15348	0.16%	0.017%
21	10.816	1270	1280	1287	rBV	1757070	2959411	30.28%	3.329%
22	10.952	1295	1303	1319	rBV	1158581	1949975	19.95%	2.194%
23	11.593	1406	1412	1418	rBV10	7053	17849	0.18%	0.020%
24	11.728	1427	1435	1438	rBV10	6170	11967	0.12%	0.013%
25	11.828	1448	1452	1456	rVB6	6464	10317	0.11%	0.012%
26	12.069	1486	1493	1499	rBV2	24160	43372	0.44%	0.049%
27	12.222	1514	1519	1524	rBV	32636	44218	0.45%	0.050%
28	12.399	1543	1549	1554	rBV2	32841	55251	0.57%	0.062%
29	12.851	1619	1626	1630	rBV9	8295	16451	0.17%	0.019%
30	12.993	1646	1650	1654	rBV7	6720	10652	0.11%	0.012%
31	13.028	1654	1656	1664	rVB8	5868	11933	0.12%	0.013%
32	13.246	1687	1693	1700	rVB10	6351	17239	0.18%	0.019%
33	13.457	1720	1729	1735	rVV3	40826	67056	0.69%	0.075%
34	13.528	1735	1741	1748	rVB	39436	65068	0.67%	0.073%
35	14.046	1822	1829	1839	rBV	3436498	4580078	46.86%	5.153%
36	14.334	1871	1878	1890	rBV	3708207	5319253	54.42%	5.984%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024623.D
 Acq On : 29 Mar 2023 23:24
 Operator : CG/JU
 Sample : 02085-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

37	14.522	1908	1910	1913	rVB4	10011	11265	0.12%	0.013%
38	14.640	1922	1930	1941	rBV	2791513	4009908	41.02%	4.511%
39	14.722	1941	1944	1951	rVB8	6982	10984	0.11%	0.012%
40	14.828	1955	1962	1973	rBV	285963	462490	4.73%	0.520%
41	15.045	1995	1999	2010	rVB10	16603	35015	0.36%	0.039%
42	15.375	2049	2055	2058	rBV5	6833	12221	0.13%	0.014%
43	15.422	2058	2063	2069	rVV	37754	56317	0.58%	0.063%
44	15.628	2090	2098	2107	rBV	4922598	7108417	72.72%	7.997%
45	15.745	2110	2118	2129	rBV	1858927	2566323	26.25%	2.887%
46	15.869	2134	2139	2146	rVB3	26610	45563	0.47%	0.051%
47	15.992	2155	2160	2165	rBV	104183	141985	1.45%	0.160%
48	17.057	2338	2341	2346	rVB7	6760	10088	0.10%	0.011%
49	17.175	2357	2361	2366	rVB2	9122	15457	0.16%	0.017%
50	17.387	2390	2397	2404	rBV	3280278	4751805	48.61%	5.346%
51	17.486	2407	2414	2425	rBV2	5703746	8360414	85.53%	9.405%
52	17.763	2459	2461	2470	rVB9	11194	17598	0.18%	0.020%
53	18.045	2506	2509	2514	rVB6	8214	12455	0.13%	0.014%
54	18.269	2542	2547	2557	rBV	249583	372913	3.82%	0.420%
55	18.345	2557	2560	2566	rVB	25582	40743	0.42%	0.046%
56	19.339	2725	2729	2734	rBV	77012	100911	1.03%	0.114%
57	19.410	2736	2741	2746	rBV	73978	119018	1.22%	0.134%
58	19.539	2759	2763	2768	rBV2	122340	157774	1.61%	0.177%
59	19.775	2797	2803	2816	rBV	7472676	9643077	98.65%	10.848%
60	21.269	3052	3057	3067	rBV3	272208	512891	5.25%	0.577%
61	21.469	3089	3091	3094	rBV	70187	81151	0.83%	0.091%
62	21.575	3103	3109	3118	rVB	3576052	4973467	50.88%	5.595%
63	23.886	3495	3502	3518	rVB2	4486438	9774720	100.00%	10.996%
64	24.051	3523	3530	3540	rVB2	2627015	5148583	52.67%	5.792%




Sum of corrected areas: 88889470

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024623.D
Acq On : 29 Mar 2023 23:24
Operator : CG/JU
Sample : 02085-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

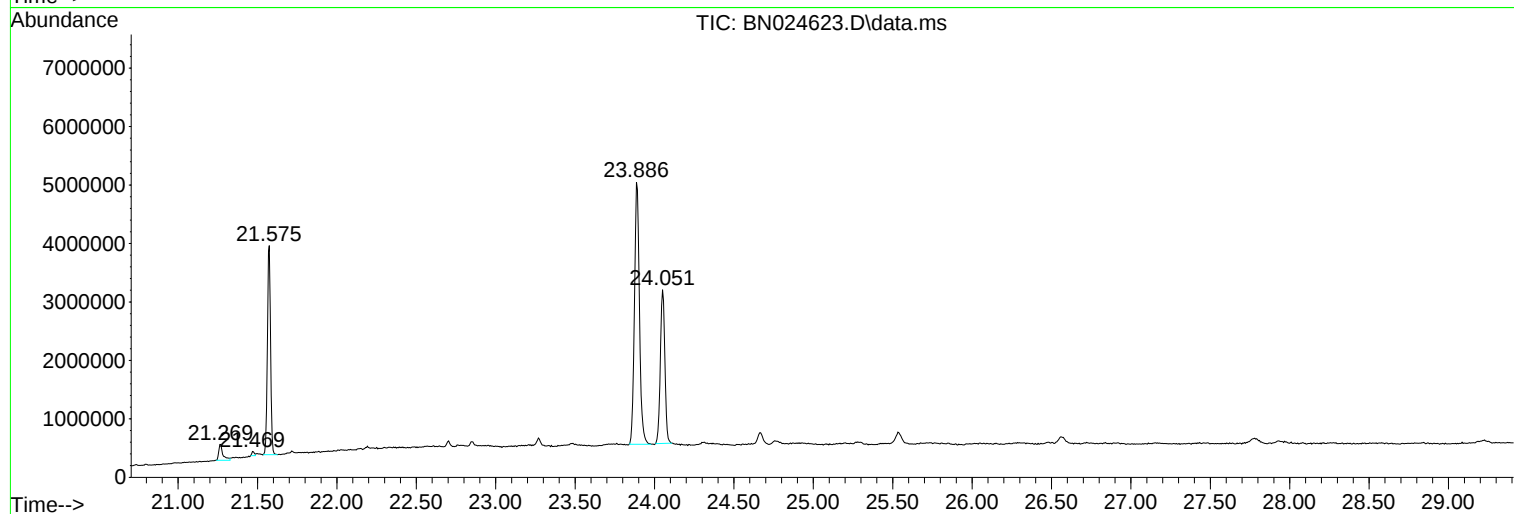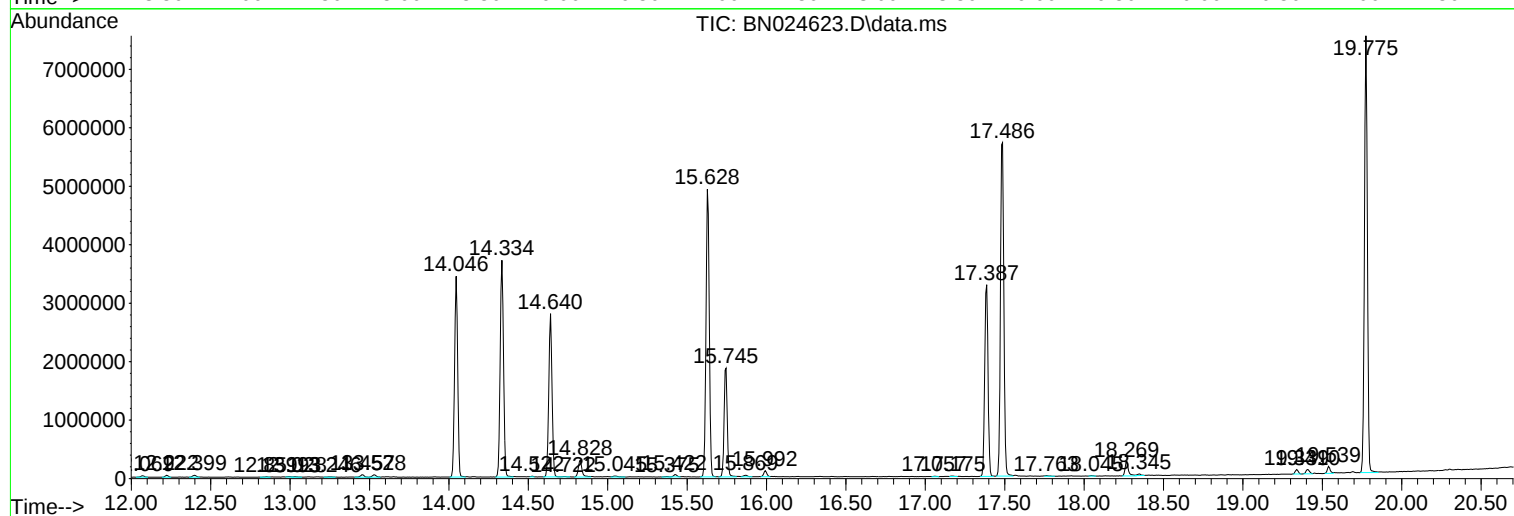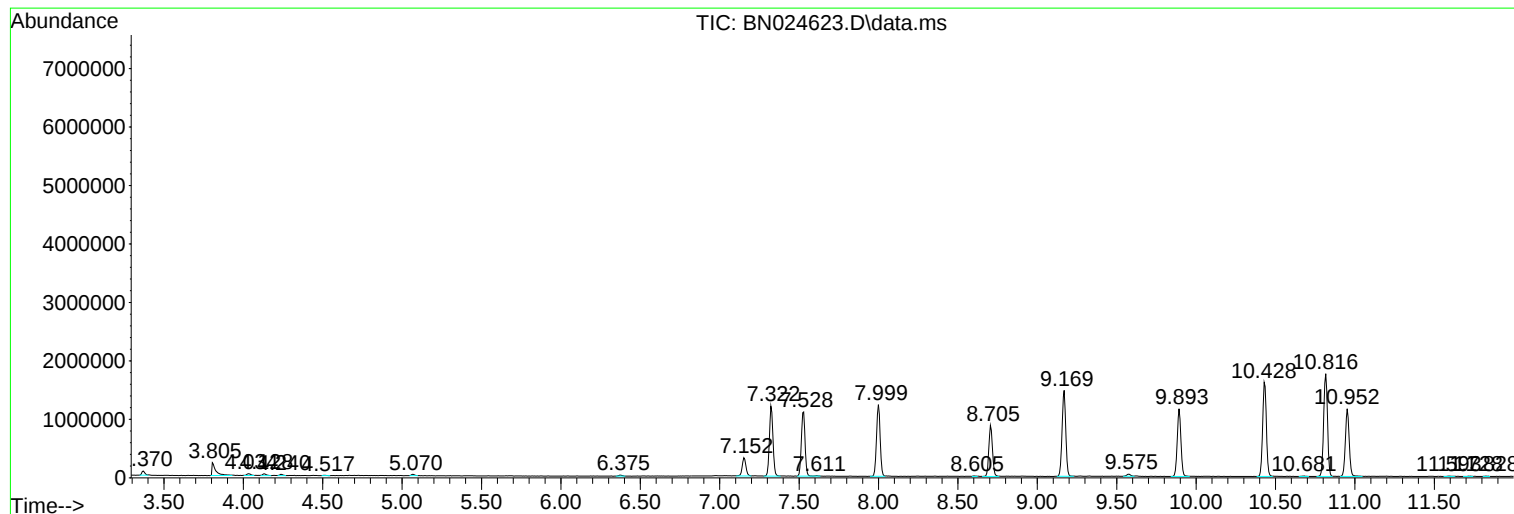

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024623.D
Acq On : 29 Mar 2023 23:24
Operator : CG/JU
Sample : 02085-03
Misc :
ALS Vial : 25 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
COMB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.269 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.269	2.06 ng/ul	512891	Chrysene-d12	21.575	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Cycloeicosane	280	C20H40	000296-56-0	93
2	Pentacos-1-ene	350	C25H50	016980-85-1	93
3	E-14-Hexadecenal	238	C16H30O	330207-53-9	92
4	Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	91
5	Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	91

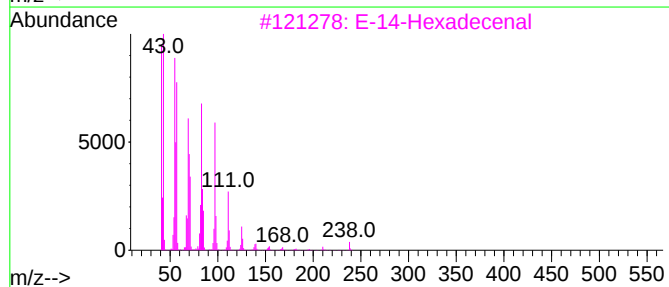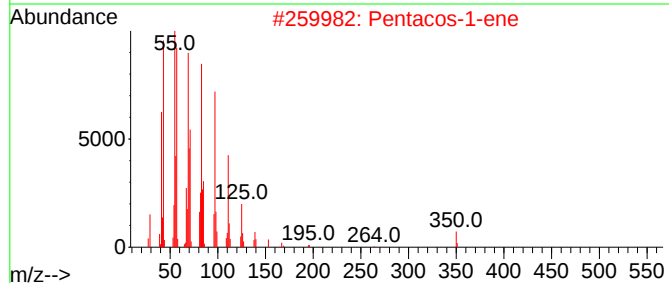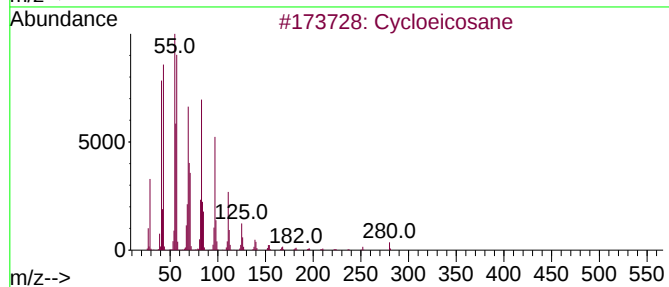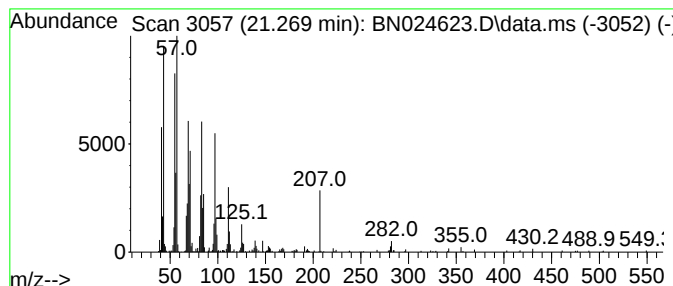

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024623.D
Acq On : 29 Mar 2023 23:24
Operator : CG/JU
Sample : 02085-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.269	2.1	ng/u1	512891	5	21.575	4973470	20.0