

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024625.D
 Acq On : 30 Mar 2023 00:37
 Operator : CG/JU
 Sample : 02038-11
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EYF63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	4	8	11	rBV	178134	247546	2.33%	0.250%
2	3.369	11	14	26	rVB	107882	175139	1.65%	0.177%
3	3.799	84	87	101	rBV	465459	788984	7.44%	0.798%
4	4.034	122	127	134	rVB	36760	60627	0.57%	0.061%
5	4.134	140	144	151	rVB	25096	36656	0.35%	0.037%
6	4.234	157	161	168	rVB5	21023	36121	0.34%	0.037%
7	4.511	205	208	213	rVB6	7699	11396	0.11%	0.012%
8	5.064	298	302	309	rVB	25820	42016	0.40%	0.042%
9	6.375	520	525	532	rBV3	21226	40938	0.39%	0.041%
10	6.969	621	626	634	rBV6	8520	20228	0.19%	0.020%
11	7.152	647	657	670	rVB	408058	691781	6.52%	0.699%
12	7.322	679	686	697	rVB	1435541	2229372	21.02%	2.254%
13	7.528	714	721	731	rVV	1321803	2162391	20.39%	2.186%
14	7.610	731	735	740	rVB8	9270	16428	0.15%	0.017%
15	7.999	792	801	808	rBV	1315424	2078076	19.59%	2.101%
16	8.705	913	921	932	rBV	1078734	1717407	16.19%	1.736%
17	9.169	992	1000	1007	rBV	1718137	2774831	26.16%	2.805%
18	9.275	1013	1018	1022	rVB8	6876	12555	0.12%	0.013%
19	9.328	1022	1027	1031	rBV6	9325	10981	0.10%	0.011%
20	9.575	1065	1069	1073	rVB3	14910	24087	0.23%	0.024%
21	9.893	1114	1123	1138	rBV	1378191	2248031	21.20%	2.273%
22	10.116	1156	1161	1169	rVB7	5998	13399	0.13%	0.014%
23	10.428	1207	1214	1225	rBV	1865517	3086082	29.10%	3.120%
24	10.816	1272	1280	1290	rBV	1897387	3098309	29.21%	3.132%
25	10.951	1295	1303	1317	rBV	1698128	2860733	26.97%	2.892%
26	11.593	1405	1412	1415	rBV4	16963	28528	0.27%	0.029%
27	11.628	1415	1418	1424	rVB4	13762	25309	0.24%	0.026%
28	12.075	1487	1494	1497	rVB2	15019	25789	0.24%	0.026%
29	12.398	1544	1549	1555	rVB	36097	55256	0.52%	0.056%
30	12.998	1645	1651	1657	rBV8	9732	15656	0.15%	0.016%
31	13.245	1688	1693	1699	rVB8	6518	11171	0.11%	0.011%
32	13.528	1737	1741	1745	rBV6	6817	12187	0.11%	0.012%
33	13.604	1748	1754	1759	rVV9	9013	18224	0.17%	0.018%
34	14.045	1822	1829	1839	rBV	3634746	5006835	47.21%	5.062%
35	14.163	1845	1849	1853	rVB5	9967	14439	0.14%	0.015%
36	14.222	1855	1859	1864	rBV2	13566	21805	0.21%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024625.D
 Acq On : 30 Mar 2023 00:37
 Operator : CG/JU
 Sample : 02038-11
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EYF63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

37	14.275	1864	1868	1871	rBV6	9754	13551	0.13%	0.014%
38	14.334	1871	1878	1890	rBV	4172537	5990627	56.48%	6.056%
39	14.640	1917	1930	1940	rBV	2895690	4184784	39.46%	4.231%
40	14.722	1942	1944	1948	rVB4	7556	10720	0.10%	0.011%
41	14.828	1955	1962	1973	rBV	408278	636304	6.00%	0.643%
42	15.039	1993	1998	2006	rVB7	28616	46298	0.44%	0.047%
43	15.428	2058	2064	2065	rBV3	8479	13978	0.13%	0.014%
44	15.451	2065	2068	2071	rVB2	11133	15000	0.14%	0.015%
45	15.628	2091	2098	2111	rVB	5547493	7906565	74.55%	7.993%
46	15.739	2111	2117	2128	rBV	2076062	2825258	26.64%	2.856%
47	15.869	2134	2139	2144	rBV2	25449	39590	0.37%	0.040%
48	15.992	2154	2160	2166	rBV	819432	1064181	10.03%	1.076%
49	16.522	2242	2250	2251	rBV8	5745	12810	0.12%	0.013%
50	16.557	2251	2256	2266	rVB	85471	121794	1.15%	0.123%
51	16.851	2300	2306	2314	rBV10	8987	15905	0.15%	0.016%
52	17.063	2339	2342	2346	rBV6	8106	11828	0.11%	0.012%
53	17.175	2358	2361	2365	rVB4	10763	15135	0.14%	0.015%
54	17.286	2378	2380	2386	rVB7	8605	10771	0.10%	0.011%
55	17.386	2390	2397	2407	rBV	3379751	4945808	46.63%	5.000%
56	17.486	2407	2414	2425	rBV	6239142	8936778	84.26%	9.034%
57	17.763	2454	2461	2466	rBV6	13691	29218	0.28%	0.030%
58	18.045	2506	2509	2514	rBV6	14405	17670	0.17%	0.018%
59	18.263	2542	2546	2551	rBV2	92368	122891	1.16%	0.124%
60	18.345	2556	2560	2565	rBV	19091	32348	0.30%	0.033%
61	19.339	2724	2729	2734	rBV2	83212	121196	1.14%	0.123%
62	19.410	2736	2741	2751	rVB	85191	150896	1.42%	0.153%
63	19.539	2760	2763	2767	rBV4	31794	39094	0.37%	0.040%
64	19.686	2786	2788	2793	rVB5	15347	16963	0.16%	0.017%
65	19.775	2797	2803	2814	rBV	7732214	10482201	98.83%	10.597%
66	21.269	3053	3057	3061	rBV3	132466	190027	1.79%	0.192%
67	21.574	3103	3109	3116	rBV	3807328	5235887	49.37%	5.293%
68	23.892	3496	3503	3515	rVB2	5527973	10606185	100.00%	10.722%
69	24.051	3523	3530	3540	rVB2	2466384	5336906	50.32%	5.395%




Sum of corrected areas: 98918480

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024625.D
Acq On : 30 Mar 2023 00:37
Operator : CG/JU
Sample : 02038-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYF63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

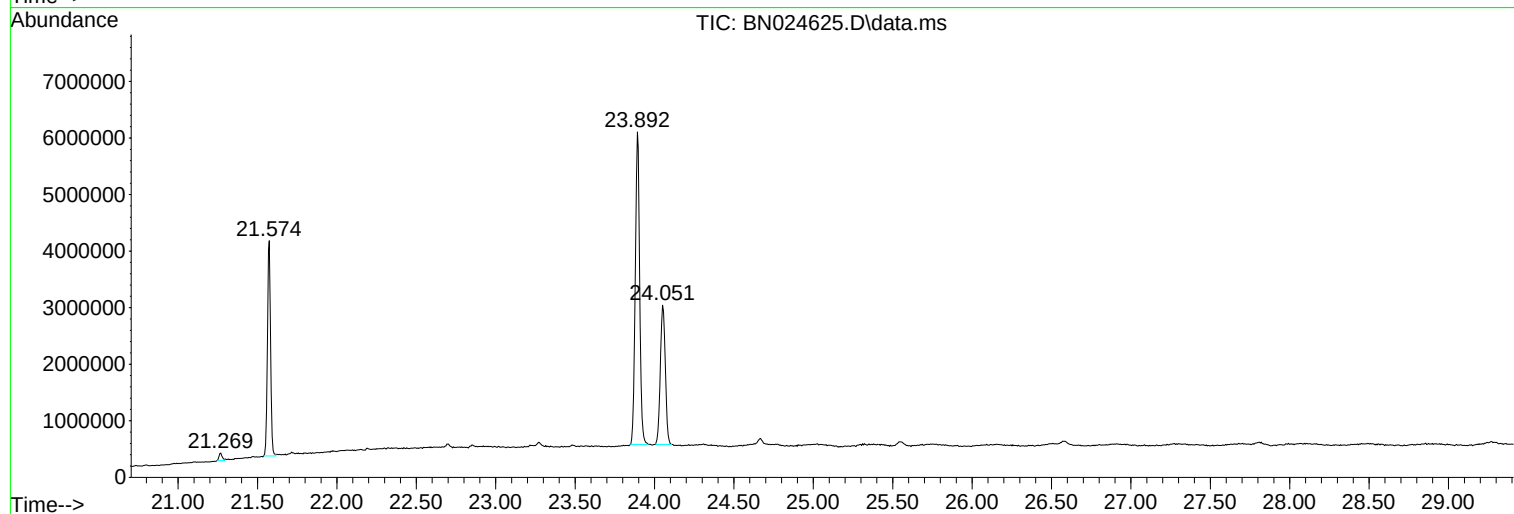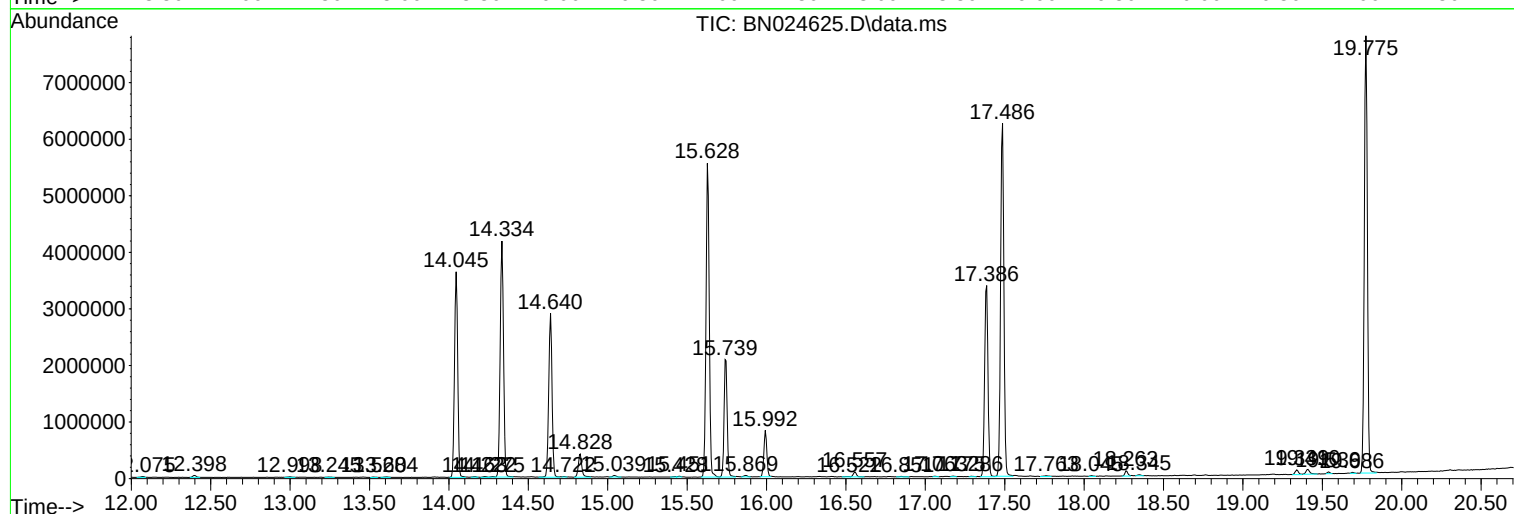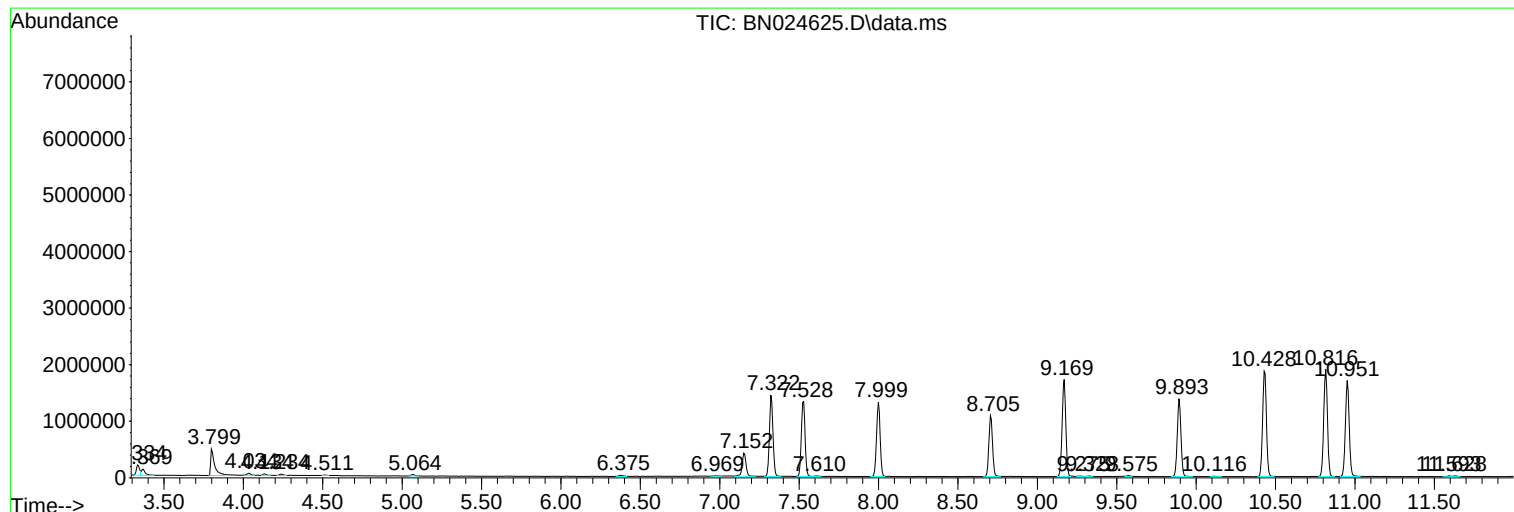

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024625.D
Acq On : 30 Mar 2023 00:37
Operator : CG/JU
Sample : 02038-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYF63










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.992	5.09 ng/ul	1064180	Acenaphthene-d10	14.640

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	91

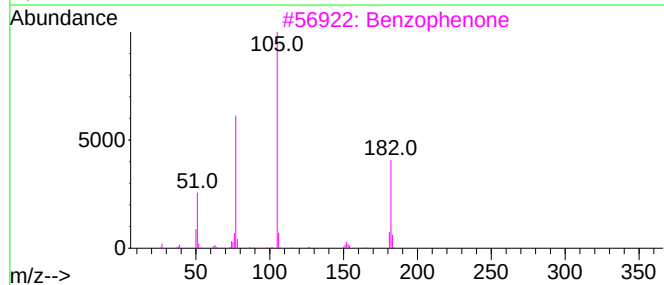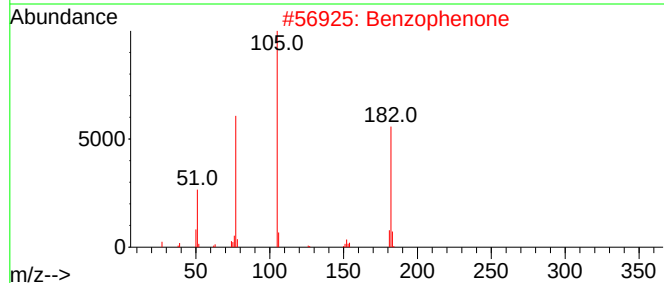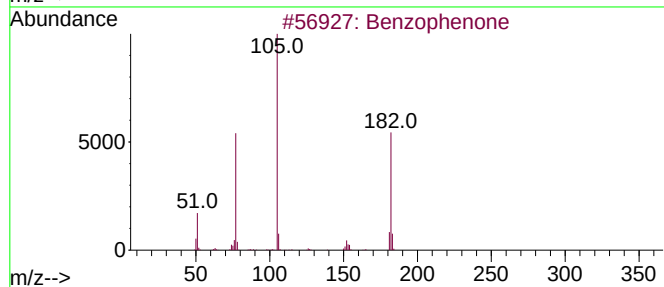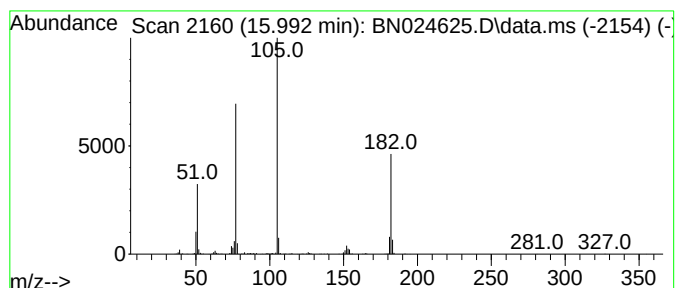

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024625.D
Acq On : 30 Mar 2023 00:37
Operator : CG/JU
Sample : 02038-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYF63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.992	5.1	ng/ul	1064180	3	14.640	4184780	20.0