

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024627.D
 Acq On : 30 Mar 2023 01:49
 Operator : CG/JU
 Sample : 02038-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EYF68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	3	8	12	rBV	252488	376029	3.33%	0.359%
2	3.370	12	14	23	rVB	108212	142480	1.26%	0.136%
3	3.799	85	87	104	rBV	379645	622134	5.51%	0.595%
4	4.034	122	127	133	rVB	40142	62253	0.55%	0.060%
5	4.134	139	144	151	rVB	26415	39109	0.35%	0.037%
6	4.234	157	161	168	rVB4	28384	41710	0.37%	0.040%
7	4.511	205	208	211	rBV5	8573	12763	0.11%	0.012%
8	5.064	297	302	310	rBV	29824	49894	0.44%	0.048%
9	6.369	520	524	532	rVB2	22952	37358	0.33%	0.036%
10	6.969	622	626	630	rBV5	8920	14883	0.13%	0.014%
11	7.152	648	657	665	rVB	421822	679772	6.03%	0.650%
12	7.322	679	686	696	rVB	1569060	2442936	21.65%	2.335%
13	7.522	711	720	729	rBV	1462136	2337538	20.72%	2.235%
14	7.611	731	735	740	rVB4	7888	12808	0.11%	0.012%
15	7.999	793	801	809	rBV	1230454	1931762	17.12%	1.847%
16	8.705	914	921	931	rBV	1183779	1851754	16.41%	1.770%
17	9.169	990	1000	1010	rBV	1916206	3094290	27.43%	2.958%
18	9.269	1013	1017	1022	rVV5	11688	23523	0.21%	0.022%
19	9.328	1024	1027	1035	rVB8	9078	17095	0.15%	0.016%
20	9.575	1063	1069	1076	rVB2	33298	55796	0.49%	0.053%
21	9.893	1115	1123	1136	rBV	1530476	2472583	21.92%	2.364%
22	10.116	1155	1161	1164	rBV8	7879	13733	0.12%	0.013%
23	10.428	1206	1214	1227	rBV	2081984	3438305	30.48%	3.287%
24	10.816	1272	1280	1289	rVB	1697202	2893102	25.64%	2.766%
25	10.952	1295	1303	1318	rBV	1972456	3306929	29.31%	3.161%
26	11.593	1408	1412	1421	rBV6	13198	24150	0.21%	0.023%
27	12.069	1486	1493	1498	rVV3	14410	26292	0.23%	0.025%
28	12.399	1543	1549	1555	rBV2	41624	70306	0.62%	0.067%
29	12.993	1642	1650	1654	rBV10	10929	21905	0.19%	0.021%
30	13.240	1690	1692	1699	rBV6	7983	11316	0.10%	0.011%
31	13.528	1735	1741	1748	rVB4	14482	25159	0.22%	0.024%
32	13.610	1748	1755	1759	rBV8	11114	23308	0.21%	0.022%
33	14.045	1820	1829	1839	rBV	4304312	5737980	50.86%	5.485%
34	14.163	1845	1849	1854	rVB6	17038	22506	0.20%	0.022%
35	14.228	1854	1860	1863	rBV	29116	41991	0.37%	0.040%
36	14.275	1863	1868	1871	rBV5	8496	11835	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
 Data File : BN024627.D
 Acq On : 30 Mar 2023 01:49
 Operator : CG/JU
 Sample : 02038-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EYF68

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
 Title : SVOA CALIBRATION

37	14.334	1871	1878	1889	rBV	4815945	6854990	60.76%	6.553%
38	14.640	1920	1930	1937	rBV	2593203	3887681	34.46%	3.716%
39	14.728	1941	1945	1953	rVB	9873	21465	0.19%	0.021%
40	14.828	1955	1962	1976	rBV	379302	594854	5.27%	0.569%
41	15.045	1994	1999	2004	rVB7	21791	39322	0.35%	0.038%
42	15.422	2058	2063	2065	rBV5	8290	14935	0.13%	0.014%
43	15.628	2089	2098	2109	rBV	6207118	8719304	77.28%	8.335%
44	15.740	2111	2117	2128	rBV	2189342	2935856	26.02%	2.807%
45	15.869	2133	2139	2144	rVB	29365	50405	0.45%	0.048%
46	15.992	2154	2160	2169	rBV	1105871	1446129	12.82%	1.382%
47	16.410	2226	2231	2235	rBV6	7749	12779	0.11%	0.012%
48	16.557	2251	2256	2262	rBV	222724	301750	2.67%	0.288%
49	17.063	2338	2342	2348	rVB7	13481	19291	0.17%	0.018%
50	17.386	2390	2397	2406	rBV	3186424	4639372	41.12%	4.435%
51	17.486	2406	2414	2425	rBV	6447332	9534760	84.51%	9.115%
52	17.563	2425	2427	2431	rVB5	18261	22750	0.20%	0.022%
53	17.663	2440	2444	2452	rVB10	7921	14108	0.13%	0.013%
54	17.757	2457	2460	2467	rVB5	11096	19184	0.17%	0.018%
55	18.263	2542	2546	2556	rBV2	156899	221250	1.96%	0.212%
56	18.339	2556	2559	2567	rVB2	14268	32213	0.29%	0.031%
57	18.692	2616	2619	2623	rBV6	11537	15081	0.13%	0.014%
58	19.339	2724	2729	2735	rBV2	86567	125042	1.11%	0.120%
59	19.404	2736	2740	2746	rBV	83630	137975	1.22%	0.132%
60	19.539	2759	2763	2768	rBV	76789	99737	0.88%	0.095%
61	19.692	2786	2789	2793	rVB3	25248	27948	0.25%	0.027%
62	19.775	2797	2803	2817	rVV	8152962	10996792	97.47%	10.512%
63	21.257	3052	3055	3063	rBV2	196532	293380	2.60%	0.280%
64	21.563	3102	3107	3115	rBV	3759874	4963631	44.00%	4.745%
65	23.898	3496	3504	3519	rBV2	5476908	11282121	100.00%	10.785%
66	24.045	3523	3529	3546	rVB2	2589238	5295871	46.94%	5.063%




Sum of corrected areas: 104607263

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024627.D
Acq On : 30 Mar 2023 01:49
Operator : CG/JU
Sample : 02038-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYF68

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

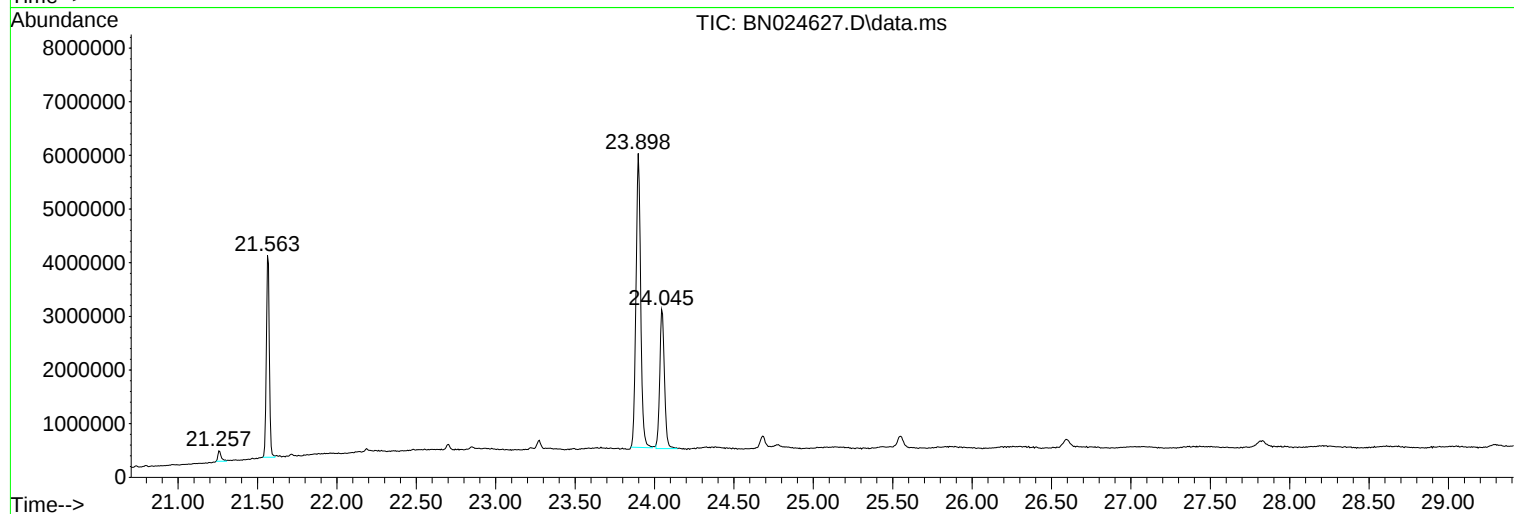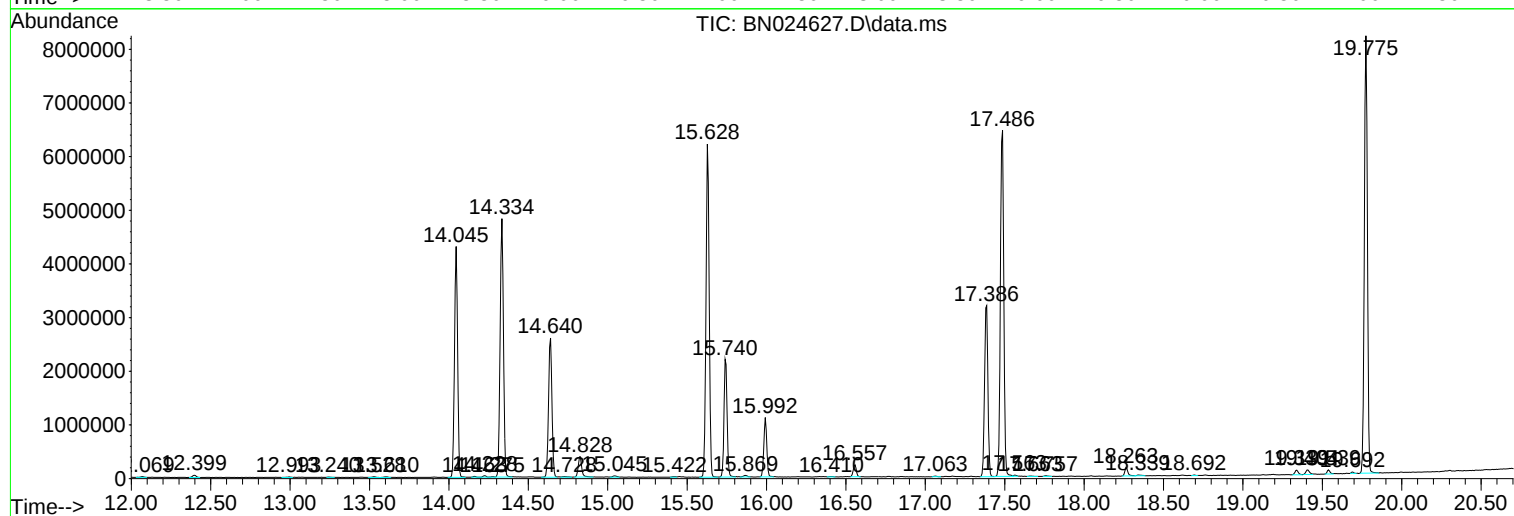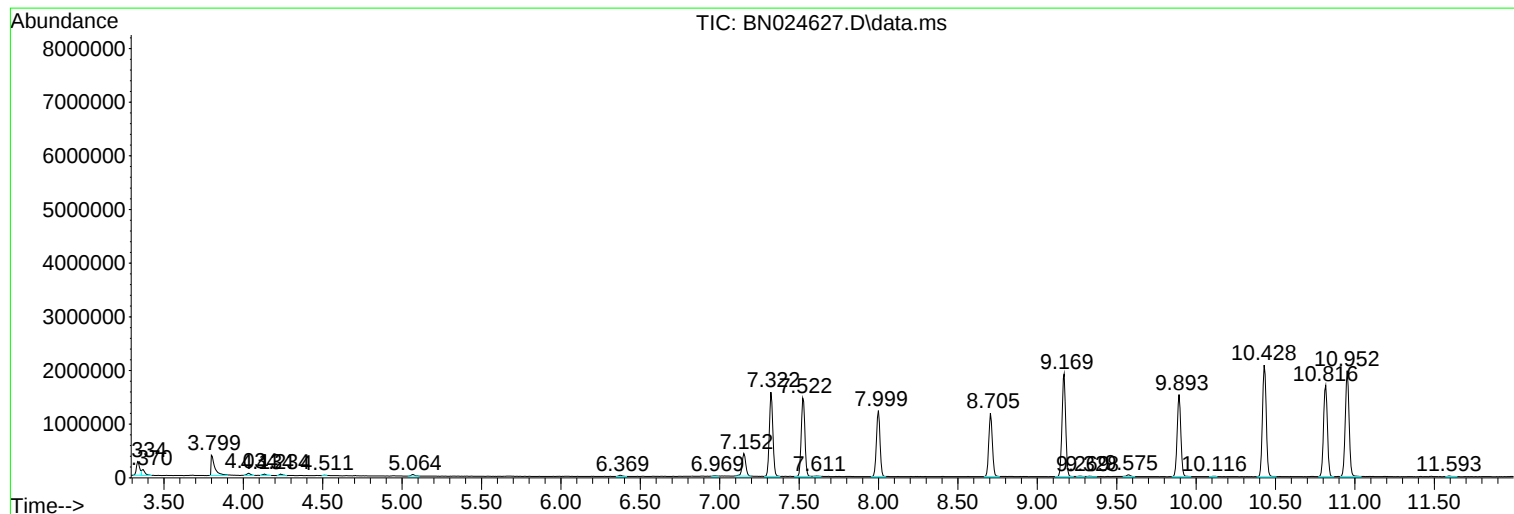

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024627.D
Acq On : 30 Mar 2023 01:49
Operator : CG/JU
Sample : 02038-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYF68










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.993	7.44 ng/ul	1446130	Acenaphthene-d10	14.640

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	97
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	78

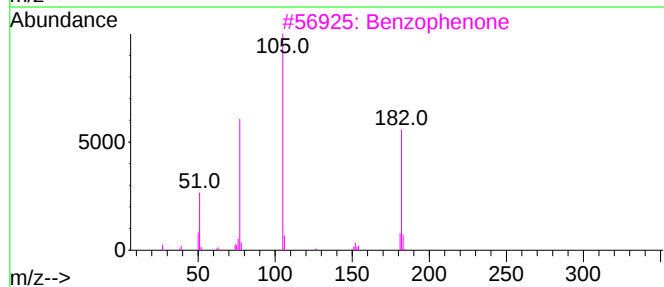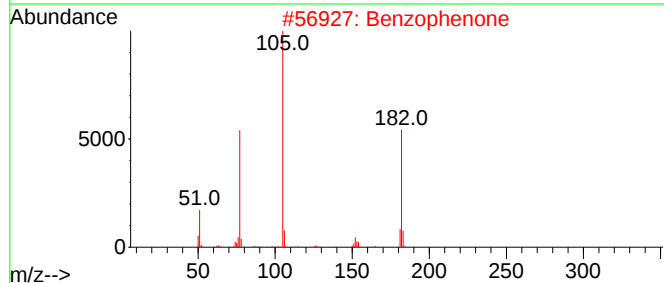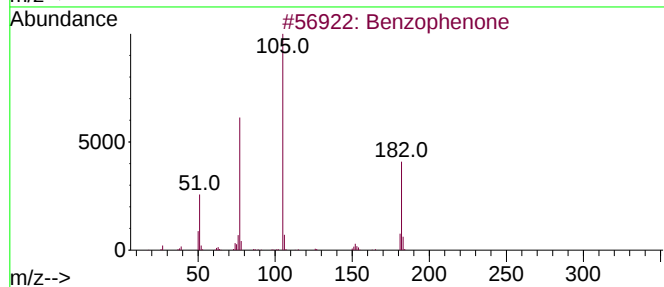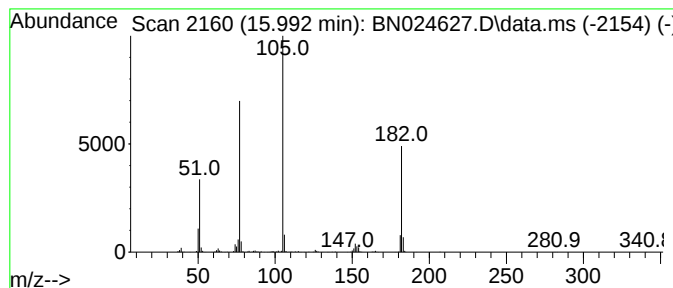

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032923\
Data File : BN024627.D
Acq On : 30 Mar 2023 01:49
Operator : CG/JU
Sample : 02038-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EYF68

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032923.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.993	7.4	ng/u1	1446130	3	14.640	3887680	20.0