




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032924\
Data File : BN030527.D
Acq On : 29 Mar 2024 10:45
Operator : MA/JU
Sample : PB159848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK848

Manual IntegrationsAPPROVED

Quant Time: Mar 29 11:32:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/30/2024
Supervised By :mohammad ahmed 03/30/2024

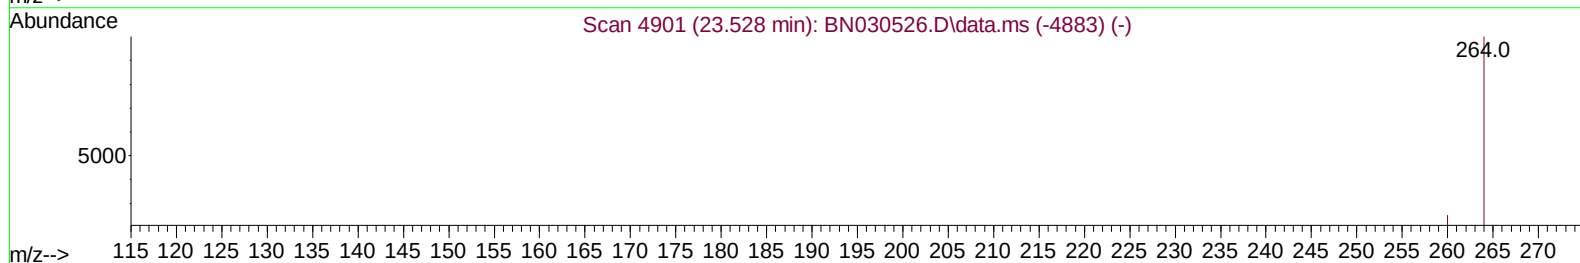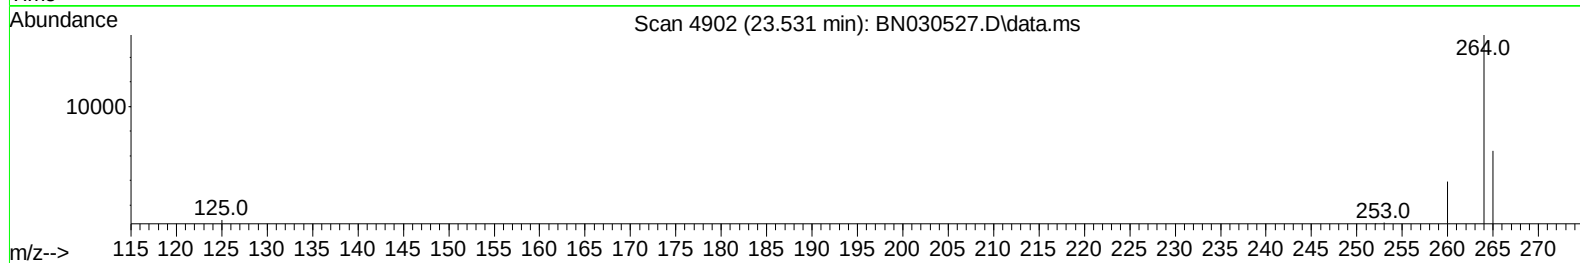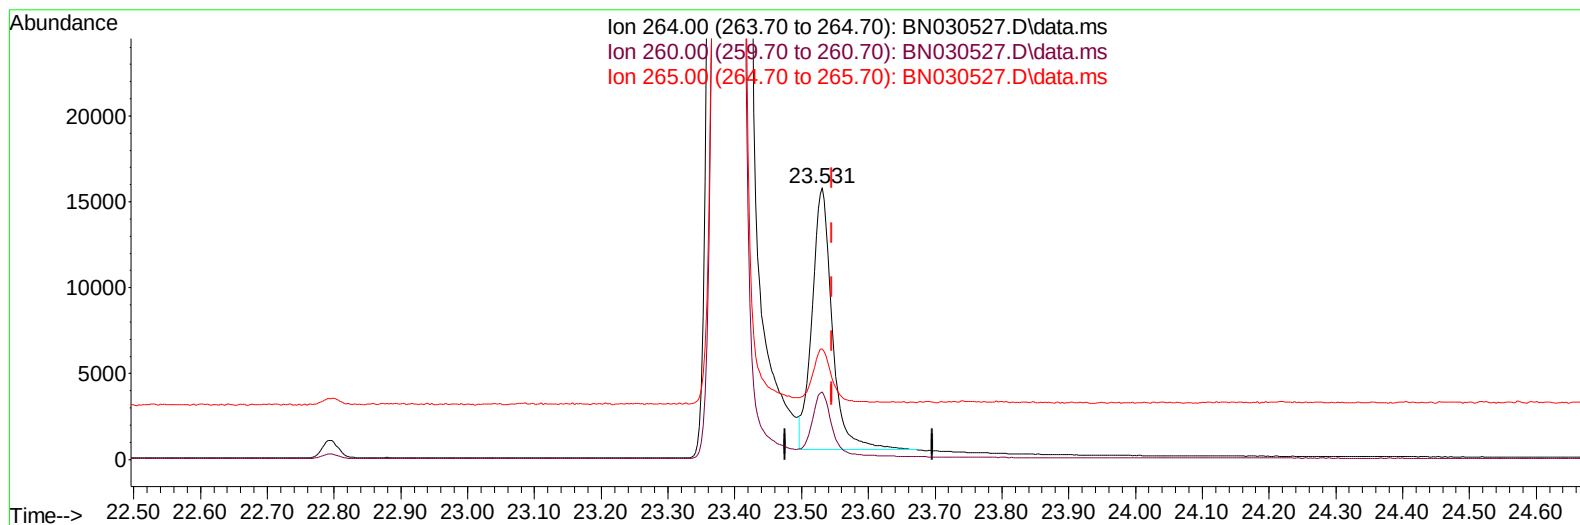

TIC: BN030527.D\data.ms

(23) Perylene-d12 (I)

23.531min (-0.015) 0.40 ng/u1

response 32438

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.89
265.00	52.70	40.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032924\
Data File : BN030527.D
Acq On : 29 Mar 2024 10:45
Operator : MA/JU
Sample : PB159848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK848

Manual IntegrationsAPPROVED

Quant Time: Mar 29 11:32:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/30/2024
Supervised By :mohammad ahmed 03/30/2024

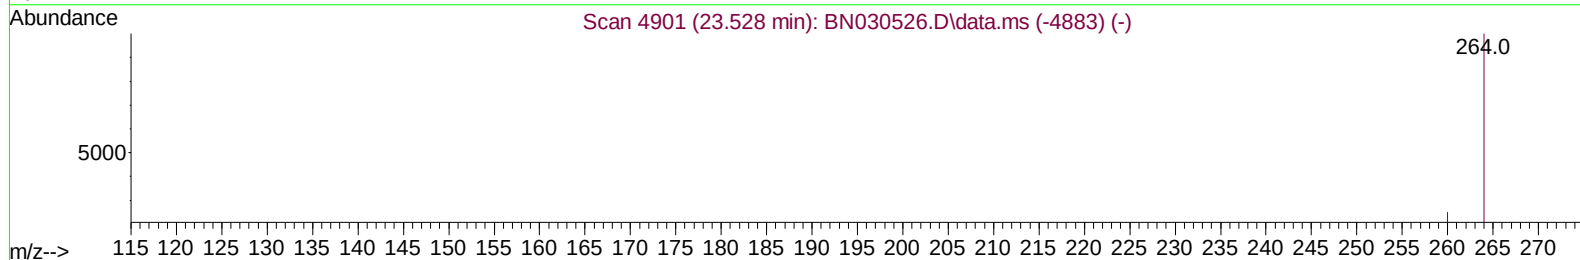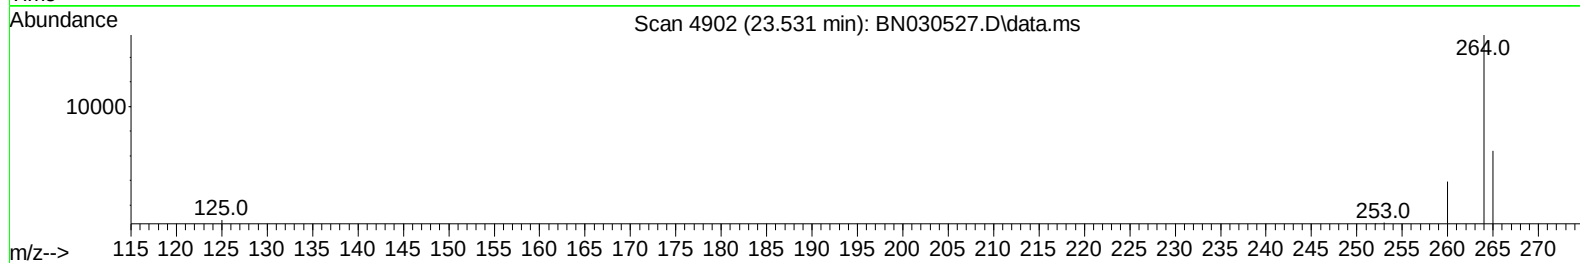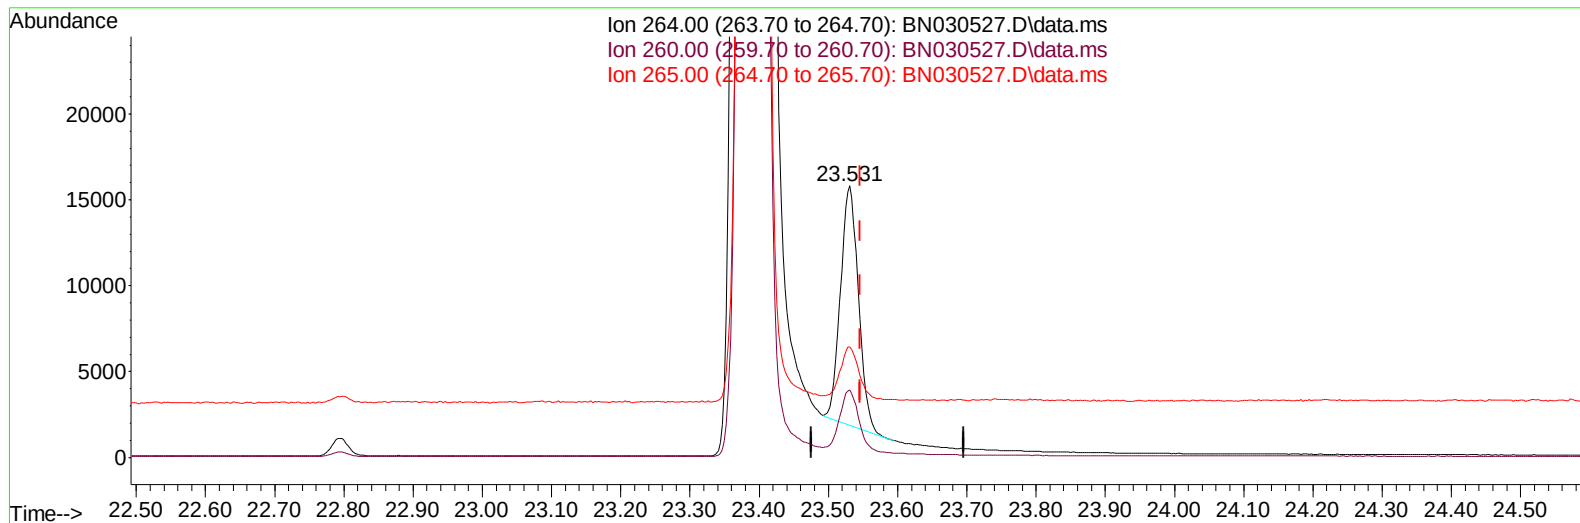

TIC: BN030527.D\data.ms

(23) Perylene-d12 (I)

23.531min (-0.015) 0.40 ng/ul m

response 25203

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.89
265.00	52.70	40.63#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032924\
 Data File : BN030527.D
 Acq On : 29 Mar 2024 10:45
 Operator : MA/JU
 Sample : PB159848BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK848

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/30/2024
 Supervised By :mohammad ahmed 03/30/2024

Quant Time: Mar 29 11:32:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.704	152	8376	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.491	136	25748	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.344	164	14990	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.095	188	34440	0.400	ng/ul	-0.01
17) Chrysene-d12	21.286	240	28324	0.400	ng/ul	-0.01
23) Perylene-d12	23.531	264	25203m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.203	96	43341	4.722	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.080	152	9663	0.249	ng/ul	-0.02
18) Fluoranthene-d10	19.128	212	22787	0.260	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032924\
Data File : BN030527.D
Acq On : 29 Mar 2024 10:45
Operator : MA/JU
Sample : PB159848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK848

Manual IntegrationsAPPROVED

Quant Time: Mar 29 11:32:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/30/2024
Supervised By :mohammad ahmed 03/30/2024

