




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032924\
Data File : BN030528.D
Acq On : 29 Mar 2024 11:21
Operator : MA/JU
Sample : P1866-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Mar 29 11:45:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/30/2024
Supervised By :mohammad ahmed 03/30/2024

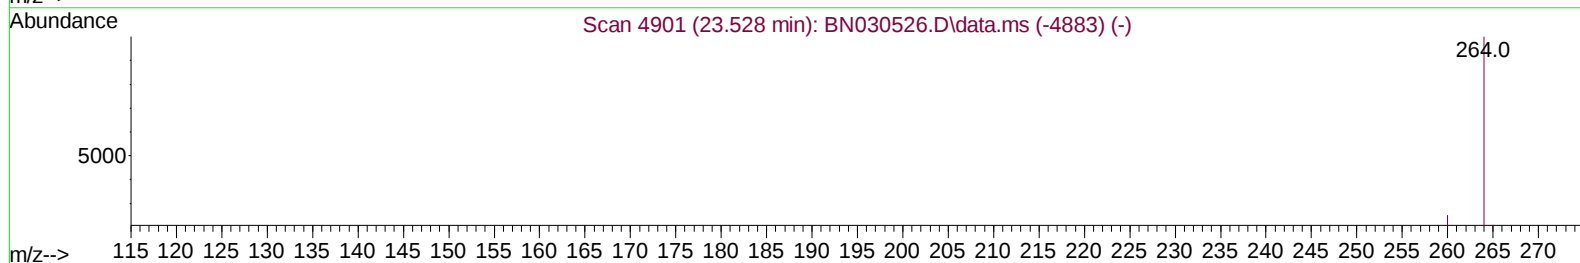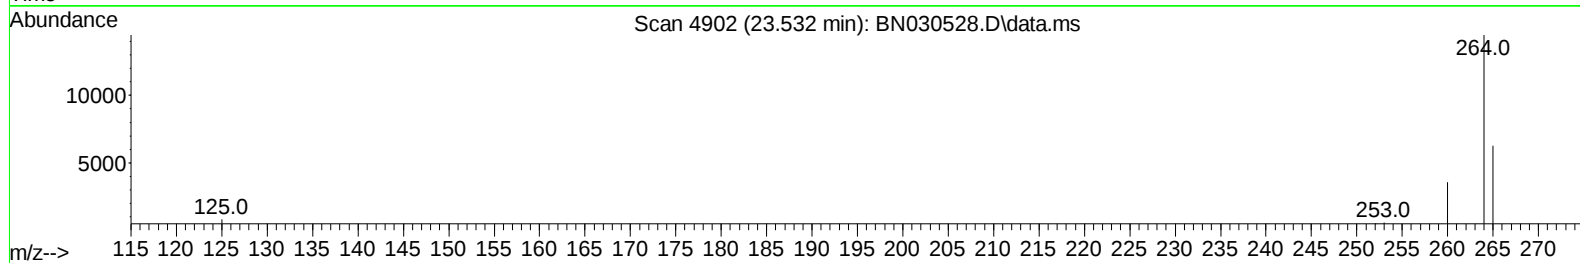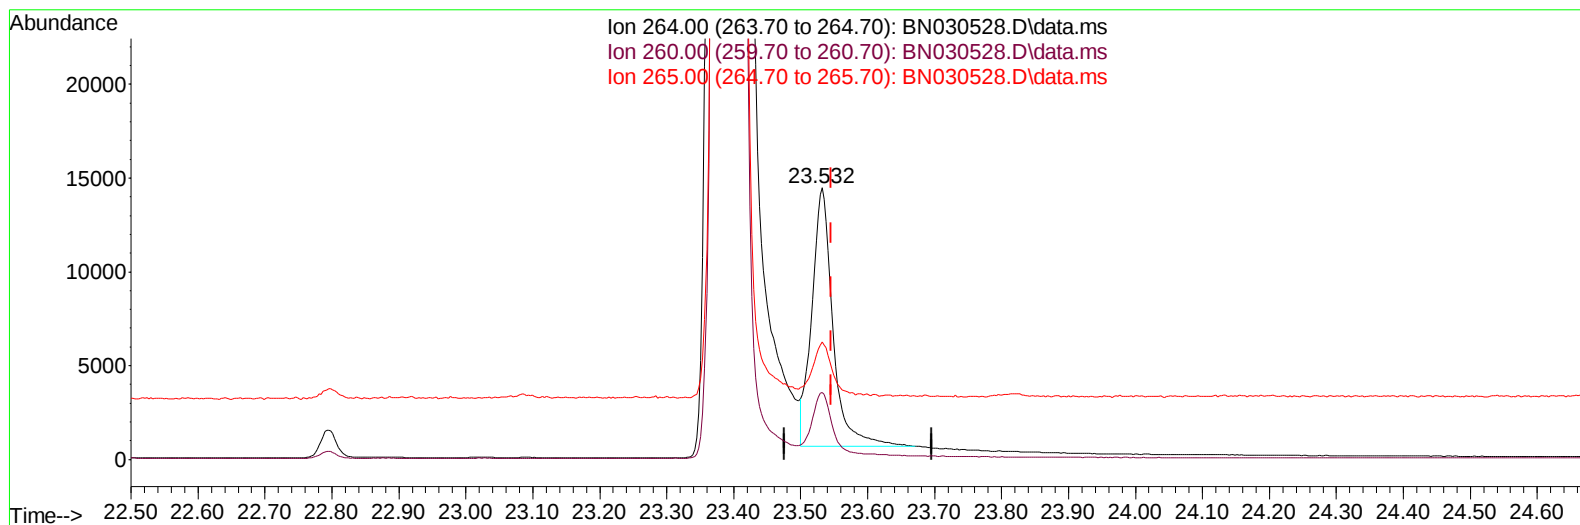

TIC: BN030528.D\data.ms

(23) Perylene-d12 (I)

23.532min (-0.014) 0.40 ng/u1

response 30450

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.62
265.00	52.70	43.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032924\
Data File : BN030528.D
Acq On : 29 Mar 2024 11:21
Operator : MA/JU
Sample : P1866-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Mar 29 11:45:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/30/2024
Supervised By :mohammad ahmed 03/30/2024

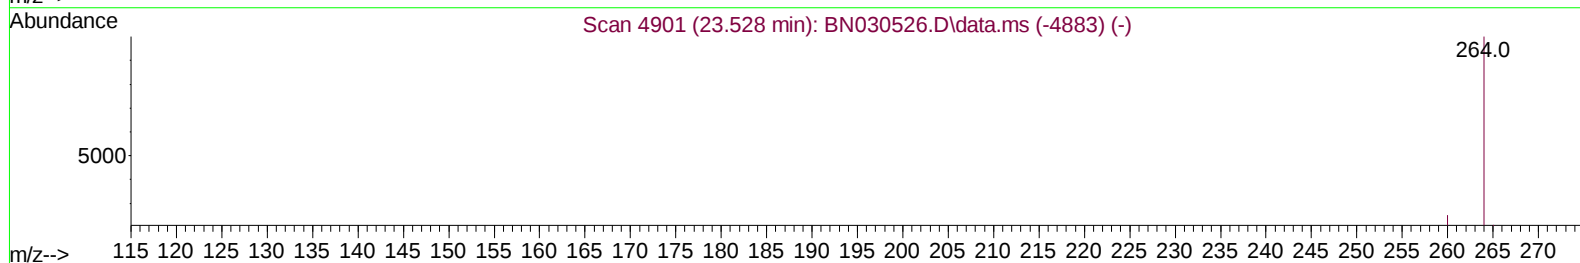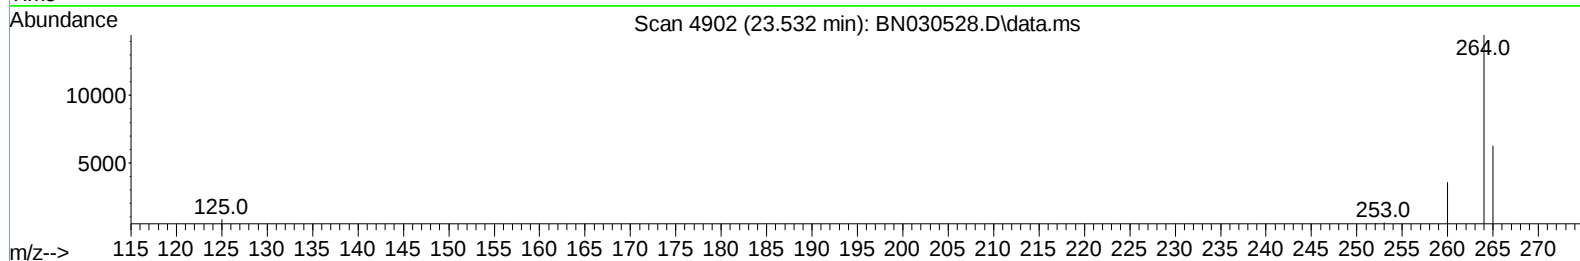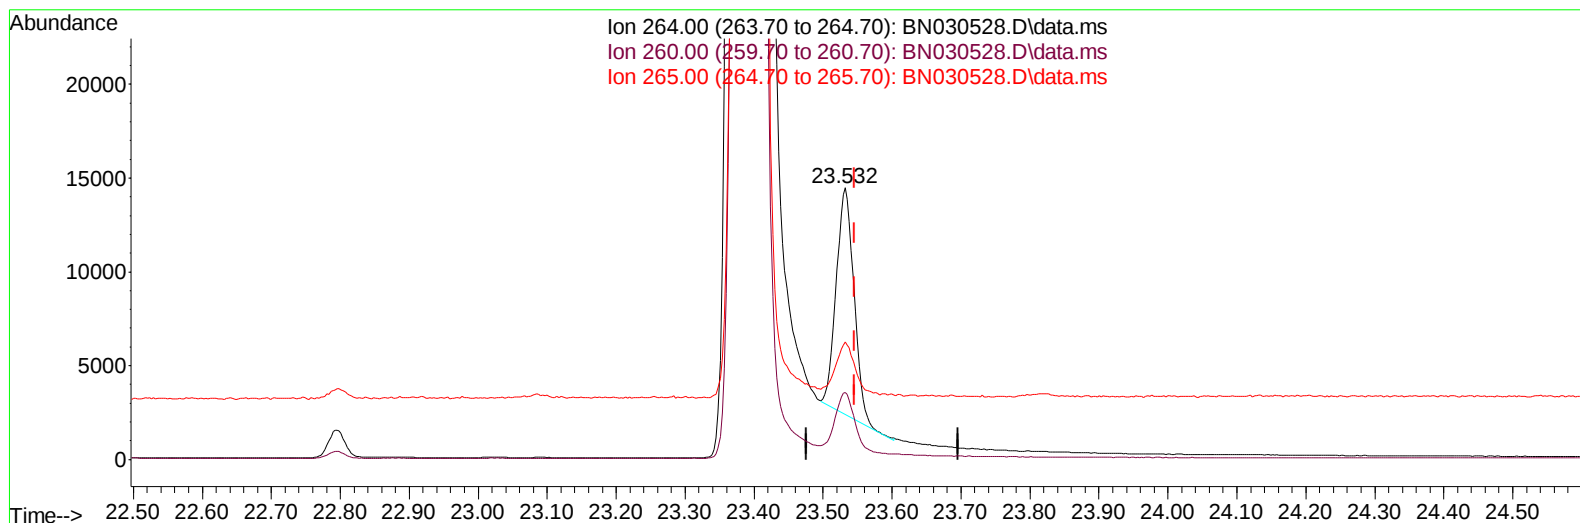

TIC: BN030528.D\data.ms

(23) Perylene-d12 (I)

23.532min (-0.014) 0.40 ng/ul m

response 21671

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.62
265.00	52.70	43.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032924\
 Data File : BN030528.D
 Acq On : 29 Mar 2024 11:21
 Operator : MA/JU
 Sample : P1866-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/30/2024
 Supervised By :mohammad ahmed 03/30/2024

Quant Time: Mar 29 11:45:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.704	152		6643	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.486	136		20519	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.346	164		12000	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.092	188		28051	0.400	ng/ul	-0.02
17) Chrysene-d12	21.287	240		24277	0.400	ng/ul	-0.01
23) Perylene-d12	23.532	264		21671m	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.202	96		37299	5.124	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.081	152		10926	0.354	ng/ul	-0.02
18) Fluoranthene-d10	19.124	212		32203	0.429	ng/ul	-0.01
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.236	88		4631	0.628	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032924\  
Data File : BN030528.D  
Acq On    : 29 Mar 2024  11:21  
Operator  : MA/JU  
Sample    : P1866-02  
Misc      :  
ALS Vial  : 4    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/30/2024
Supervised By :mohammad ahmed 03/30/2024

Quant Time: Mar 29 11:45:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

