

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040120\
 Data File : BN010369.D
 Acq On : 01 Apr 2020 20:54
 Operator : CG/JU
 Sample : L2093-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBF17

Quant Time: Apr 02 00:27:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 01 17:35:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	505522	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	2187611	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	1460125	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	3403054	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	3888676	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	4284052	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	46819	4.38	ng/uL	0.00
5) Phenol-d5	6.79	99	957644	22.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	534840	24.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	805881	24.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	851876	23.91	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	411734	25.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	433727	25.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	880509	24.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	1871039	44.39	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	3124398	28.36	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	3651301	28.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	480909	23.24	ng/ul	0.00
58) Fluorene-d10	15.23	176	2797740	29.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	387711	19.90	ng/ul	0.00
71) Anthracene-d10	17.08	188	4383945	28.06	ng/ul	0.00
79) Pyrene-d10	19.38	212	5195208	25.93	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	6041074	28.35	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.70	163	973237	8.555	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040120\
Data File : BN010369.D
Acq On : 01 Apr 2020 20:54
Operator : CG/JU
Sample : L2093-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBF17

Quant Time: Apr 02 00:27:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 01 17:35:00 2020
Response via : Initial Calibration

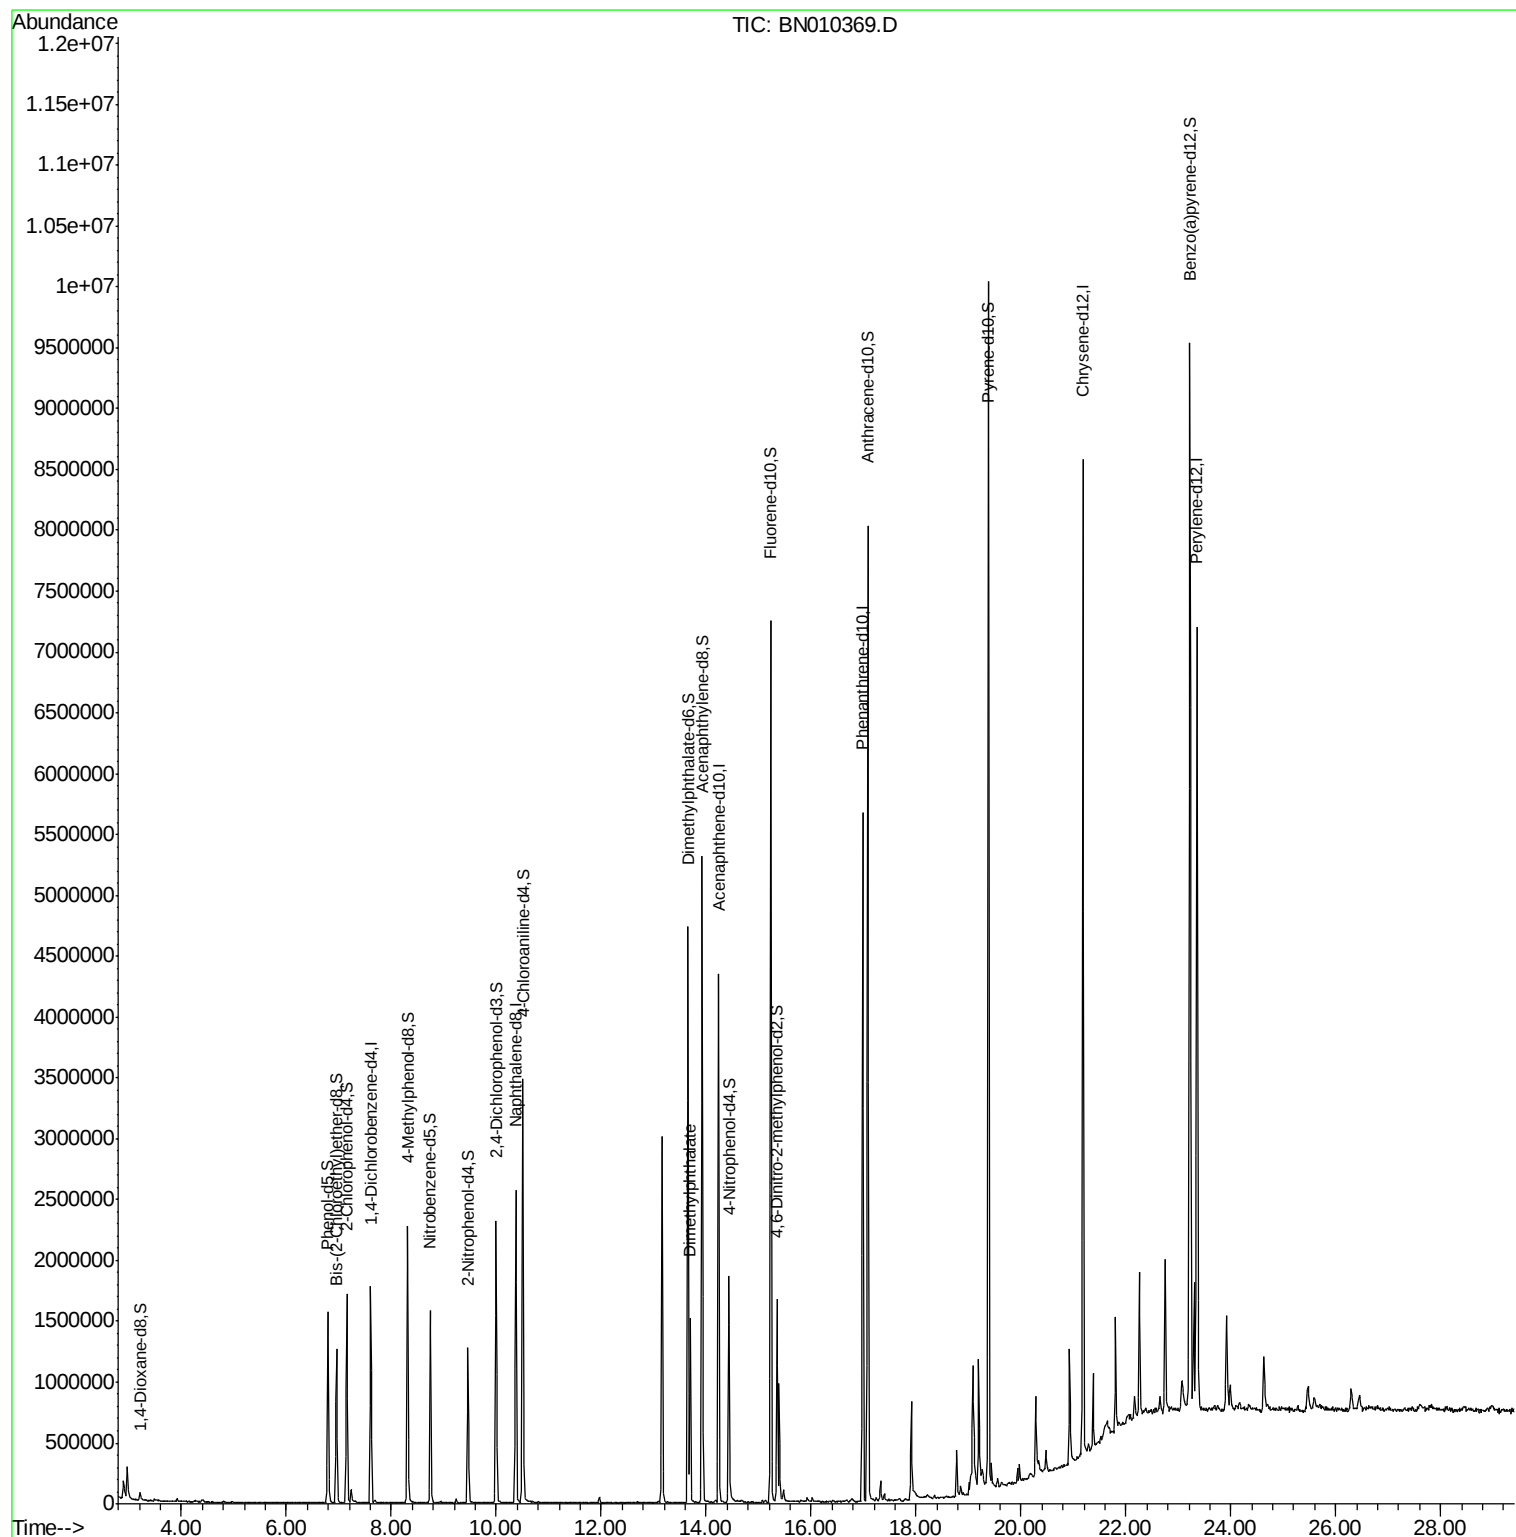

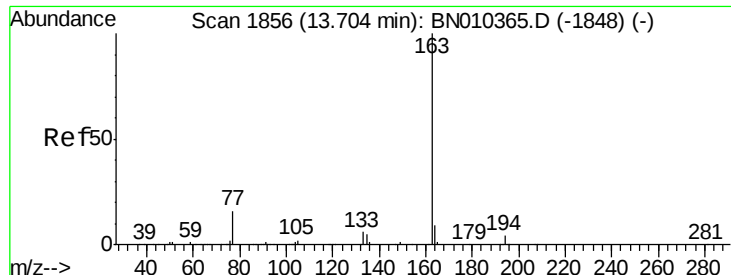

#45

Dimethylphthalate

Concen: 8.555 ng/ul

RT: 13.70 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BN010369.D

Acq: 01 Apr 2020 20:54

Instrument :

BNA_N

ClientSampleId :

DBF17

Tot Ion:163 Resp: 973237

Ion Ratio Lower Upper

163 100

194 4.1 3.7 5.5

164 10.3 8.0 12.0

