

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040120\
 Data File : BN010383.D
 Acq On : 02 Apr 2020 08:47
 Operator : CG/JU
 Sample : L2065-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBF04

Quant Time: Apr 02 10:34:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 01 17:35:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	434540	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.36	136	2006784	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	1404261	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	3218748	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	3667540	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	4281557	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	11592	1.26	ng/uL	0.00
5) Phenol-d5	6.78	99	274175	7.56	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.94	67	613131	32.29	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.14	132	826850	28.73	ng/ul	-0.01
13) 4-Methylphenol-d8	8.30	113	573667	18.73	ng/ul	-0.02
19) Nitrobenzene-d5	8.74	128	510885	34.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	583637	37.00	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.99	165	1137908	34.79	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.50	131	8423	0.22	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	3889508	36.71	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	4571868	36.94	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	135004	6.78	ng/ul	-0.01
58) Fluorene-d10	15.23	176	3469951	37.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	577979	31.36	ng/ul	0.00
71) Anthracene-d10	17.08	188	5498732	37.21	ng/ul	0.00
79) Pyrene-d10	19.38	212	6471657	34.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	8051722	37.80	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.69	163	670016	6.124	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040120\
Data File : BN010383.D
Acq On : 02 Apr 2020 08:47
Operator : CG/JU
Sample : L2065-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBF04

Quant Time: Apr 02 10:34:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 01 17:35:00 2020
Response via : Initial Calibration

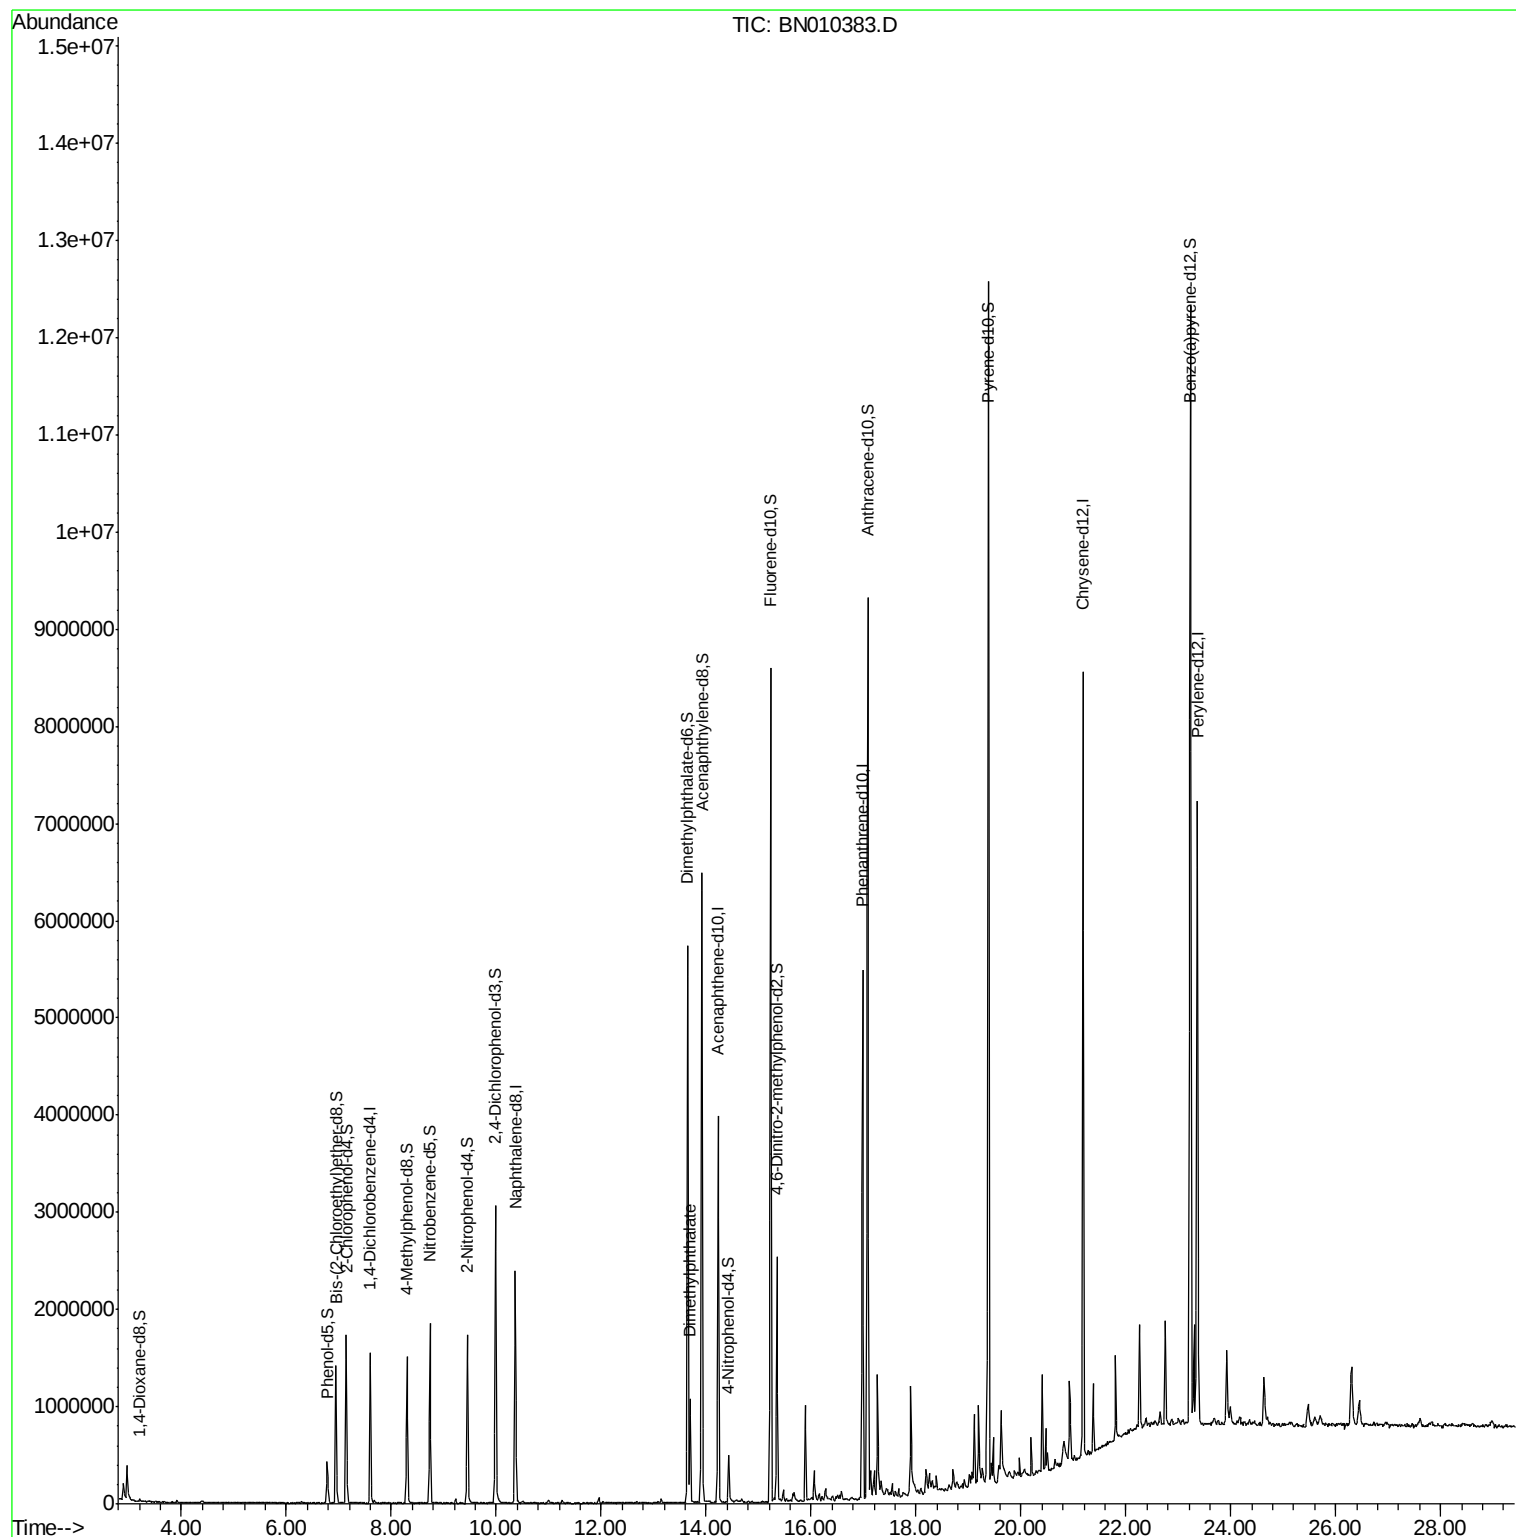

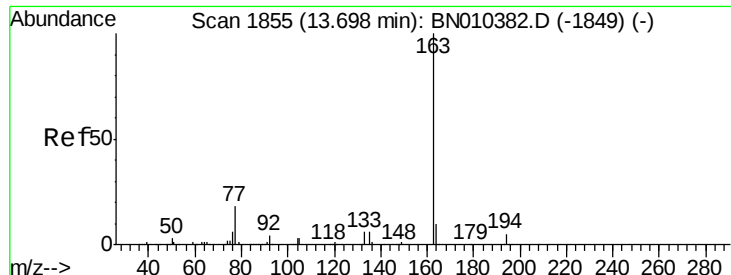

#45

Dimethylphthalate

Concen: 6.124 ng/ul

RT: 13.69 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BN010383.D

Acq: 02 Apr 2020 08:47

Instrument :

BNA_N

ClientSampleId :

DBF04


Tot Ion:163 Resp: 670016

Ion Ratio Lower Upper

163 100

194 4.1 3.7 5.5

164 10.8 8.0 12.0

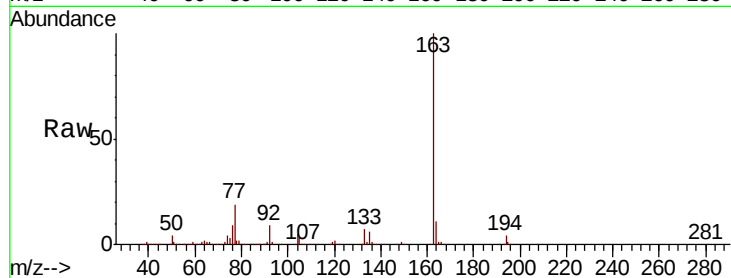

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

