




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
 Data File : BN030574.D
 Acq On : 31 Mar 2024 11:49
 Operator : MA/JU
 Sample : PB159893BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK893

Manual IntegrationsAPPROVED

Quant Time: Mar 31 14:07:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

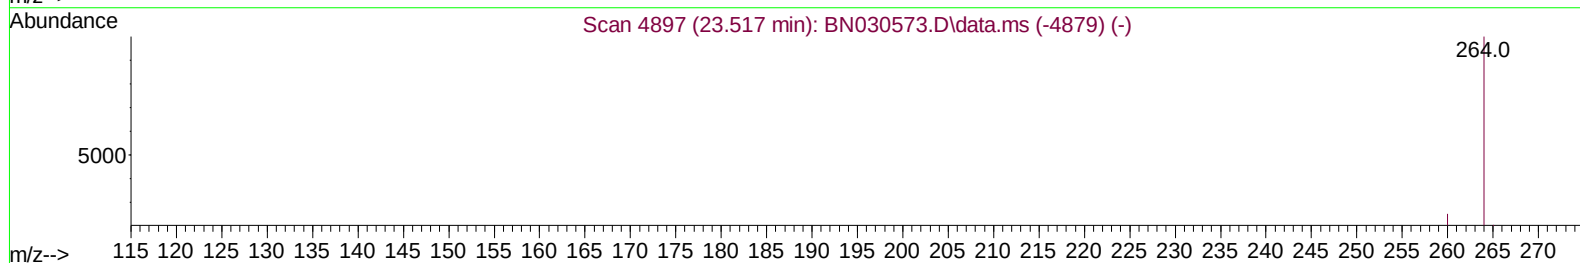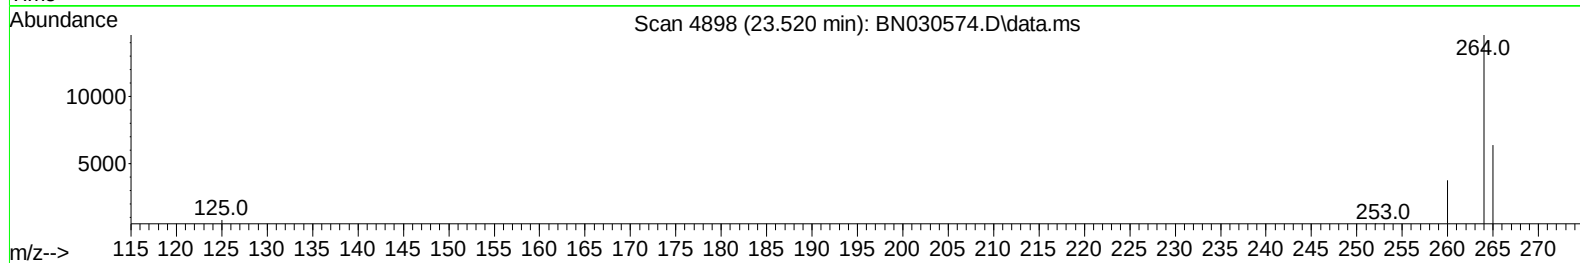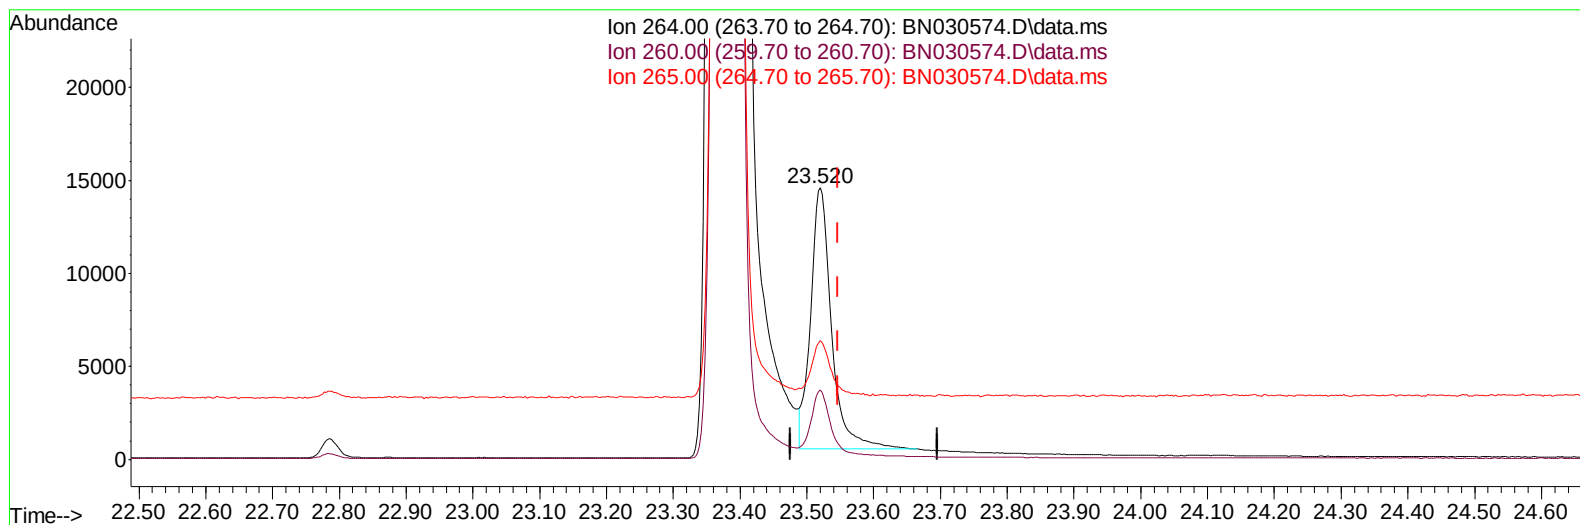

TIC: BN030574.D\data.ms

(23) Perylene-d12 (I)

23.520min (-0.026) 0.40 ng/u1

response 30976

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	25.70
265.00	52.70	43.74
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
Data File : BN030574.D
Acq On : 31 Mar 2024 11:49
Operator : MA/JU
Sample : PB159893BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK893

Manual IntegrationsAPPROVED

Quant Time: Mar 31 14:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024

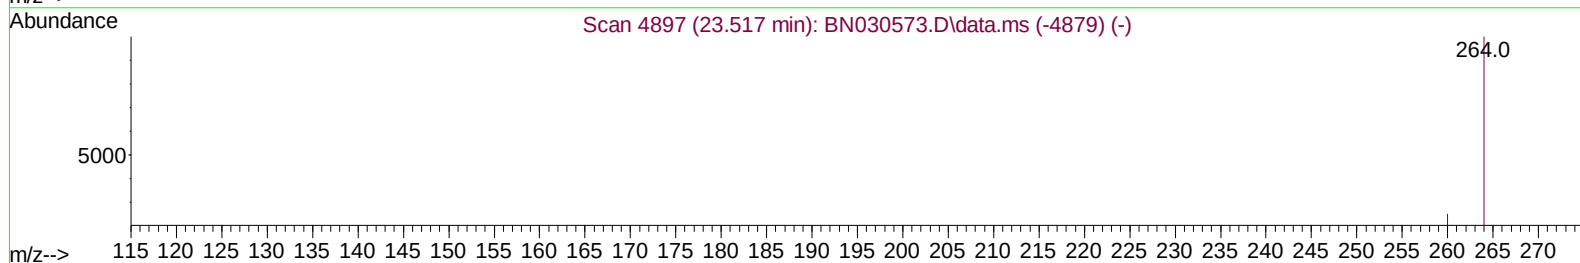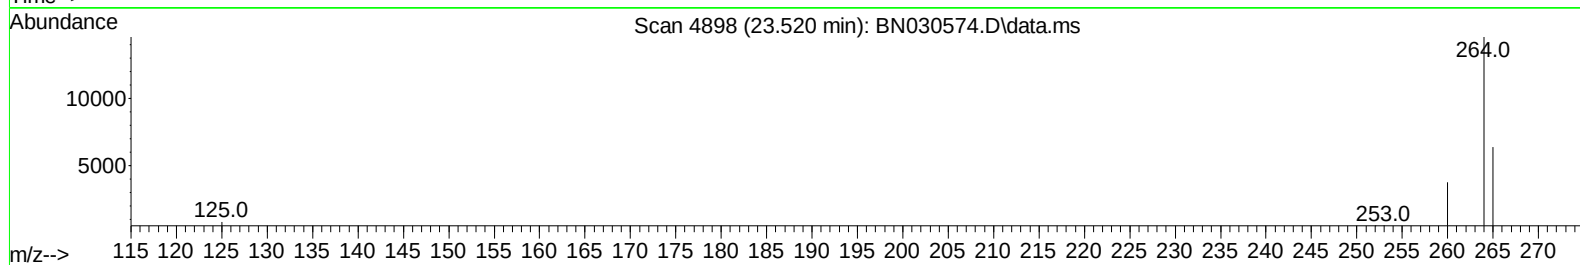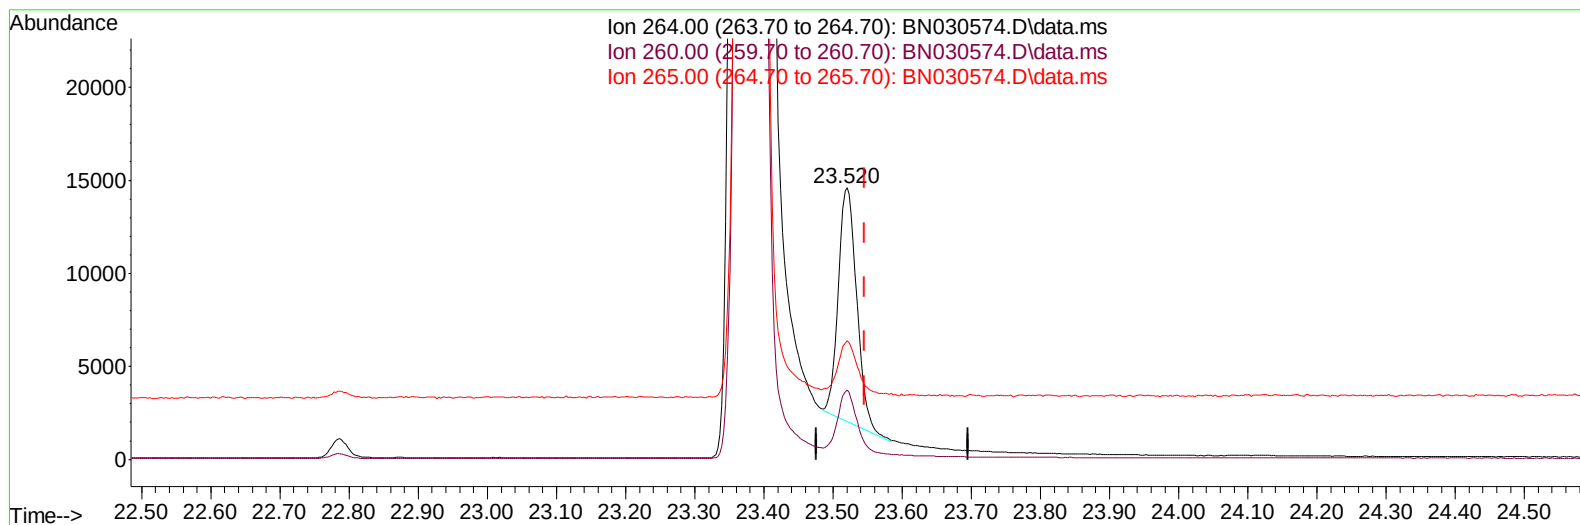

TIC: BN030574.D\data.ms

(23) Perylene-d12 (I)

23.520min (-0.026) 0.40 ng/ul m

response 23226

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	25.70
265.00	52.70	43.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
 Data File : BN030574.D
 Acq On : 31 Mar 2024 11:49
 Operator : MA/JU
 Sample : PB159893BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK893

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Mar 31 14:07:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	8407	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.481	136	26273	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.341	164	14873	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.088	188	33399	0.400	ng/ul	-0.02
17) Chrysene-d12	21.281	240	26626	0.400	ng/ul	-0.02
23) Perylene-d12	23.520	264	23226m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.198	96	67131	7.288	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.075	152	10510	0.266	ng/ul	-0.03
18) Fluoranthene-d10	19.119	212	23676	0.288	ng/ul	-0.02

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
Data File : BN030574.D
Acq On : 31 Mar 2024 11:49
Operator : MA/JU
Sample : PB159893BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK893

Manual IntegrationsAPPROVED

Quant Time: Mar 31 14:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024

