




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
 Data File : BN030576.D
 Acq On : 31 Mar 2024 13:01
 Operator : MA/JU
 Sample : P1929-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL5

Manual IntegrationsAPPROVED

Quant Time: Mar 31 14:09:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

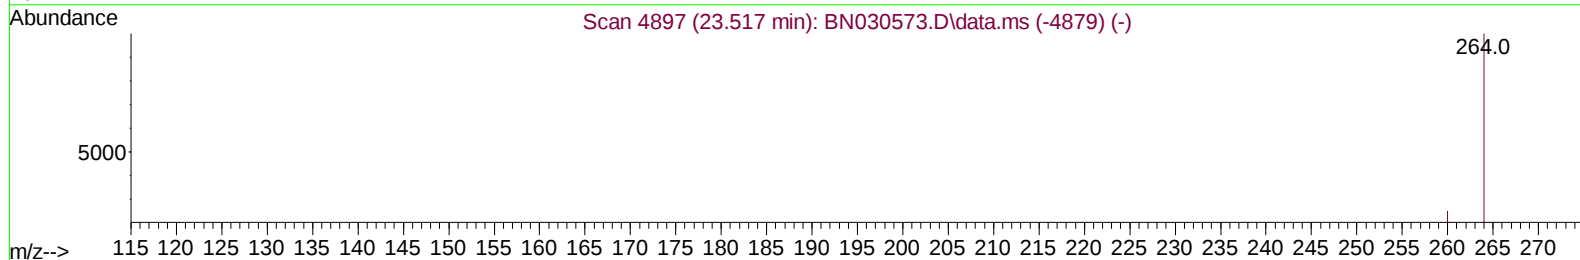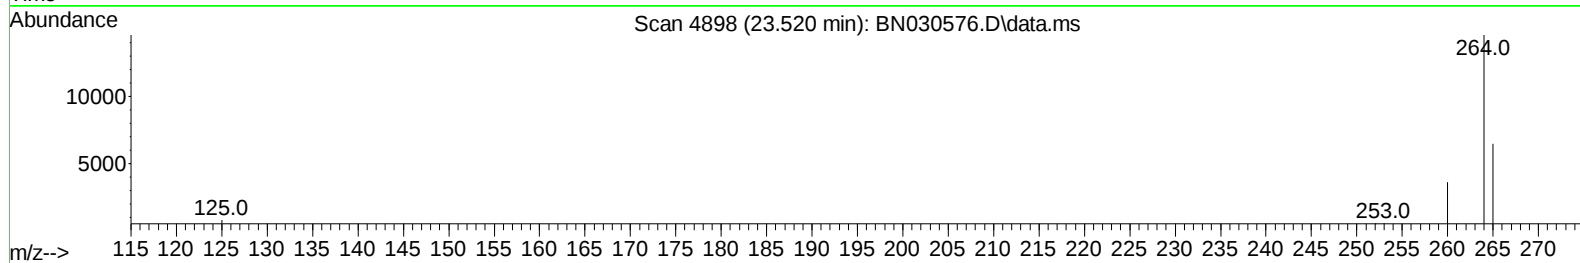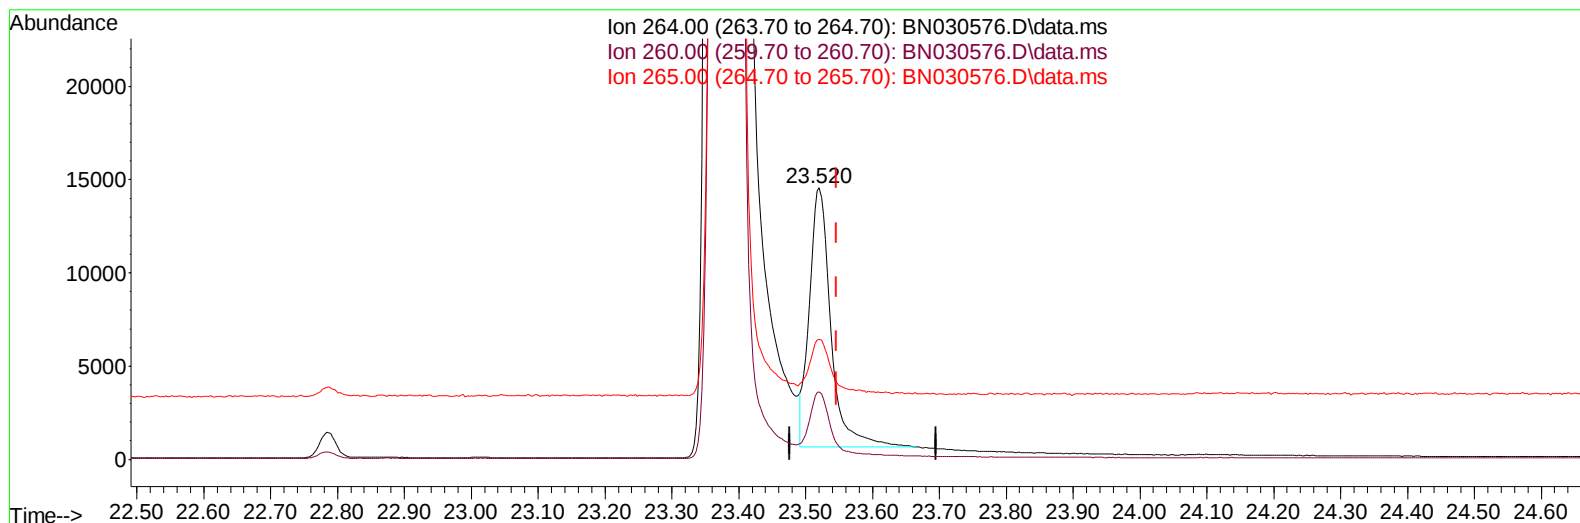

TIC: BN030576.D\data.ms

(23) Perylene-d12 (I)

23.520min (-0.026) 0.40 ng/u1

response 31058

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.89
265.00	52.70	44.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
Data File : BN030576.D
Acq On : 31 Mar 2024 13:01
Operator : MA/JU
Sample : P1929-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Manual IntegrationsAPPROVED

Quant Time: Mar 31 14:09:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024

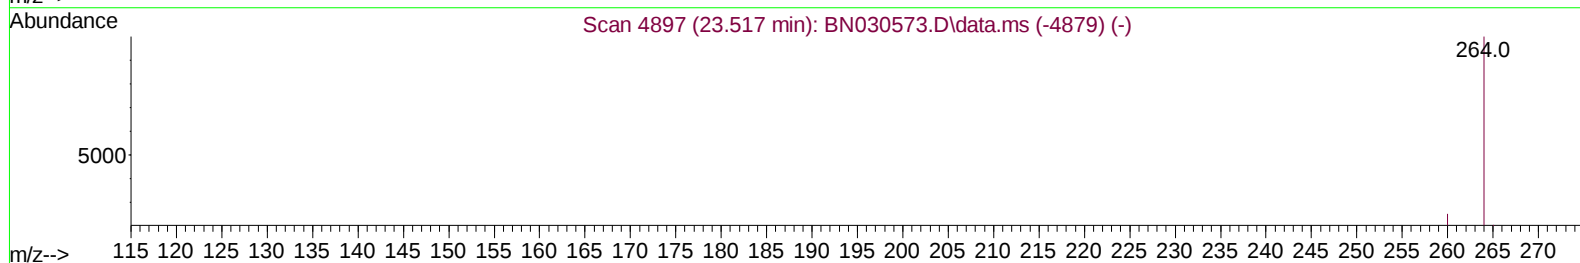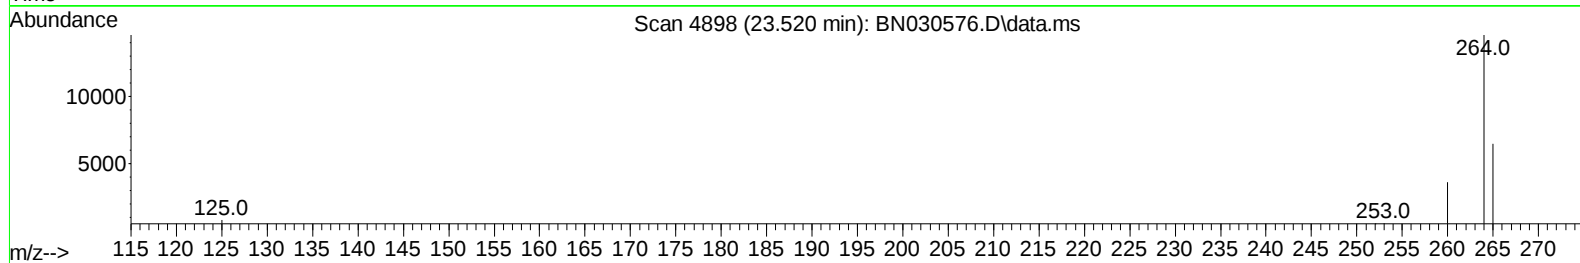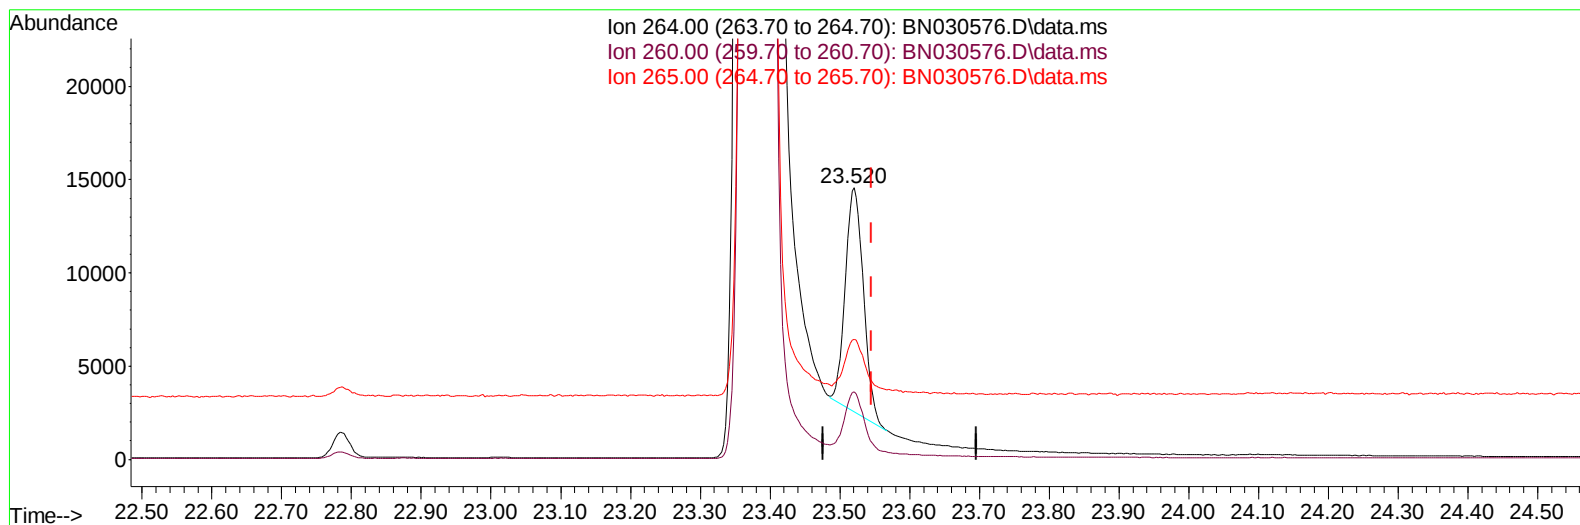

TIC: BN030576.D\data.ms

(23) Perylene-d12 (I)

23.520min (-0.026) 0.40 ng/ul m

response 21711

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.89
265.00	52.70	44.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
 Data File : BN030576.D
 Acq On : 31 Mar 2024 13:01
 Operator : MA/JU
 Sample : P1929-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Mar 31 14:09:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.700	152		7940	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.481	136		24787	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.341	164		14041	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.088	188		31736	0.400	ng/ul	-0.02
17) Chrysene-d12	21.282	240		25776	0.400	ng/ul	-0.02
23) Perylene-d12	23.520	264		21711m	0.400	ng/ul	-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.198	96		47522	5.462	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.076	152		13630	0.365	ng/ul	-0.03
18) Fluoranthene-d10	19.120	212		32906	0.413	ng/ul	-0.02
Target Compounds							
2) 1,4-Dioxane	3.236	88		7555	0.857	ng/ul#	Qvalue 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
Data File : BN030576.D
Acq On : 31 Mar 2024 13:01
Operator : MA/JU
Sample : P1929-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Manual IntegrationsAPPROVED

Quant Time: Mar 31 14:09:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024

