




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
 Data File : BN030577.D
 Acq On : 31 Mar 2024 13:37
 Operator : MA/JU
 Sample : P1929-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL6

Manual IntegrationsAPPROVED

Quant Time: Mar 31 14:11:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

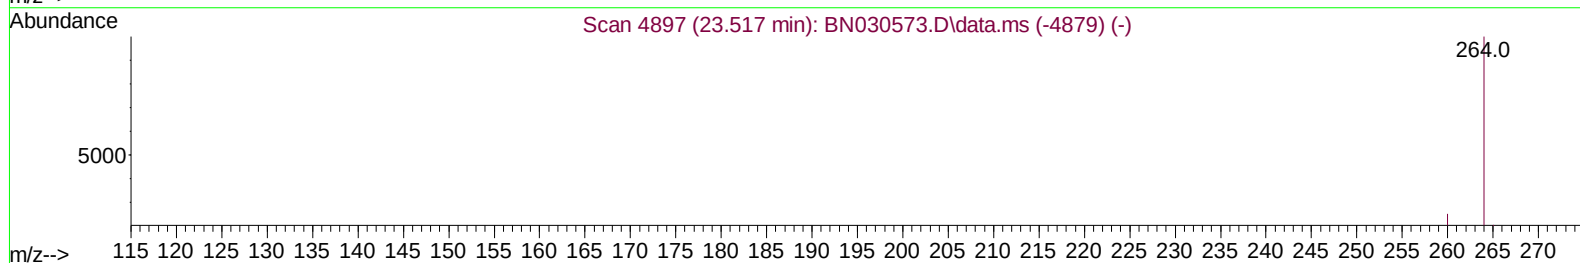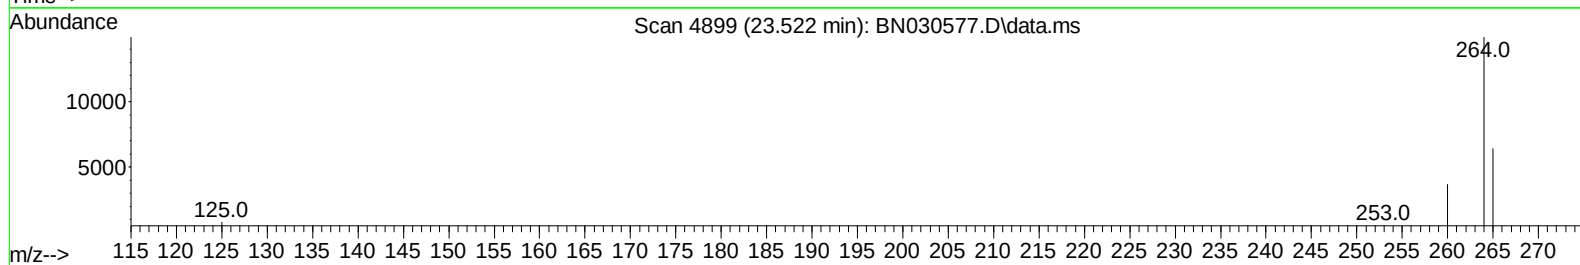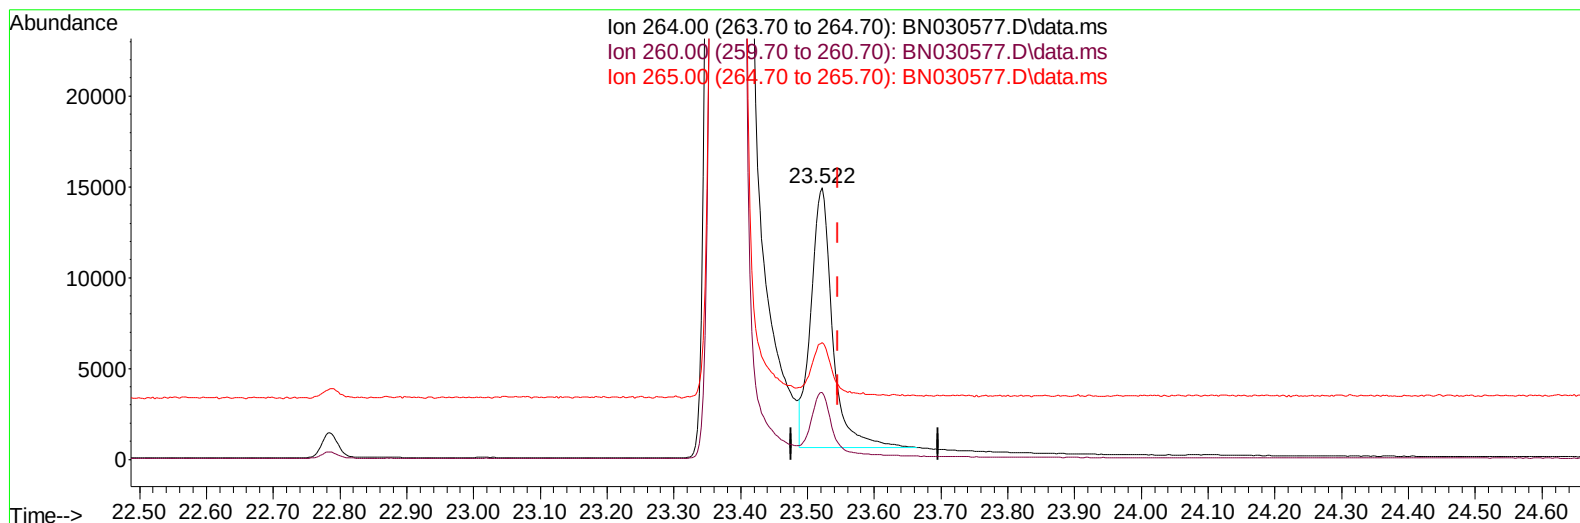

TIC: BN030577.D\data.ms

(23) Perylene-d12 (I)

23.522min (-0.024) 0.40 ng/u1

response 32443

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.73
265.00	52.70	43.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
Data File : BN030577.D
Acq On : 31 Mar 2024 13:37
Operator : MA/JU
Sample : P1929-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL6

Manual IntegrationsAPPROVED

Quant Time: Mar 31 14:11:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024

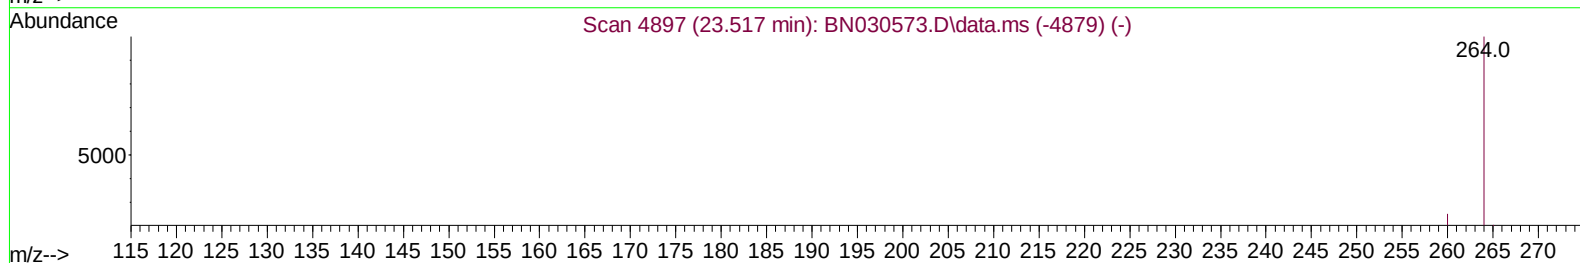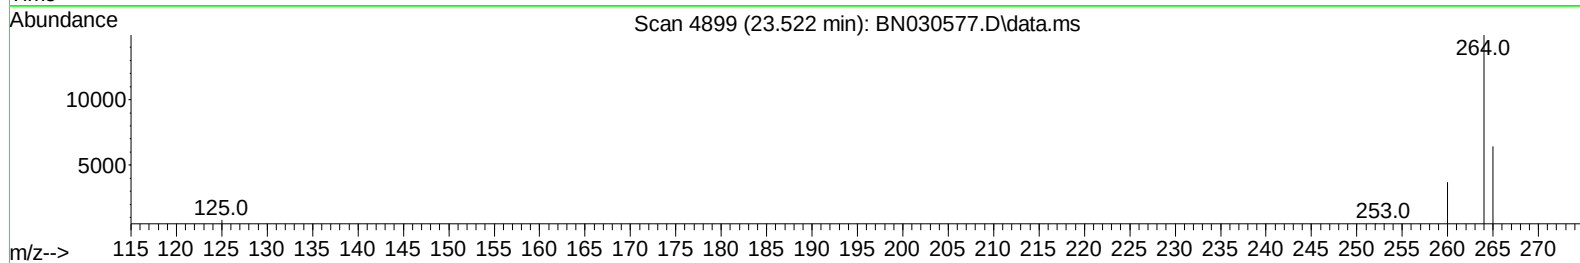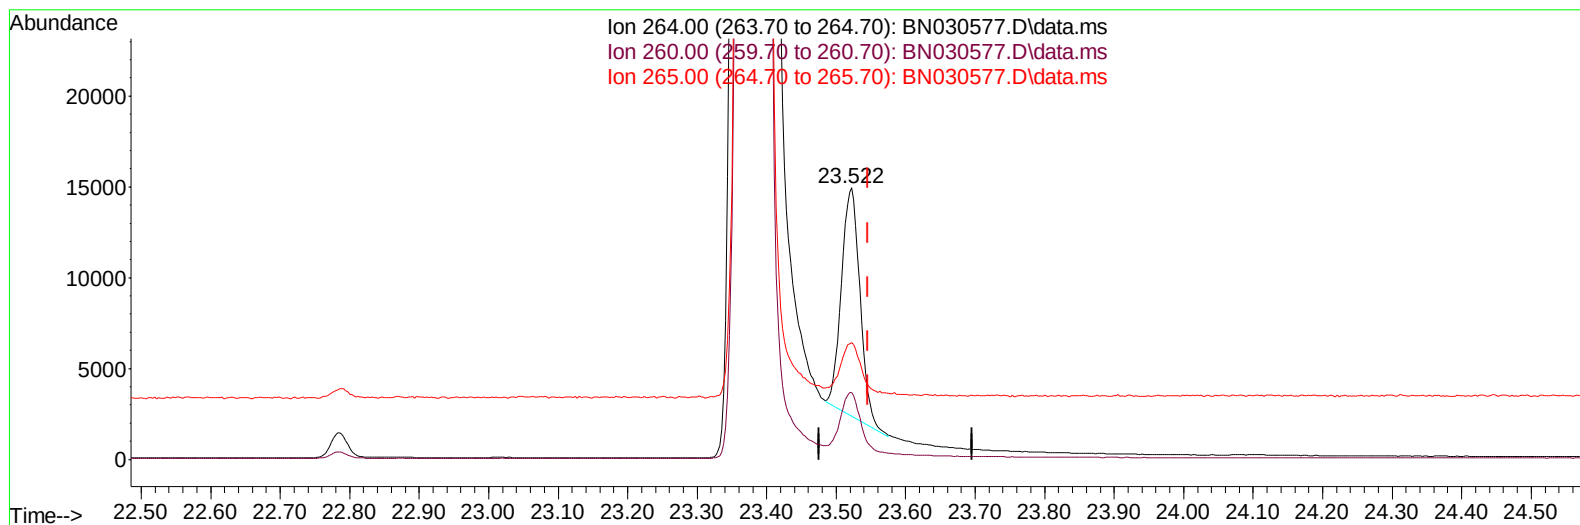

TIC: BN030577.D\data.ms

(23) Perylene-d12 (I)

23.522min (-0.024) 0.40 ng/ul m

response 23278

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.73
265.00	52.70	43.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
 Data File : BN030577.D
 Acq On : 31 Mar 2024 13:37
 Operator : MA/JU
 Sample : P1929-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Mar 31 14:11:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.700	152		8670	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.485	136		26957	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.340	164		15320	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.087	188		34485	0.400	ng/ul	-0.02
17) Chrysene-d12	21.280	240		27737	0.400	ng/ul	-0.02
23) Perylene-d12	23.522	264		23278m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.198	96		44254	4.658	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.074	152		12883	0.317	ng/ul	-0.03
18) Fluoranthene-d10	19.119	212		32145	0.375	ng/ul	-0.02
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.232	88		6685	0.694	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
Data File : BN030577.D
Acq On : 31 Mar 2024 13:37
Operator : MA/JU
Sample : P1929-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL6

Manual IntegrationsAPPROVED

Quant Time: Mar 31 14:11:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024

