

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
 Data File : BN030565.D
 Acq On : 31 Mar 2024 02:34
 Operator : MA/JU
 Sample : PB159893BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK893

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Mar 31 14:03:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.704	152	8142	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.486	136	25446	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.341	164	14663	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.092	188	33289	0.400	ng/ul	-0.02
17) Chrysene-d12	21.281	240	27893	0.400	ng/ul	-0.02
23) Perylene-d12	23.523	264	24919m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.198	96	63287	7.094	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.081	152	10492	0.274	ng/ul	-0.02
18) Fluoranthene-d10	19.124	212	24083	0.279	ng/ul	-0.01
Target Compounds						Qvalue
12) Fluorene	15.340	166	3381	0.056	ng/ul#	15

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
Data File : BN030565.D
Acq On : 31 Mar 2024 02:34
Operator : MA/JU
Sample : PB159893BL
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SBLK893

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024


Quant Time: Mar 31 14:03:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

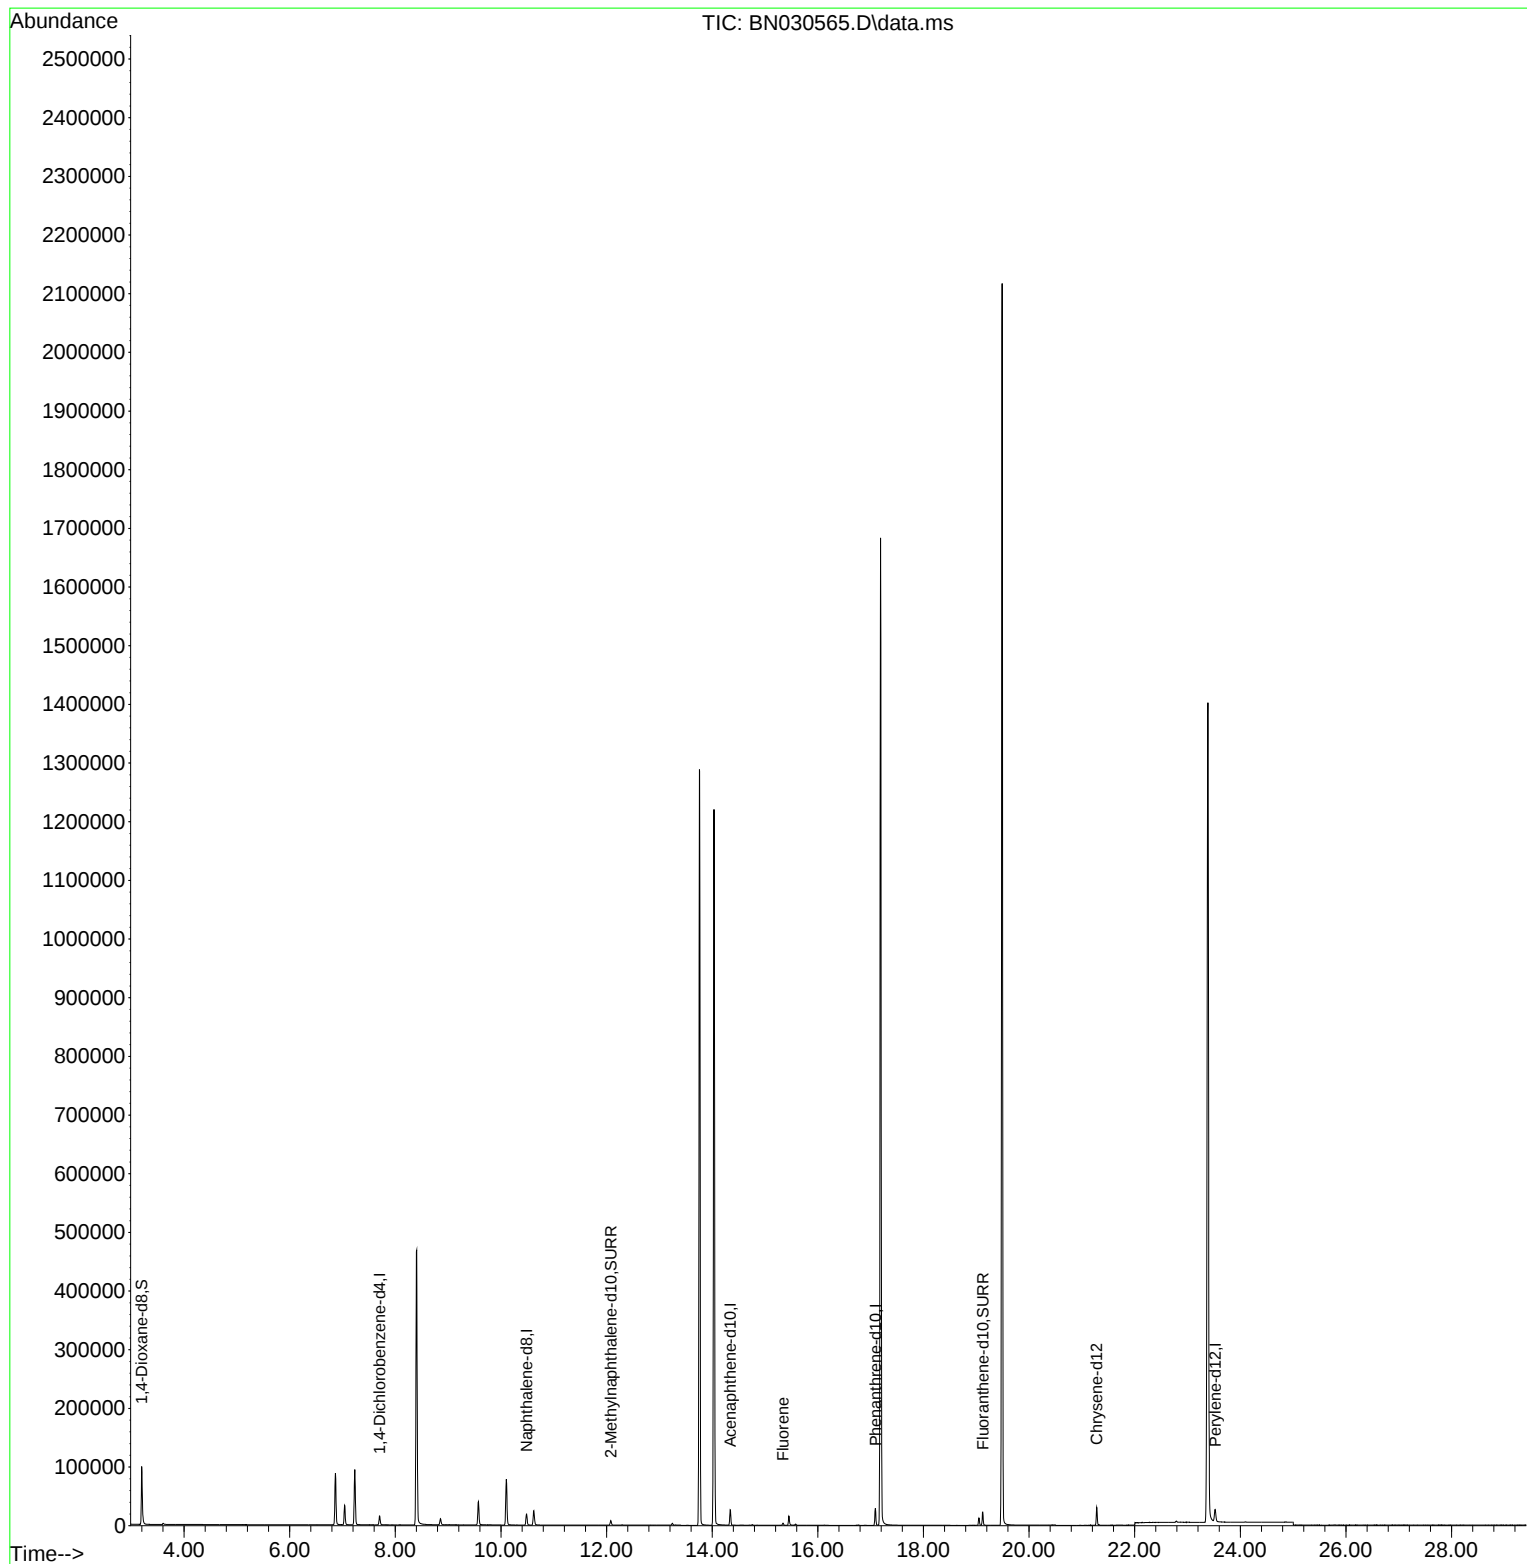

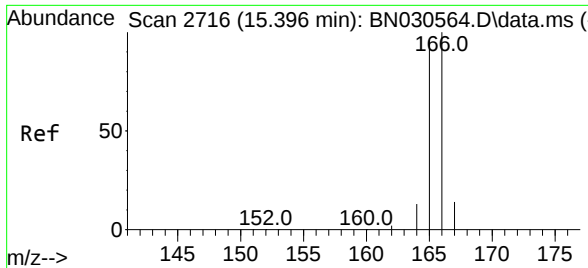

#12
 Fluorene
 Concen: 0.056 ng/ul
 RT: 15.340 min Scan# 21
 Delta R.T. -0.072 min
 Lab File: BN030565.D
 Acq: 31 Mar 2024 02:34

Instrument :
 BNA_N
 ClientSampleId :
 SBLK893

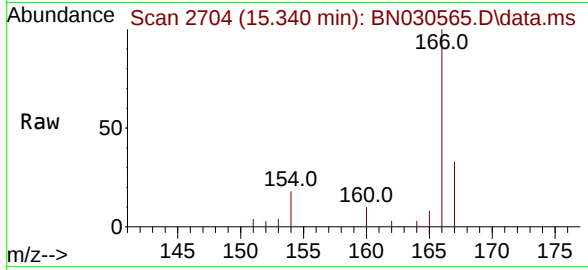

Tgt Ion:166 Resp: 338

Ion	Ratio	Lower	Upper
166	100		
165	8.4	77.5	116.3
167	33.3	11.0	16.6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

