

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
 Data File : BN030567.D
 Acq On : 31 Mar 2024 03:47
 Operator : MA/JU
 Sample : P1929-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL5

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Mar 31 14:04:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.704	152	6924	0.400	ng/u1	-0.02
4) Naphthalene-d8	10.485	136	21879	0.400	ng/u1	-0.02
9) Acenaphthene-d10	14.344	164	12646	0.400	ng/u1	-0.02
13) Phenanthrene-d10	17.091	188	28696	0.400	ng/u1	-0.02
17) Chrysene-d12	21.283	240	24327	0.400	ng/u1	-0.02
23) Perylene-d12	23.522	264	21270m	0.400	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.198	96	41917	5.525	ng/u1	-0.02
6) 2-Methylnaphthalene-d10	12.080	152	12259	0.372	ng/u1	-0.02
18) Fluoranthene-d10	19.123	212	29837	0.397	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.236	88	6599	0.858	ng/u1	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
Data File : BN030567.D
Acq On : 31 Mar 2024 03:47
Operator : MA/JU
Sample : P1929-03
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AL5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024


Quant Time: Mar 31 14:04:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

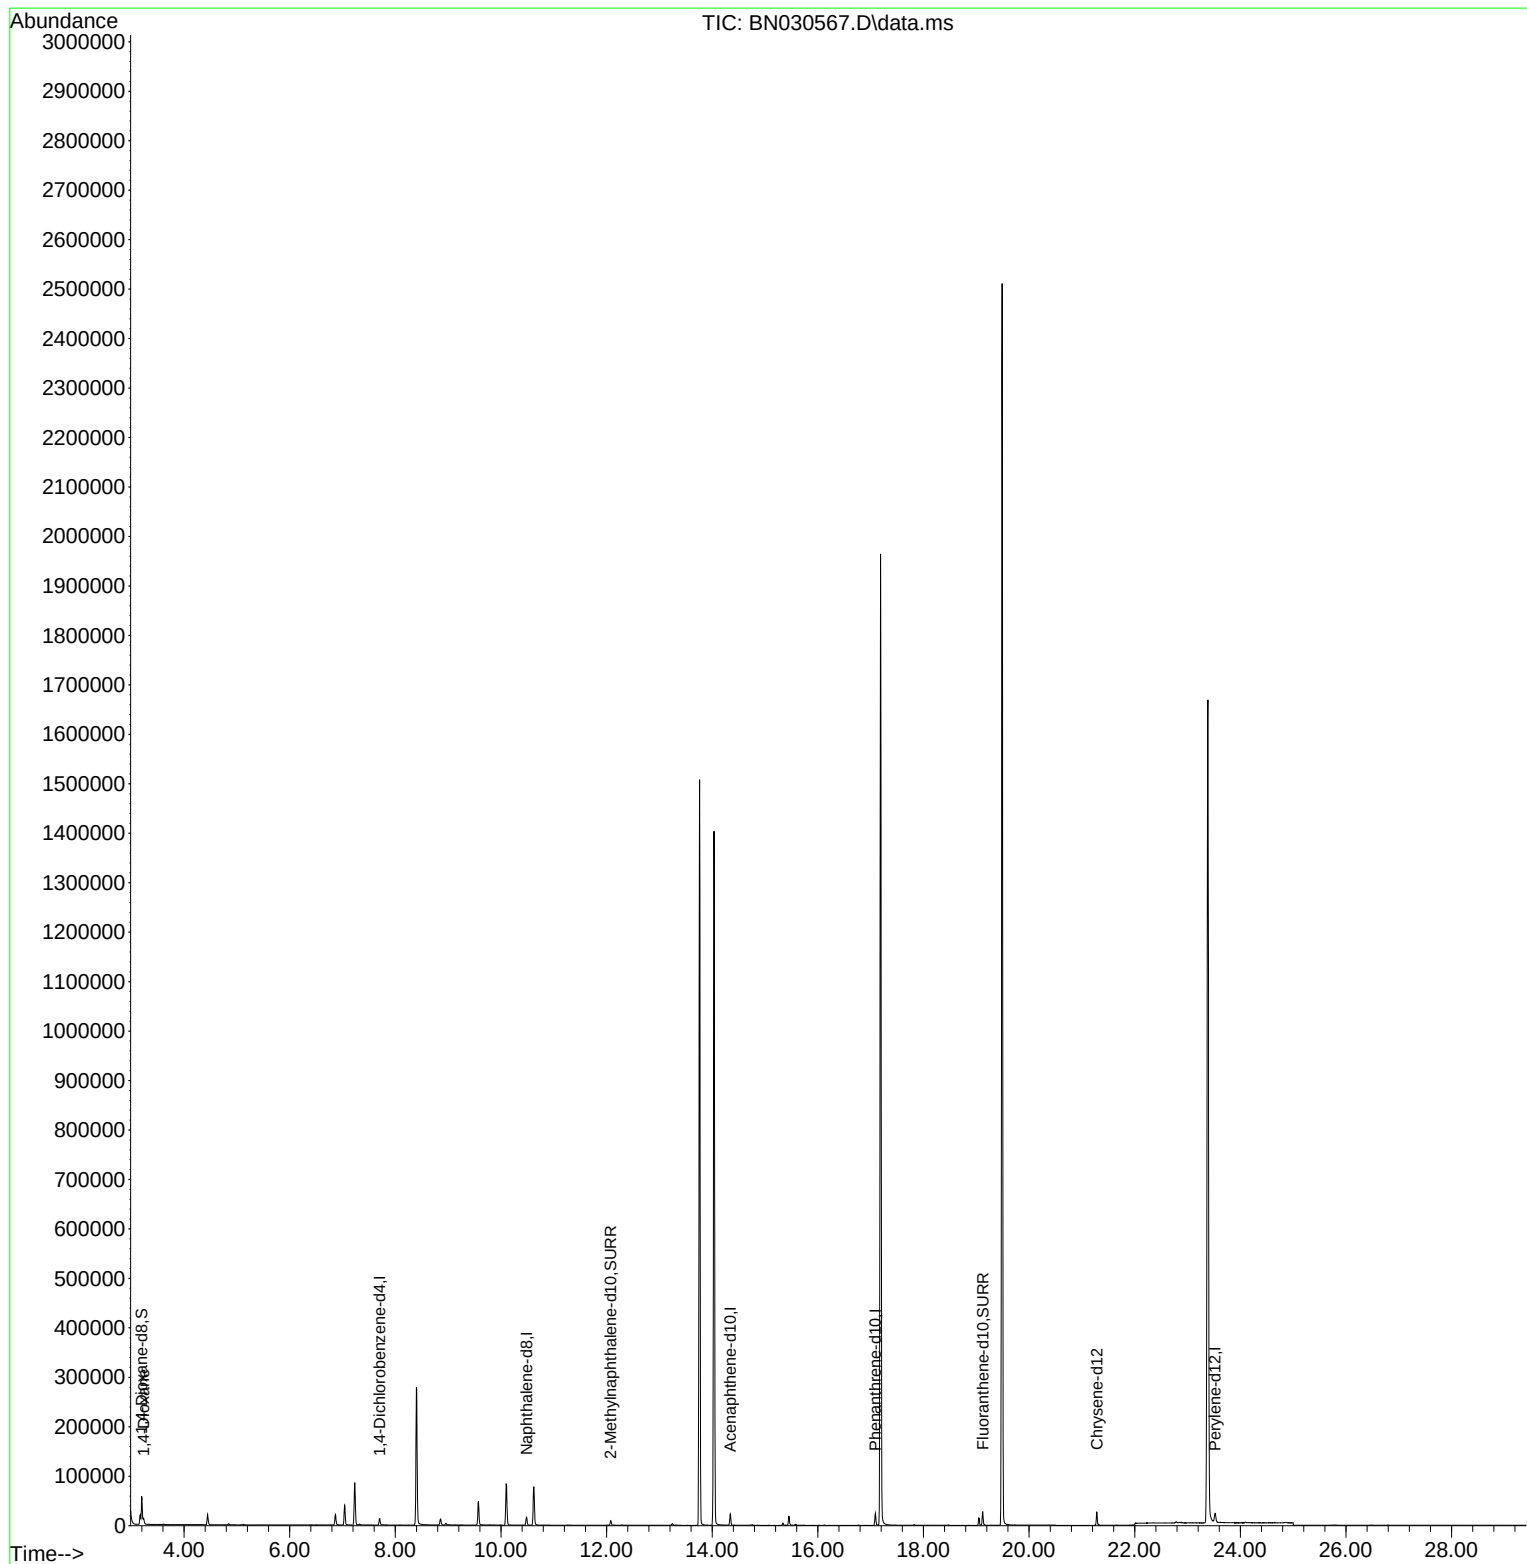

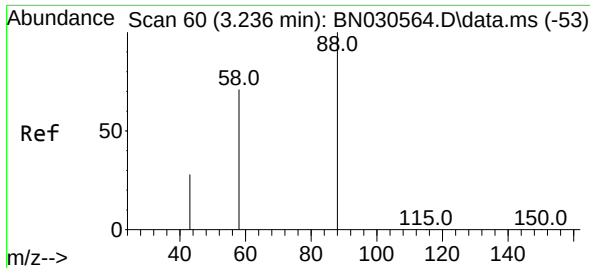

#2
 1,4-Dioxane
 Concen: 0.858 ng/ul
 RT: 3.236 min Scan# 60
 Delta R.T. -0.020 min
 Lab File: BN030567.D
 Acq: 31 Mar 2024 03:47

Instrument :
 BNA_N
 ClientSampleId :
 C0AL5

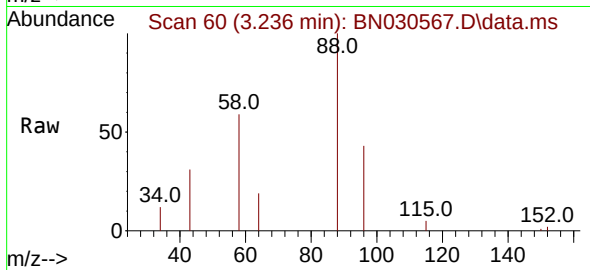

Tgt Ion: 88 Resp: 6599
 Ion Ratio Lower Upper
 88 100
 43 30.7 22.9 34.3
 58 58.7 40.3 60.5

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

