

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
 Data File : BN030577.D
 Acq On : 31 Mar 2024 13:37
 Operator : MA/JU
 Sample : P1929-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Mar 31 14:11:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 15:11:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	8670	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.485	136	26957	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.340	164	15320	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.087	188	34485	0.400	ng/ul	-0.02
17) Chrysene-d12	21.280	240	27737	0.400	ng/ul	-0.02
23) Perylene-d12	23.522	264	23278m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.198	96	44254	4.658	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.074	152	12883	0.317	ng/ul	-0.03
18) Fluoranthene-d10	19.119	212	32145	0.375	ng/ul	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.232	88	6685	0.694	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040124\
Data File : BN030577.D
Acq On : 31 Mar 2024 13:37
Operator : MA/JU
Sample : P1929-04
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AL6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024


Quant Time: Mar 31 14:11:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 15:11:42 2024
Response via : Initial Calibration

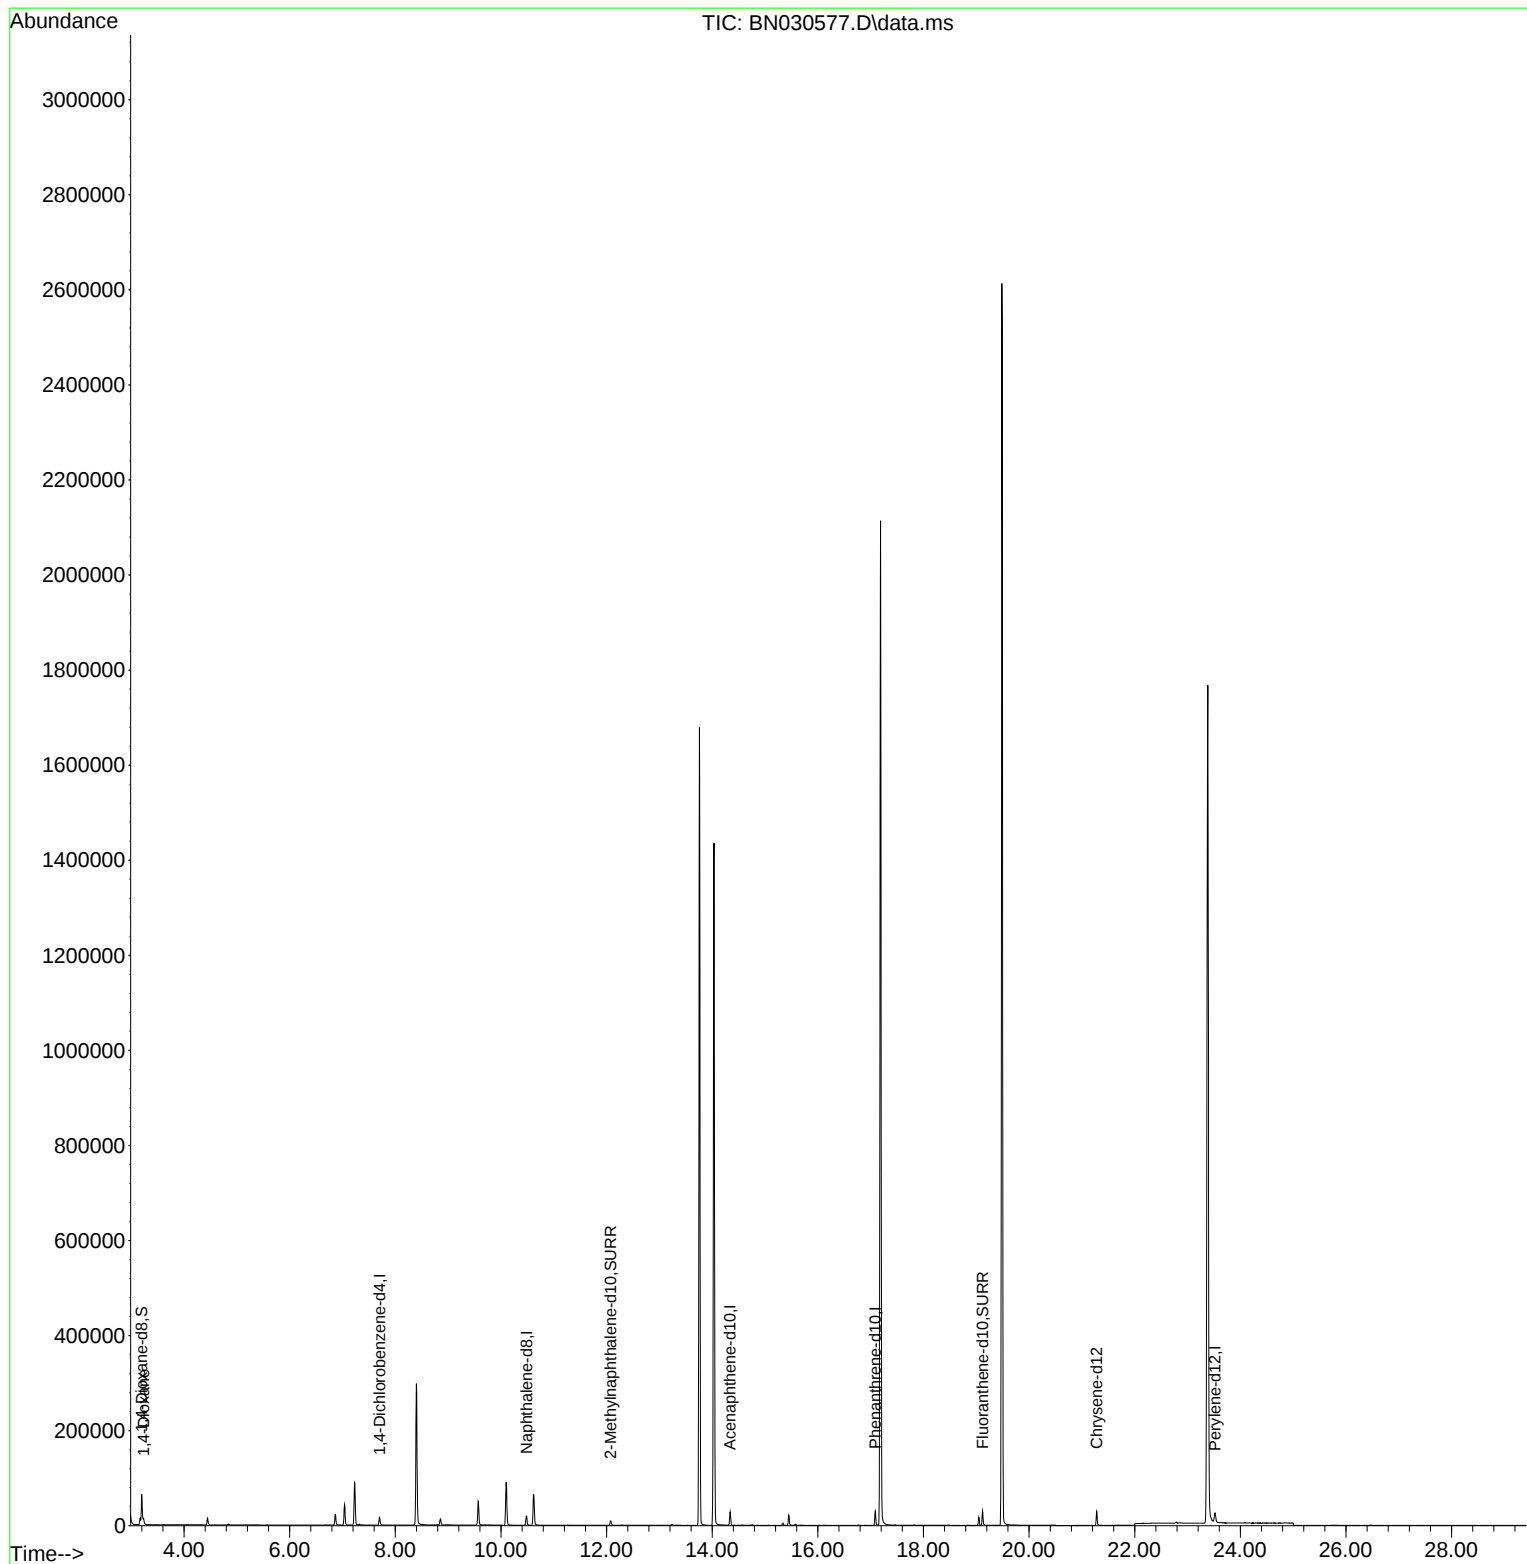

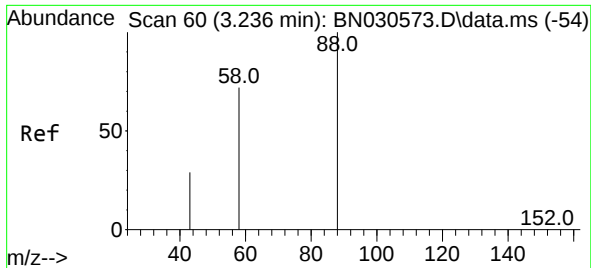

#2
 1,4-Dioxane
 Concen: 0.694 ng/ul
 RT: 3.232 min Scan# 59
 Delta R.T. -0.024 min
 Lab File: BN030577.D
 Acq: 31 Mar 2024 13:37

Instrument :
 BNA_N
 ClientSampleId :
 C0AL6

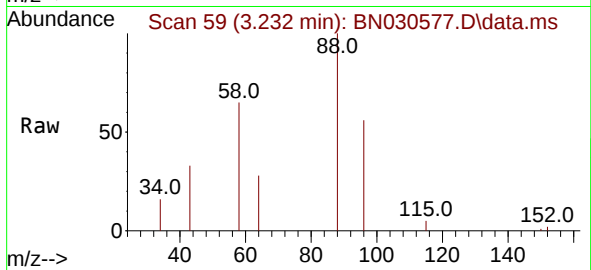

Tgt Ion: 88 Resp: 668
 Ion Ratio Lower Upper
 88 100
 43 32.5 22.9 34.3
 58 65.3 40.3 60.5

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

