


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040219\
 Data File : BN005052.D
 Acq On : 02 Apr 2019 09:16
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 29 03:42:17 2019

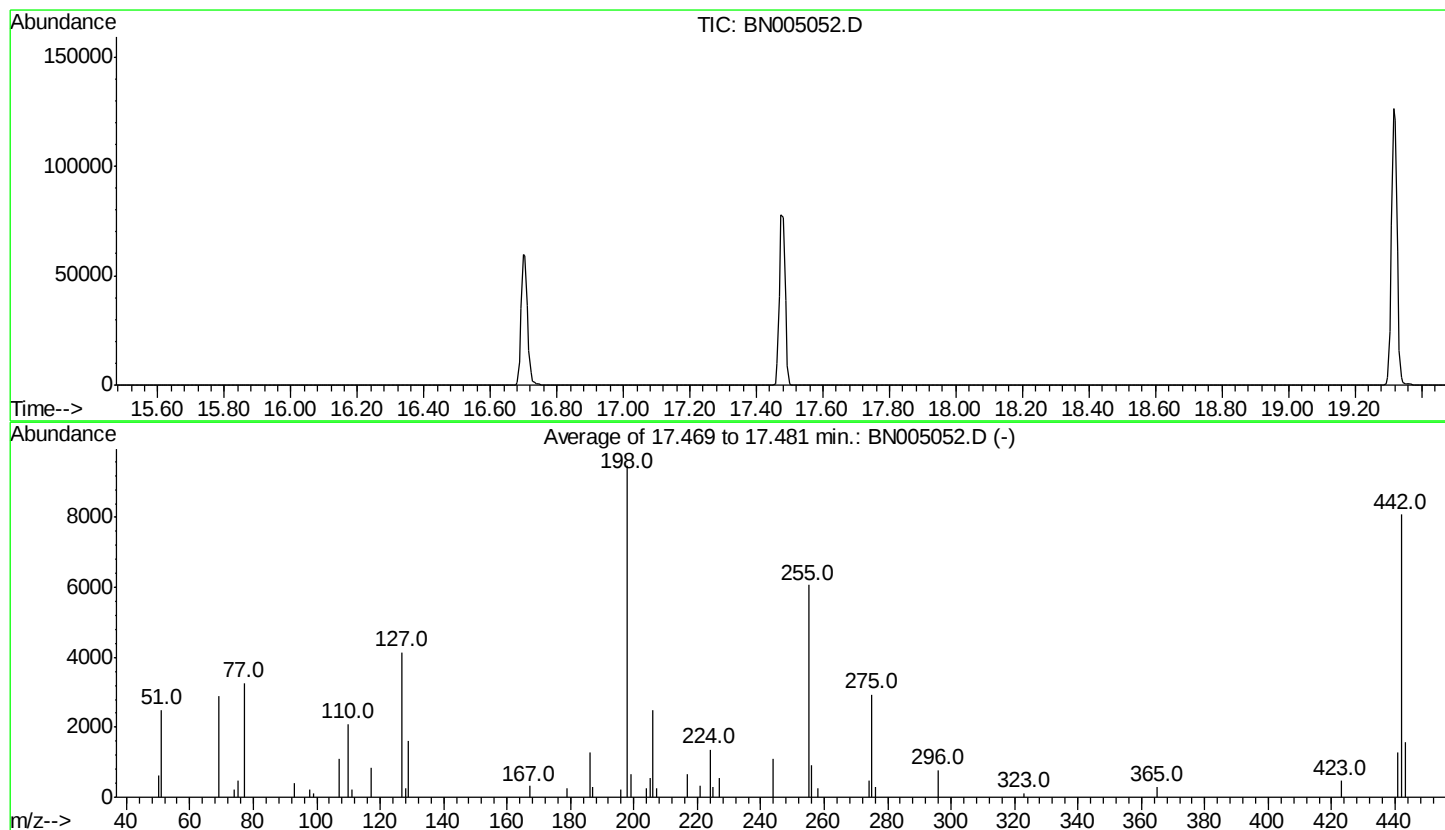

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.3	2498	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.5	2892	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.7	4148	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9483	PASS
199	198	5	9	6.9	655	PASS
275	198	10	60	31.0	2944	PASS
365	198	1	100	3.3	312	PASS
441	198	0.01	100	13.6	1285	PASS
442	198	50	100	85.2	8076	PASS
443	442	15	24	19.4	1570	PASS