

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040319\
 Data File : BN005071.D
 Acq On : 03 Apr 2019 21:16
 Operator : JU/SJ
 Sample : K1695-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DPC-91723-SO-TP5-B

Quant Time: Apr 04 04:29:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 05:27:09 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	10201	20.00	ng	-0.02
21) Naphthalene-d8	10.44	136	40119	20.00	ng	-0.02
39) Acenaphthene-d10	14.30	164	22612	20.00	ng	-0.02
64) Phenanthrene-d10	17.05	188	49004	20.00	ng	-0.02
76) Chrysene-d12	21.25	240	45526	20.00	ng	-0.02
87) Perylene-d12	23.48	264	43235	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	70940	120.23	ng	-0.02
7) Phenol-d6	6.83	99	84796	108.35	ng	-0.02
23) Nitrobenzene-d5	8.82	82	56673	85.45	ng	-0.02
42) 2,4,6-Tribromophenol	15.80	330	52459	143.85	ng	-0.02
45) 2-Fluorobiphenyl	12.92	172	147444	86.41	ng	-0.02
79) Terphenyl-d14	19.69	244	230846	97.62	ng	-0.02
Target Compounds						
4) n-Nitrosodimethylamine	3.19	42	510	2.604	ng	# 1
19) n-Nitroso-di-n-propylamine	8.82	70	7177	13.989	ng	# 75
51) 2,6-Dinitrotoluene	14.30	165	2751	6.508	ng	# 29
57) 2,4-Dinitrotoluene	14.30	165	2751	4.789	ng	# 27
67) 4-Bromophenyl-phenylether	15.80	248	3063	5.009	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040319\
Data File : BN005071.D
Acq On : 03 Apr 2019 21:16
Operator : JU/SJ
Sample : K1695-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DPC-91723-SO-TP5-B

Quant Time: Apr 04 04:29:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

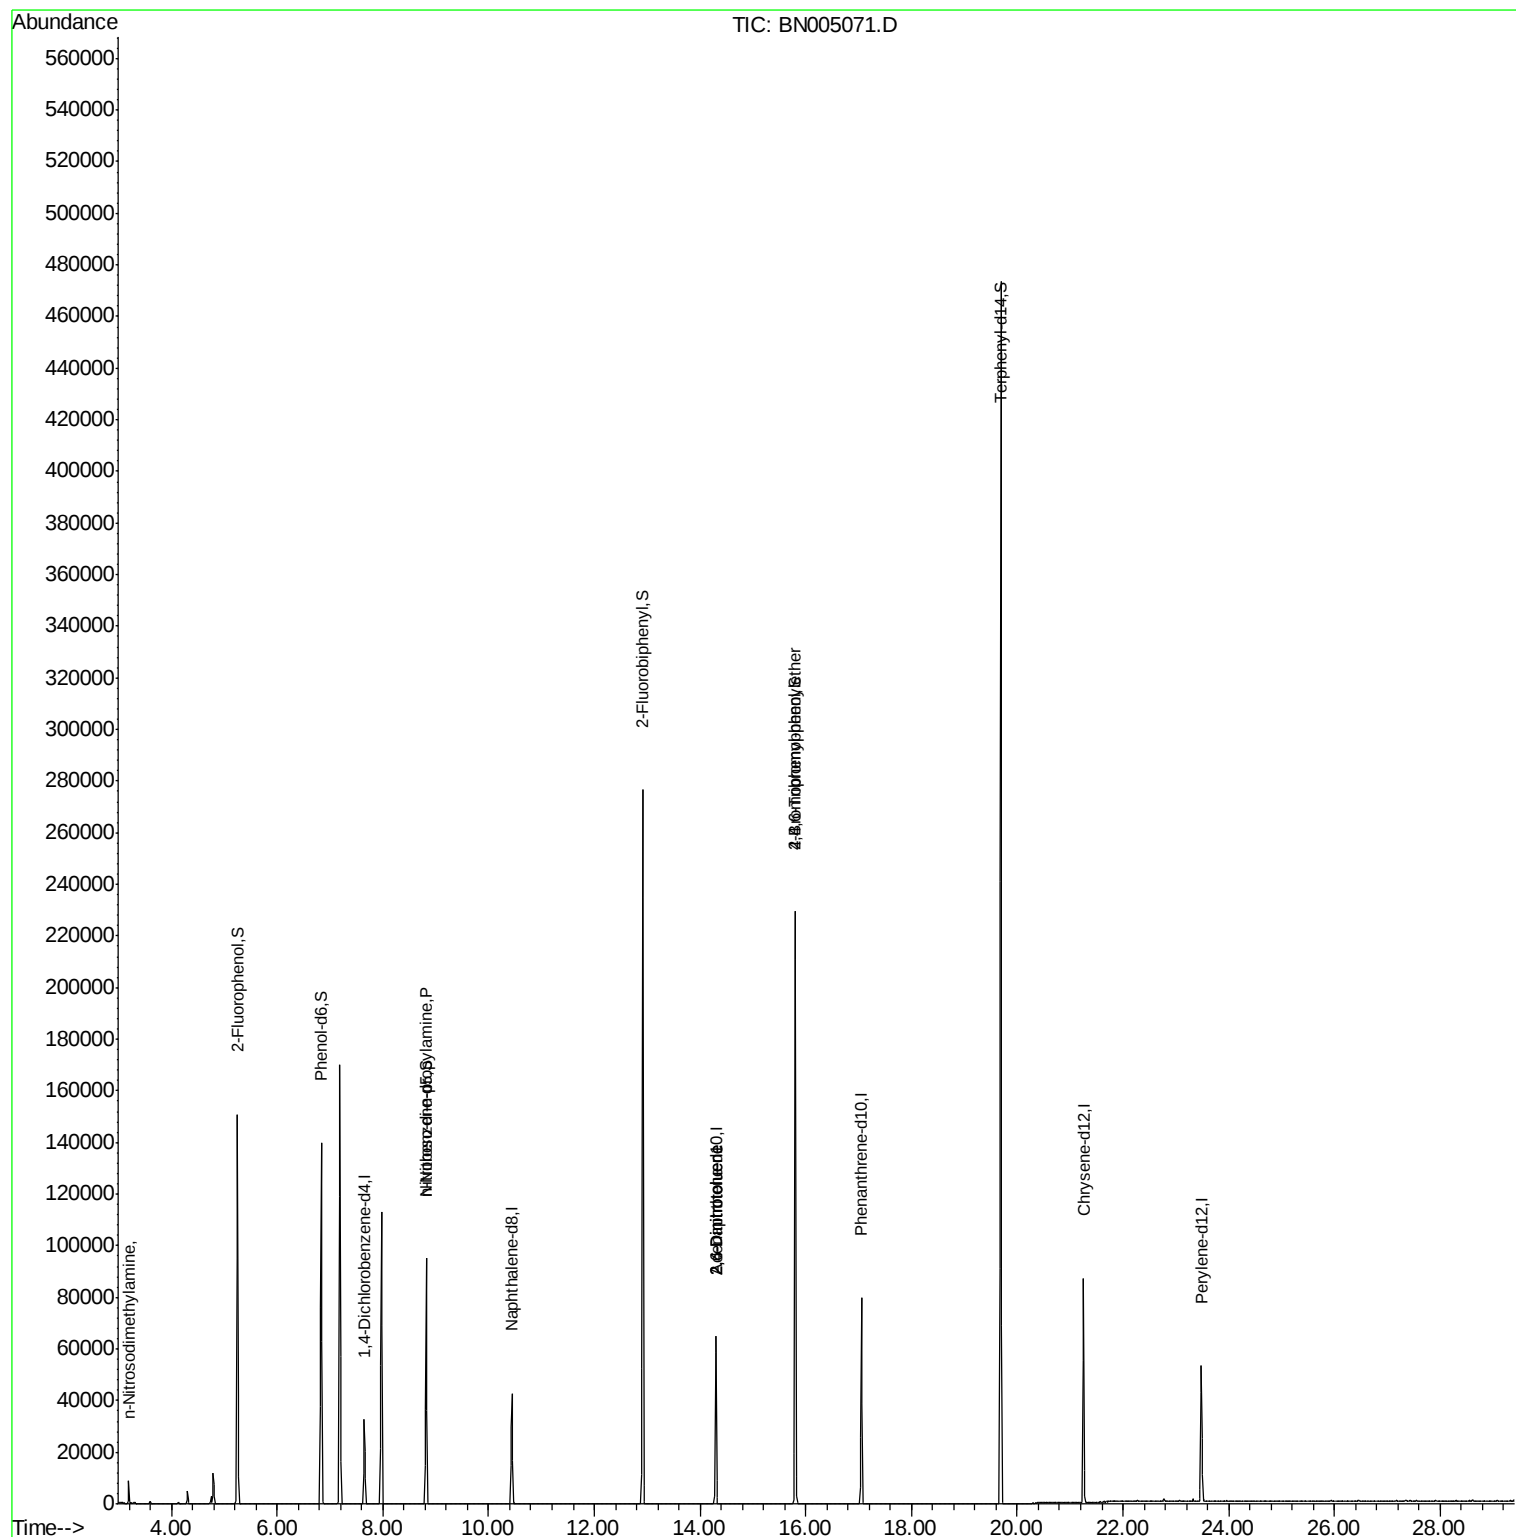


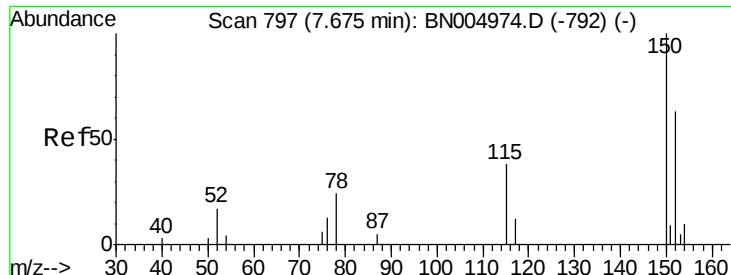




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.65 min Scan# 793
 Delta R.T. -0.02 min
 Lab File: BN005071.D
 Acq: 03 Apr 2019 21:16

Instrument :
 BNA_N
 ClientSampleId :
 DPC-91723-SO-TP5-B

Tgt Ion: 152 Resp: 10201
 Ion Ratio Lower Upper
 152 100
 150 155.2 126.9 190.3
 115 60.0 47.8 71.6

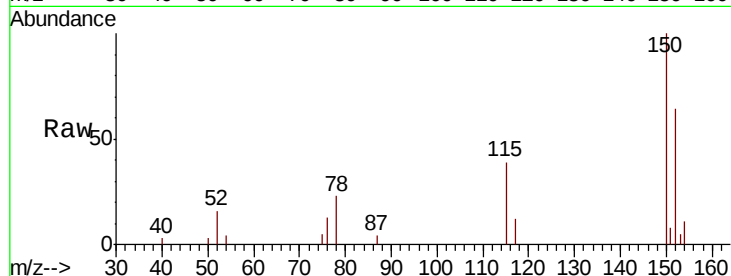


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E


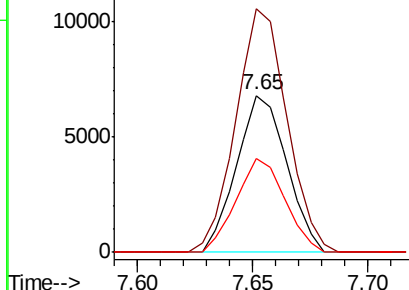



#4
 n-Nitrosodimethylamine
 Concen: 2.604 ng
 RT: 3.19 min Scan# 35
 Delta R.T. -0.33 min
 Lab File: BN005071.D
 Acq: 03 Apr 2019 21:16

Tgt Ion: 42 Resp: 510
 Ion Ratio Lower Upper
 42 100
 74 0.0 130.8 196.2#
 44 0.0 5.7 8.5#

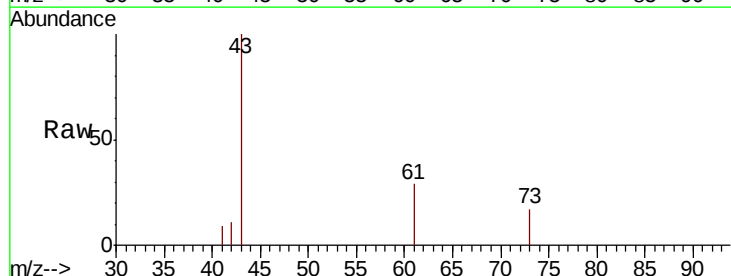

Abundance Ion 42.00 (41.70 to 42.70): BNC
 Ion 74.00 (73.70 to 74.70): BNC
 Ion 44.00 (43.70 to 44.70): BNC

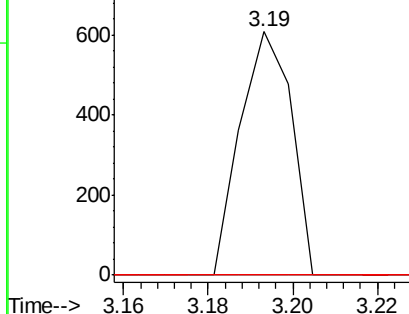



#5

2-Fluorophenol

Concen: 120.231 ng

RT: 5.25 min Scan# 385

Delta R.T. -0.02 min

Lab File: BN005071.D

Acq: 03 Apr 2019 21:16

Instrument :

BNA_N

ClientSampleId :

DPC-91723-SO-TP5-B


Tgt Ion: 112 Resp: 70940

Ion Ratio Lower Upper

112 100

64 49.8 41.9 62.9




63 25.0 21.4 32.0



Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

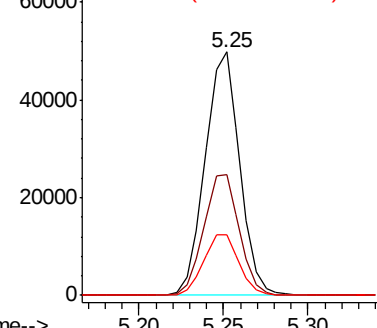

#7

Phenol-d6

Concen: 108.354 ng

RT: 6.83 min Scan# 654

Delta R.T. -0.02 min

Lab File: BN005071.D

Acq: 03 Apr 2019 21:16


Tgt Ion: 99 Resp: 84796

Ion Ratio Lower Upper

99 100

42 13.8 11.4 17.0



71 31.8 25.8 38.8




Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

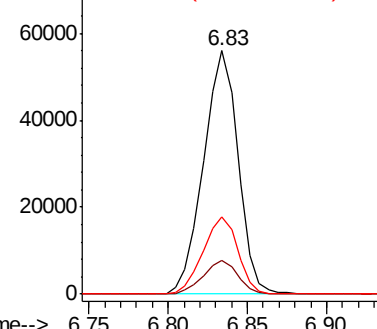

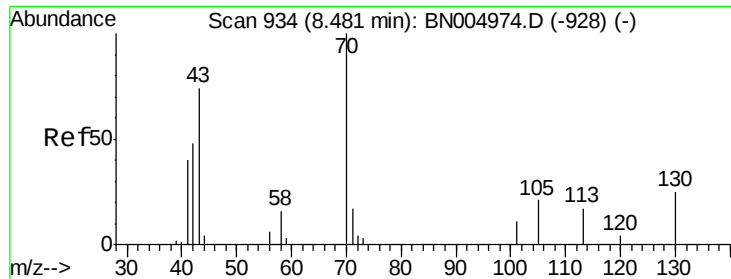

#19

n-Nitroso-di-n-propylamine

Concen: 13.989 ng

RT: 8.82 min Scan# 992

Delta R.T. 0.34 min

Lab File: BN005071.D

Acq: 03 Apr 2019 21:16

Instrument :

BNA_N

ClientSampleId :

DPC-91723-SO-TP5-B

Tgt Ion: 70 Resp: 7177



Ion Ratio Lower Upper

70 100

42 40.0 38.4 57.6

101 0.0 8.8 13.2#

130 0.0 19.8 29.8#


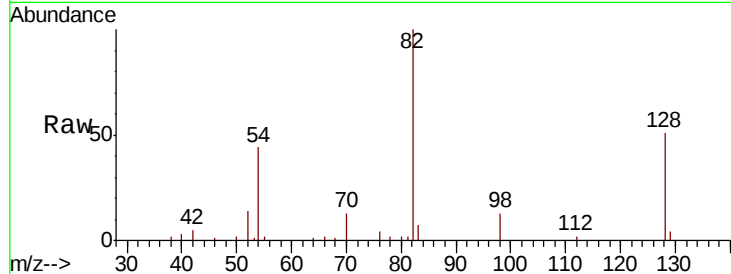


Abundance Ion 70.00 (69.70 to 70.70): BN0

Ion 42.00 (41.70 to 42.70): BN0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

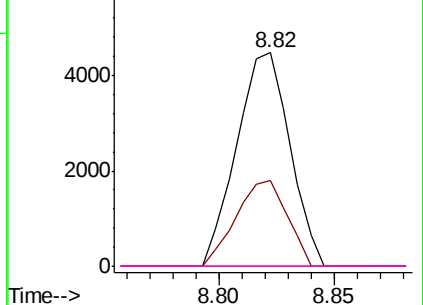

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.44 min Scan# 1267

Delta R.T. -0.02 min

Lab File: BN005071.D

Acq: 03 Apr 2019 21:16

Tgt Ion: 136 Resp: 40119



Ion Ratio Lower Upper

136 100

137 10.7 8.9 13.3

54 6.3 5.3 7.9

68 5.1 4.6 6.8

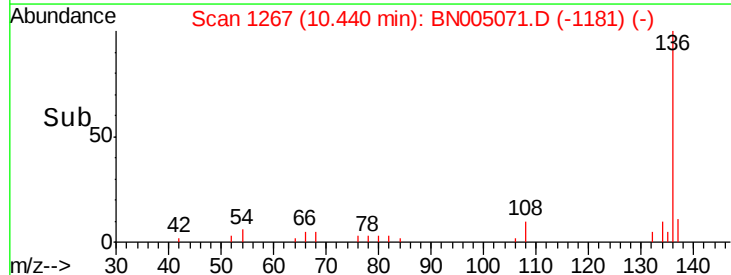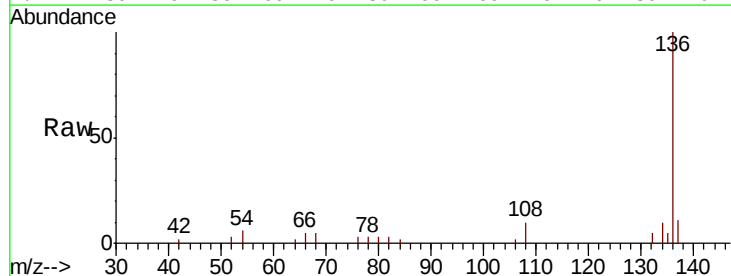



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BN0

Ion 68.00 (67.70 to 68.70): BN0

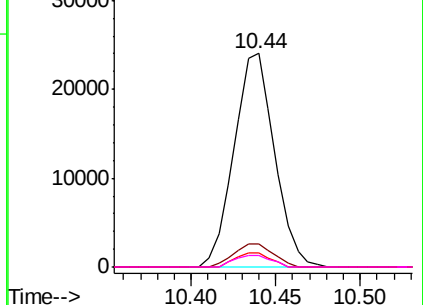


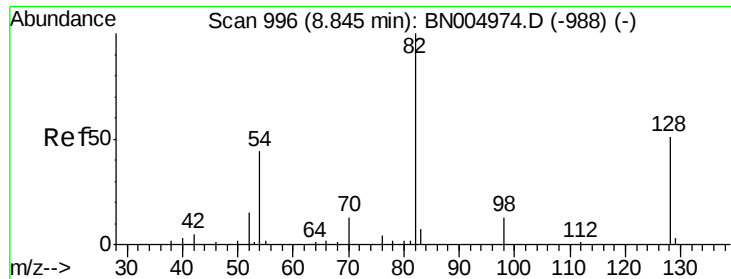




#23
 Nitrobenzene-d5
 Concen: 85.452 ng
 RT: 8.82 min Scan# 992
 Delta R.T. -0.02 min
 Lab File: BN005071.D
 Acq: 03 Apr 2019 21:16

Instrument :
 BNA_N
 ClientSampleId :
 DPC-91723-SO-TP5-B

Tgt Ion: 82 Resp: 56673
 Ion Ratio Lower Upper
 82 100
 128 50.9 40.6 60.8
 54 44.1 35.2 52.8

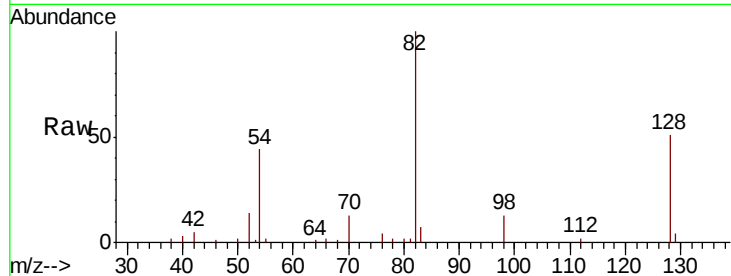


Abundance Ion 82.00 (81.70 to 82.70): BN0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BN0

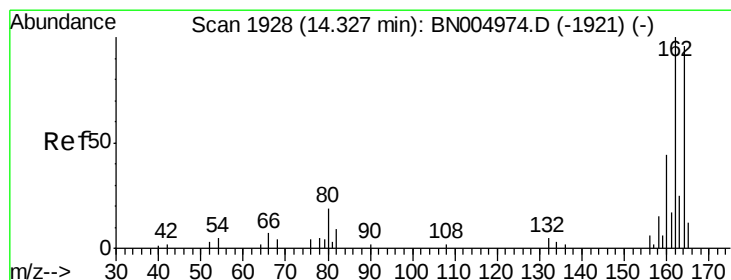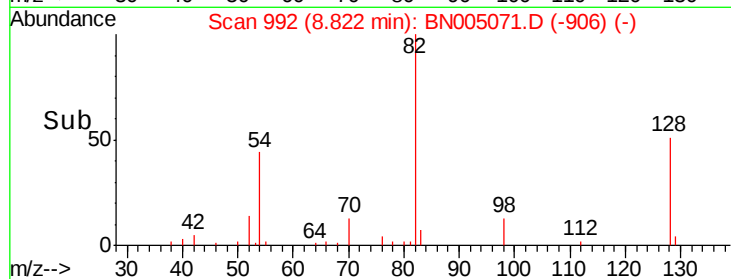
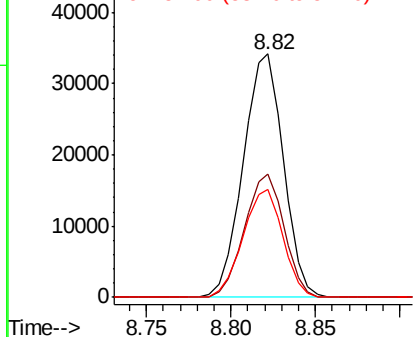



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.30 min Scan# 1924
 Delta R.T. -0.02 min
 Lab File: BN005071.D
 Acq: 03 Apr 2019 21:16

Tgt Ion: 164 Resp: 22612
 Ion Ratio Lower Upper
 164 100
 162 107.0 83.4 125.0
 160 46.3 36.6 55.0



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

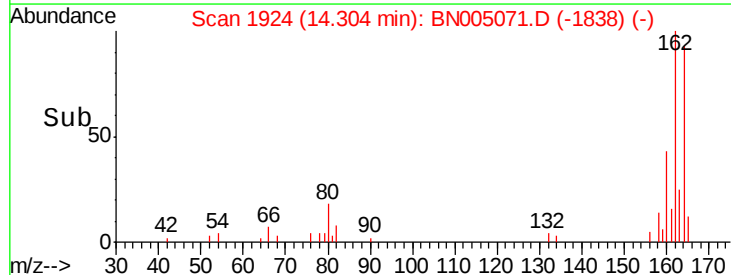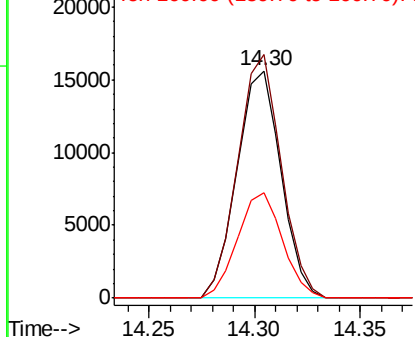


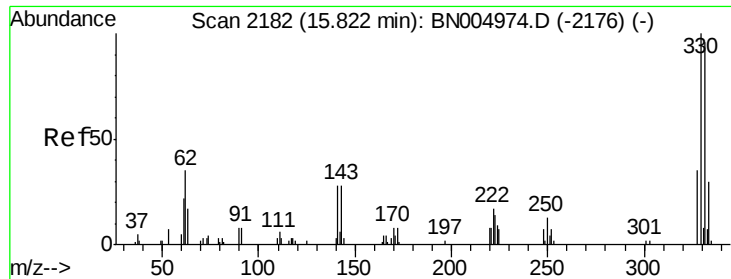




#42
 2,4,6-Tribromophenol
 Concen: 143.846 ng
 RT: 15.80 min Scan# 2178
 Delta R.T. -0.02 min
 Lab File: BN005071.D
 Acq: 03 Apr 2019 21:16

Instrument :
 BNA_N
 ClientSampleId :
 DPC-91723-SO-TP5-B

Tgt Ion:330 Resp: 52459
 Ion Ratio Lower Upper
 330 100
 332 96.0 77.4 116.0
 141 24.7 22.1 33.1




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

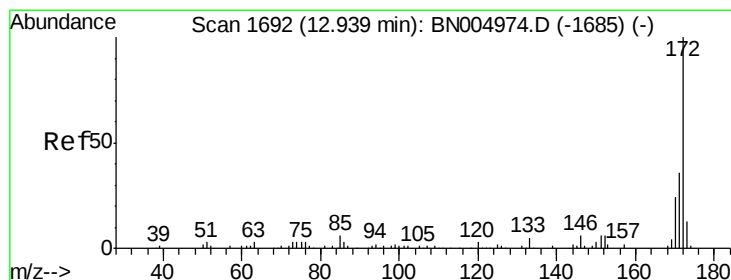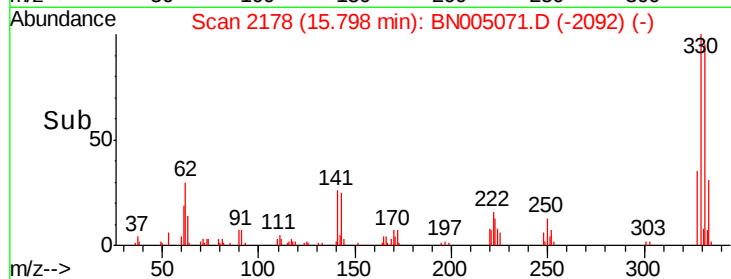
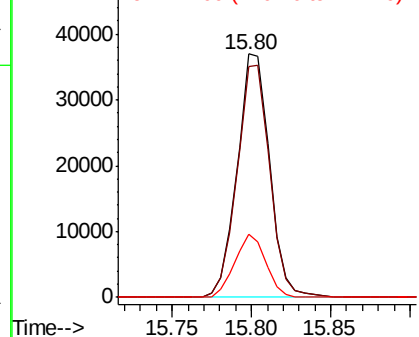



#45
 2-Fluorobiphenyl
 Concen: 86.406 ng
 RT: 12.92 min Scan# 1688
 Delta R.T. -0.02 min
 Lab File: BN005071.D
 Acq: 03 Apr 2019 21:16

Tgt Ion:172 Resp: 147444
 Ion Ratio Lower Upper
 172 100
 171 36.1 28.6 42.8
 170 23.4 18.9 28.3

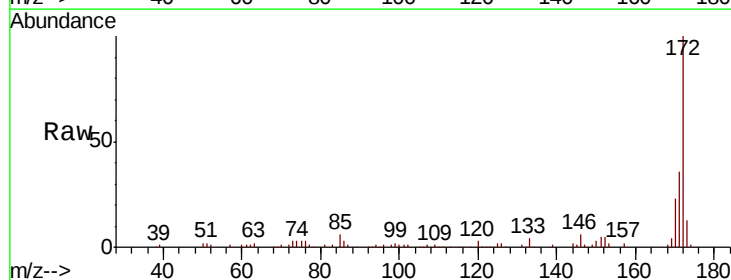

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

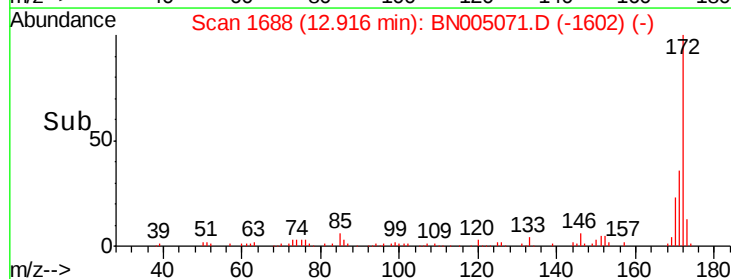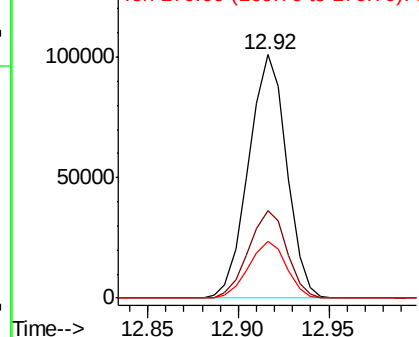


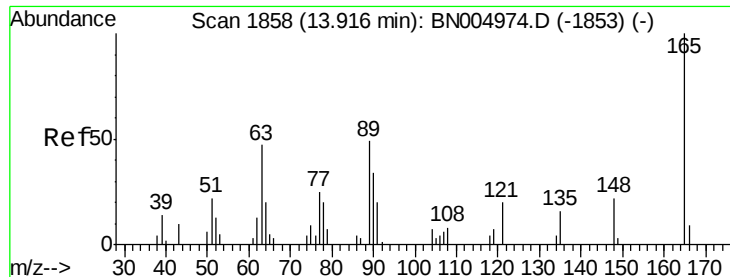

#51
 2,6-Dinitrotoluene
 Concen: 6.508 ng
 RT: 14.30 min Scan# 1924
 Delta R.T. 0.39 min
 Lab File: BN005071.D
 Acq: 03 Apr 2019 21:16

Instrument :
 BNA_N
 ClientSampleId :
 DPC-91723-SO-TP5-B




Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	37.3	55.9#
89	0.0	39.2	58.8#

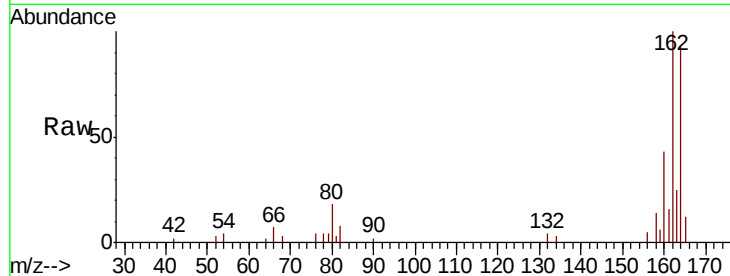

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BNC

Ion 89.00 (88.70 to 89.70): BNC

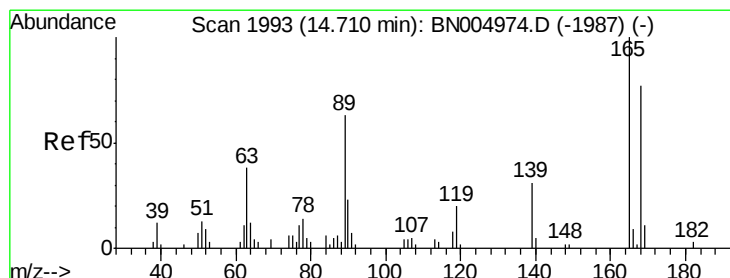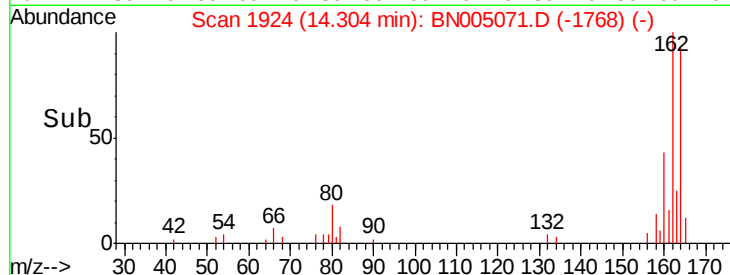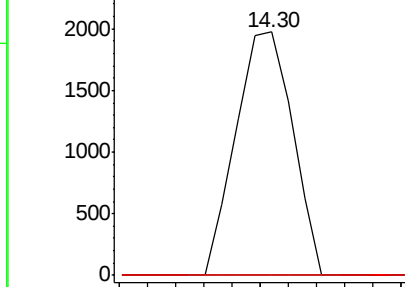

#57
 2,4-Dinitrotoluene
 Concen: 4.789 ng
 RT: 14.30 min Scan# 1924
 Delta R.T. -0.41 min
 Lab File: BN005071.D
 Acq: 03 Apr 2019 21:16




Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	30.4	45.6#
89	0.0	50.7	76.1#
182	0.0	2.5	3.7#


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BNC

Ion 89.00 (88.70 to 89.70): BNC

Ion 182.00 (181.70 to 182.70): E

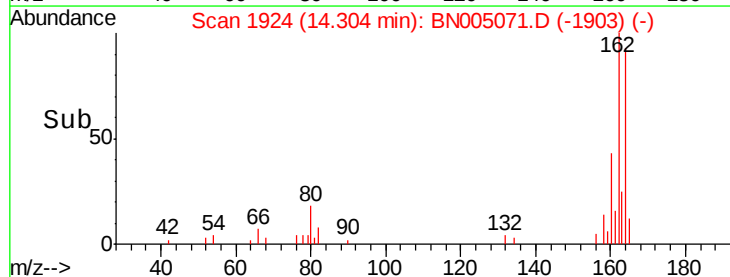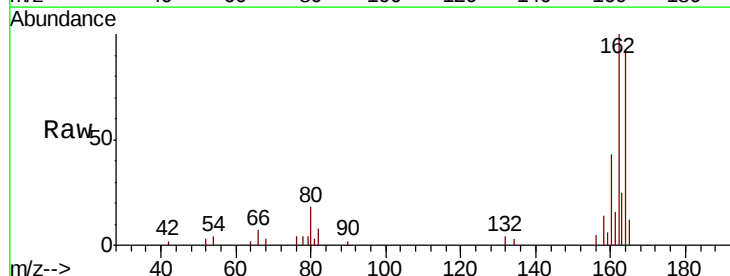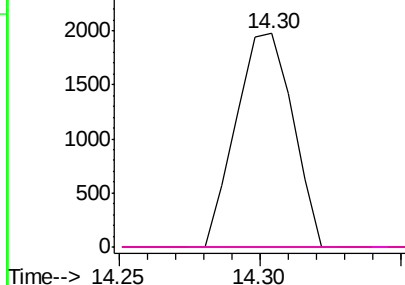



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.05 min Scan# 2391

Delta R.T. -0.02 min

Lab File: BN005071.D

Acq: 03 Apr 2019 21:16

Instrument :

BNA_N

ClientSampleId :

DPC-91723-SO-TP5-B


Tgt Ion:188 Resp: 49004

Ion Ratio Lower Upper

188 100

94 8.9 7.2 10.8




80 9.8 7.8 11.6

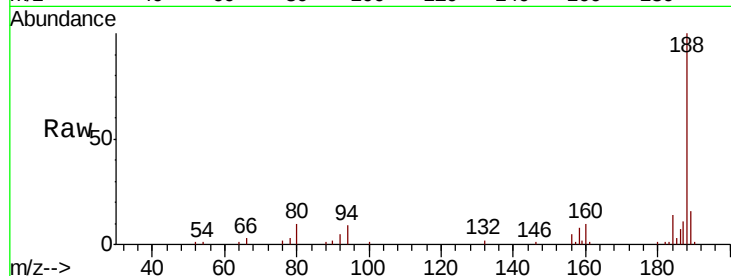

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

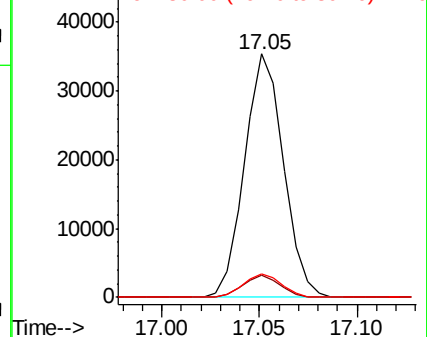

#67

4-Bromophenyl-phenylether

Concen: 5.009 ng

RT: 15.80 min Scan# 2178

Delta R.T. -0.47 min

Lab File: BN005071.D

Acq: 03 Apr 2019 21:16


Tgt Ion:248 Resp: 3063

Ion Ratio Lower Upper

248 100

250 199.3 79.4 119.2#



141 405.4 52.3 78.5#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

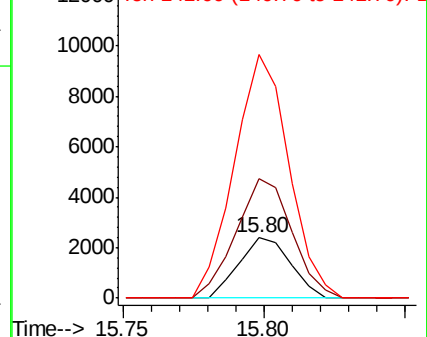


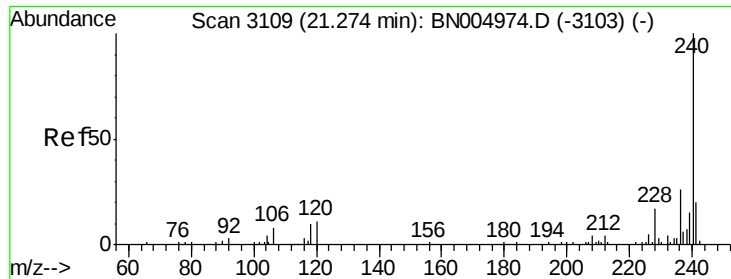




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.25 min Scan# 3105
Delta R.T. -0.02 min
Lab File: BN005071.D
Acq: 03 Apr 2019 21:16

Instrument :
BNA_N
ClientSampleId :
DPC-91723-SO-TP5-B

Tgt Ion:240 Resp: 45526
Ion Ratio Lower Upper
240 100
120 10.2 8.5 12.7
236 25.5 21.2 31.8

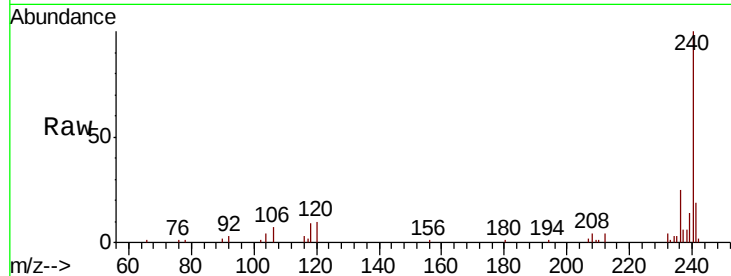


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E


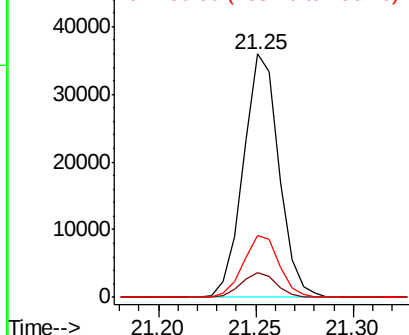



#79
Terphenyl-d14
Concen: 97.622 ng
RT: 19.69 min Scan# 2840
Delta R.T. -0.02 min
Lab File: BN005071.D
Acq: 03 Apr 2019 21:16

Tgt Ion:244 Resp: 230846
Ion Ratio Lower Upper
244 100
212 6.6 5.4 8.0
122 9.2 7.4 11.2



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

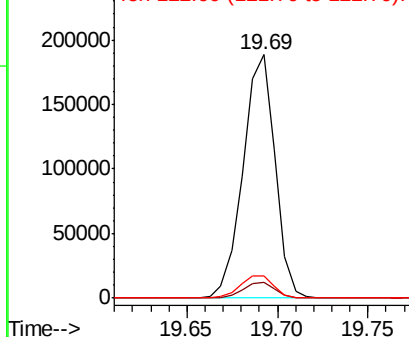

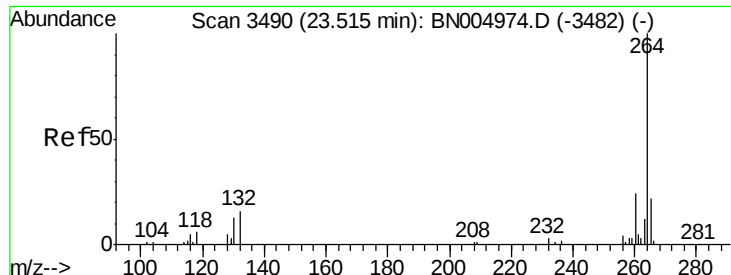

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.48 min Scan# 3484
Delta R.T. -0.04 min
Lab File: BN005071.D
Acq: 03 Apr 2019 21:16

Instrument :
BNA_N
ClientSampleId :
DPC-91723-SO-TP5-B

Tgt Ion:	264	Resp:	43235
Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.0	28.4
265	21.7	17.2	25.8

