

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040319\
 Data File : BN005086.D
 Acq On : 04 Apr 2019 09:52
 Operator : JU/SJ
 Sample : PB118559BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118559BL

Quant Time: Apr 04 16:06:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 14:56:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	6762	20.00	ng	0.00
21) Naphthalene-d8	10.43	136	26738	20.00	ng	0.00
39) Acenaphthene-d10	14.30	164	16432	20.00	ng	0.00
64) Phenanthrene-d10	17.05	188	39655	20.00	ng	0.00
76) Chrysene-d12	21.25	240	47327	20.00	ng	0.00
87) Perylene-d12	23.48	264	49021	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	27407	70.07	ng	0.00
7) Phenol-d6	6.83	99	34280	66.08	ng	0.00
23) Nitrobenzene-d5	8.82	82	28830	65.22	ng	0.00
42) 2,4,6-Tribromophenol	15.80	330	15140	57.13	ng	0.00
45) 2-Fluorobiphenyl	12.91	172	85342	68.82	ng	0.00
79) Terphenyl-d14	19.69	244	148229	60.30	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040319\
Data File : BN005086.D
Acq On : 04 Apr 2019 09:52
Operator : JU/SJ
Sample : PB118559BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118559BL

Quant Time: Apr 04 16:06:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 14:56:07 2019
Response via : Initial Calibration

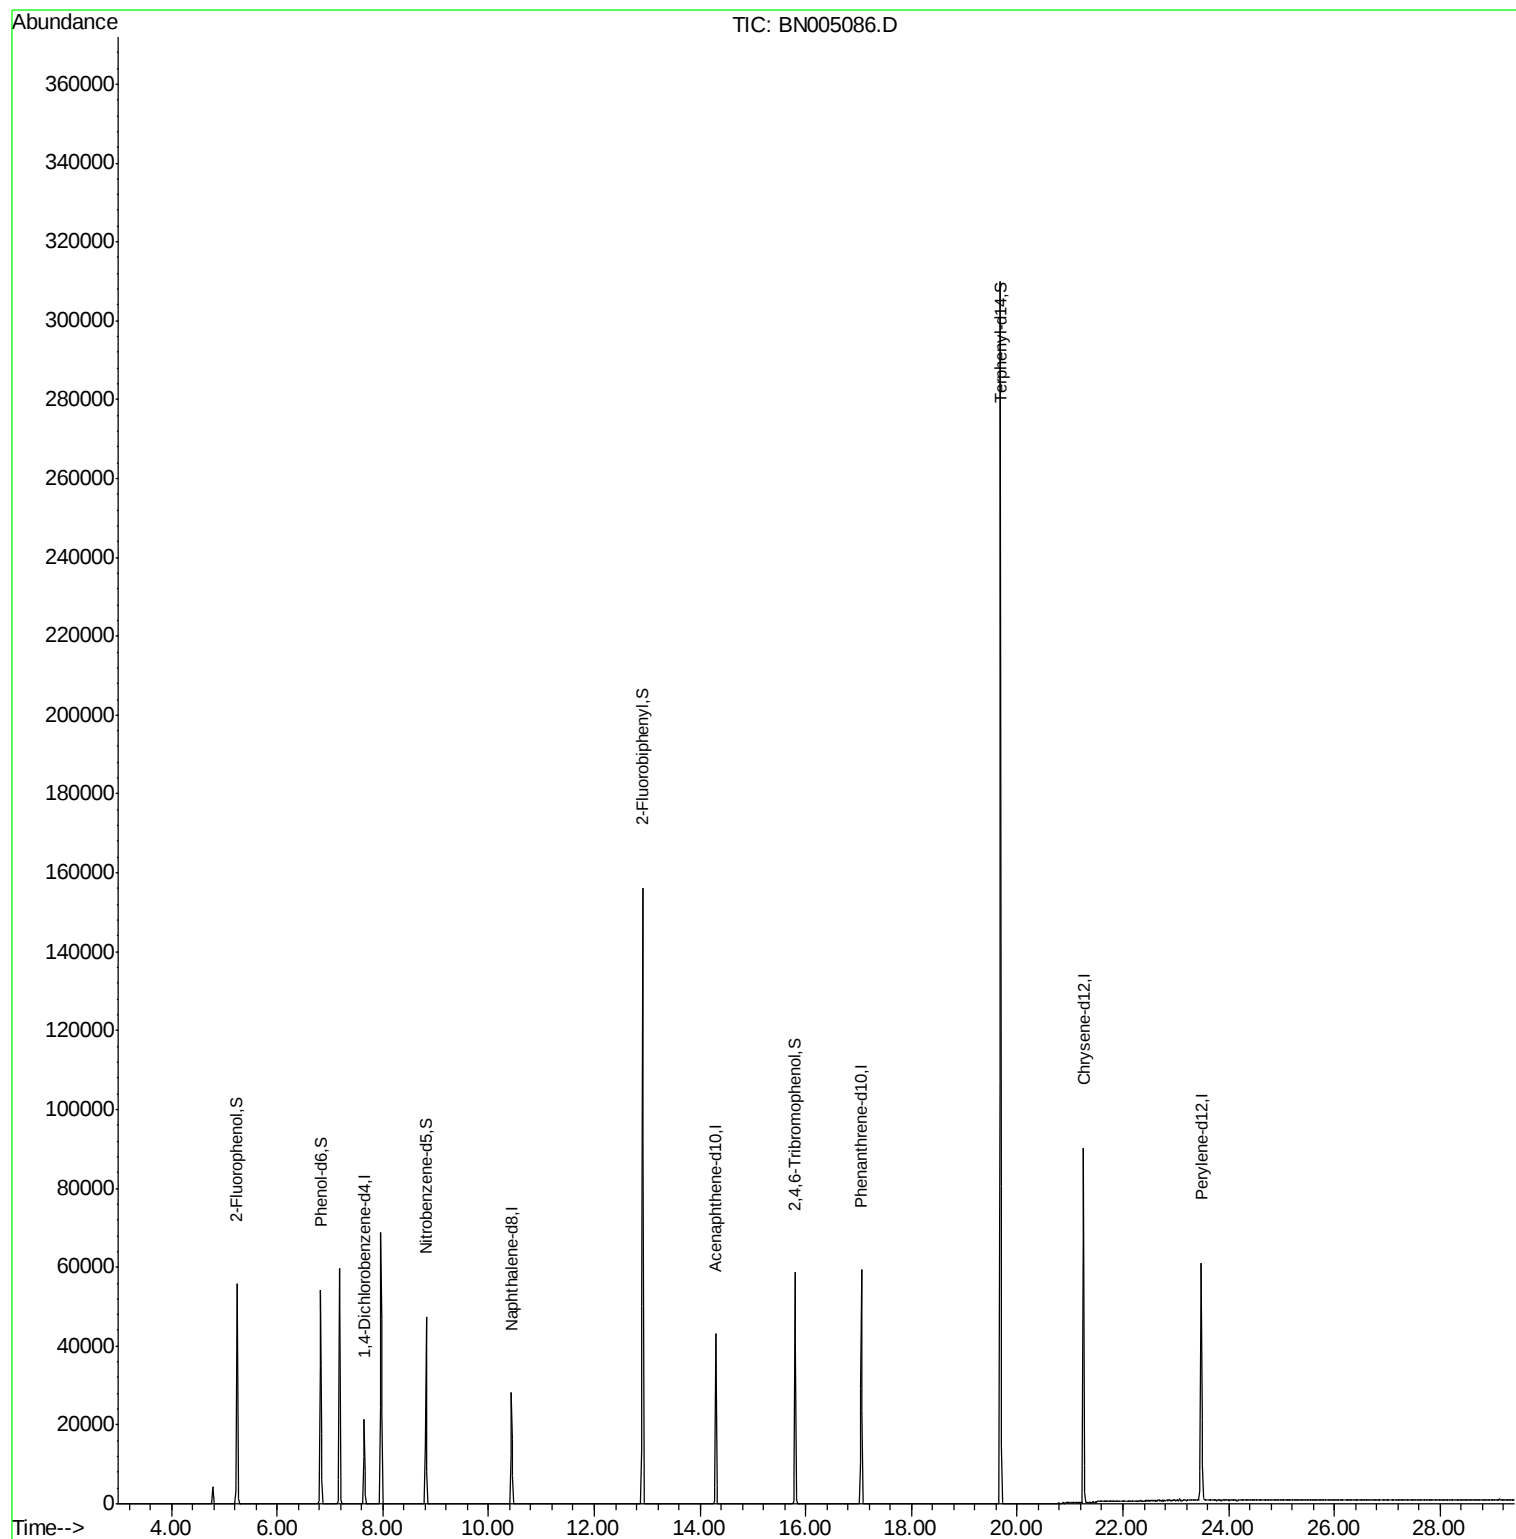

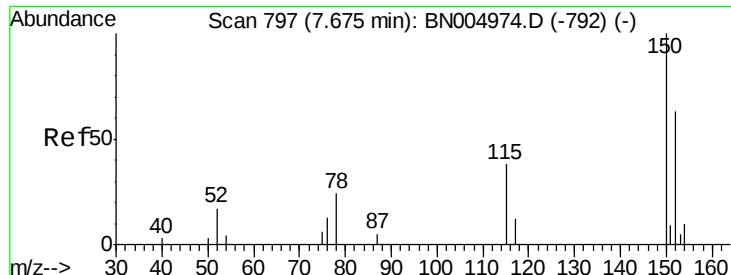


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.65 min Scan# 793
Delta R.T. 0.00 min
Lab File: BN005086.D
Acq: 04 Apr 2019 09:52

Instrument :
BNA_N
ClientSampleId :
PB118559BL

Tot Ion:152 Resp: 6762
Ion Ratio Lower Upper
152 100
150 154.2 125.8 188.6
115 58.0 47.9 71.9

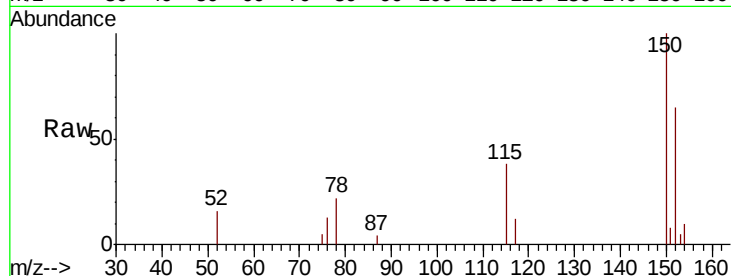


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

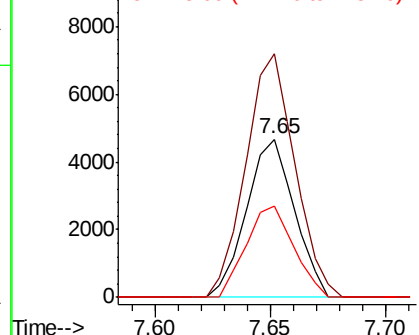



#5


2-Fluorophenol
Concen: 70.074 ng
RT: 5.25 min Scan# 384
Delta R.T. 0.01 min
Lab File: BN005086.D
Acq: 04 Apr 2019 09:52

Tgt Ion:112 Resp: 27407
Ion Ratio Lower Upper
112 100
64 50.6 41.2 61.8
63 25.5 20.7 31.1

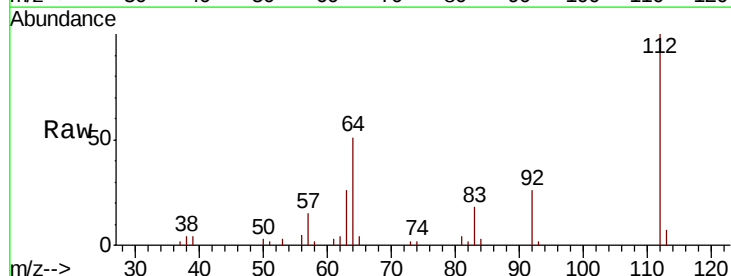

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

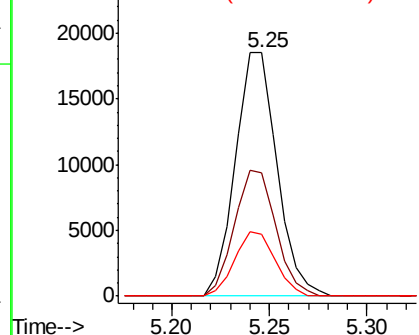

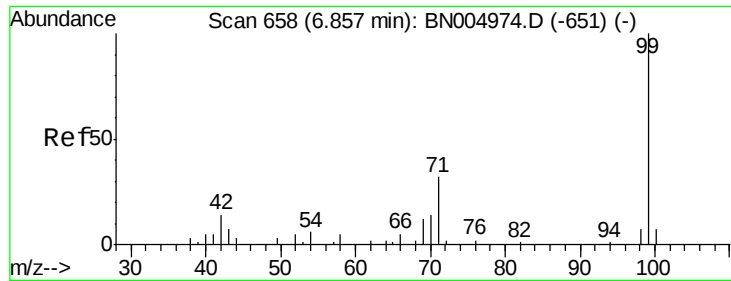

#7

Phenol-d6

Concen: 66.081 ng

RT: 6.83 min Scan# 653

Delta R.T. 0.00 min

Lab File: BN005086.D

Acq: 04 Apr 2019 09:52

Instrument :

BNA_N

ClientSampleId :

PB118559BL


Tot Ion: 99 Resp: 34280

Ion Ratio Lower Upper

99 100

42 14.0 11.0 16.4




71 32.6 25.8 38.8

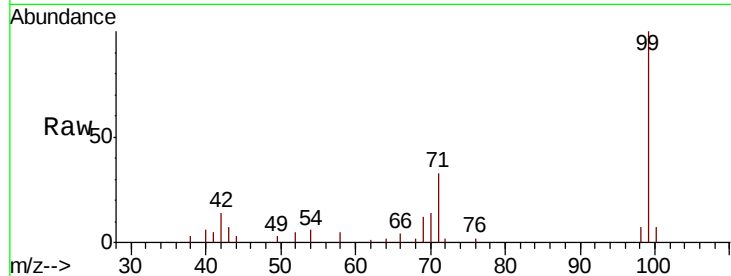

Abundance Ion 99.00 (98.70 to 99.70): BN004974.D (-651) (-)

Ion 42.00 (41.70 to 42.70): BN004974.D (-651) (-)

Ion 71.00 (70.70 to 71.70): BN004974.D (-651) (-)

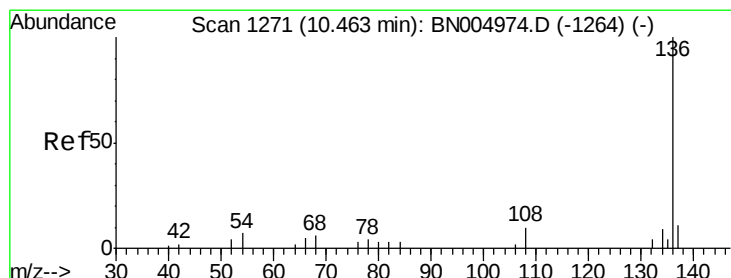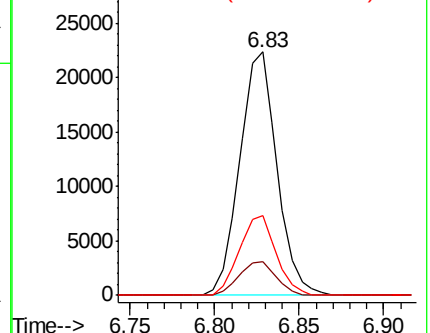

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1266

Delta R.T. -0.01 min

Lab File: BN005086.D

Acq: 04 Apr 2019 09:52

Tgt Ion: 136 Resp: 26738


Ion Ratio Lower Upper

136 100

137 11.4 8.6 12.8

54 6.5 5.0 7.4

68 5.6 4.2 6.4


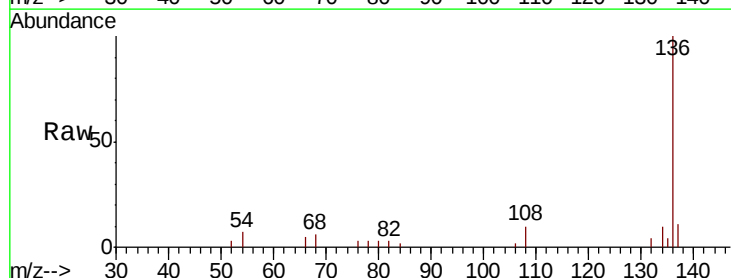


Abundance Ion 136.00 (135.70 to 136.70): BN004974.D (-1264) (-)

Ion 137.00 (136.70 to 137.70): BN004974.D (-1264) (-)

Ion 54.00 (53.70 to 54.70): BN004974.D (-1264) (-)

Ion 68.00 (67.70 to 68.70): BN004974.D (-1264) (-)

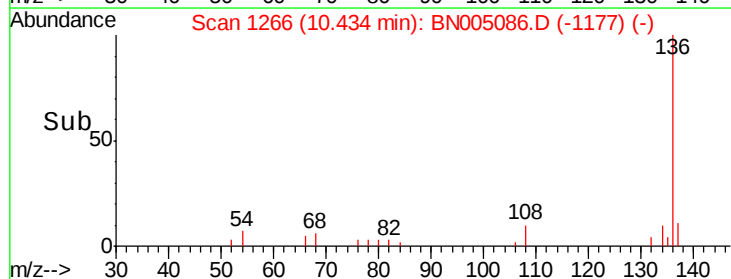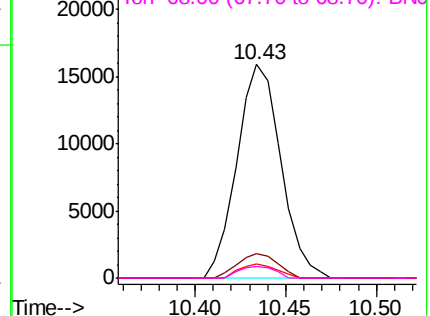







#23
Nitrobenzene-d5
Concen: 65.224 ng
RT: 8.82 min Scan# 991
Delta R.T. -0.01 min
Lab File: BN005086.D
Acq: 04 Apr 2019 09:52

Instrument :
BNA_N
ClientSampleId :
PB118559BL

Tot Ion: 82 Resp: 28830
Ion Ratio Lower Upper
82 100
128 51.1 40.6 60.8
54 43.4 34.4 51.6

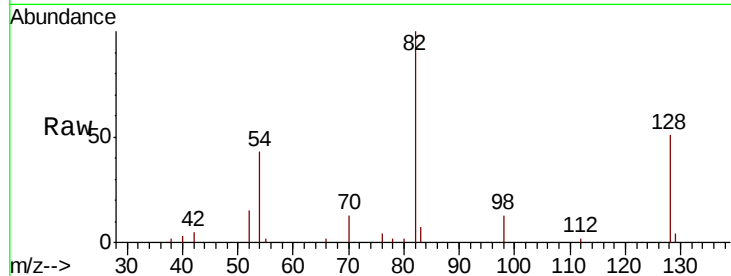


Abundance Ion 82.00 (81.70 to 82.70): BNC
Ion 128.00 (127.70 to 128.70): BNC
Ion 54.00 (53.70 to 54.70): BNC

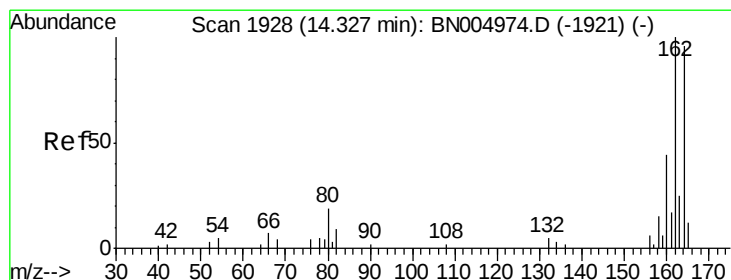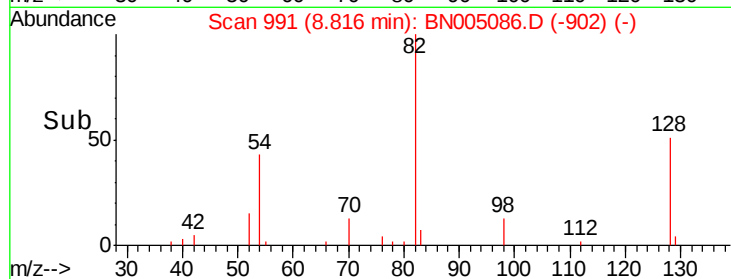
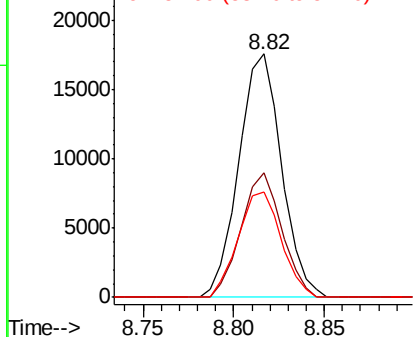



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.30 min Scan# 1923
Delta R.T. -0.01 min
Lab File: BN005086.D
Acq: 04 Apr 2019 09:52

Tgt Ion: 164 Resp: 16432
Ion Ratio Lower Upper
164 100
162 103.0 83.8 125.6
160 45.4 36.0 54.0

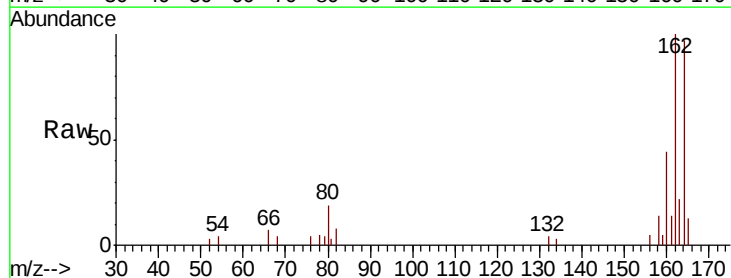

Abundance Ion 164.00 (163.70 to 164.70): BNC
Ion 162.00 (161.70 to 162.70): BNC
Ion 160.00 (159.70 to 160.70): BNC

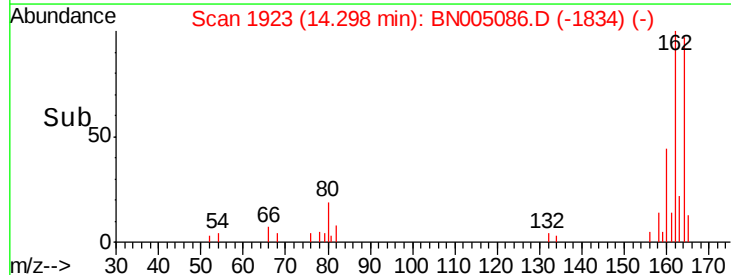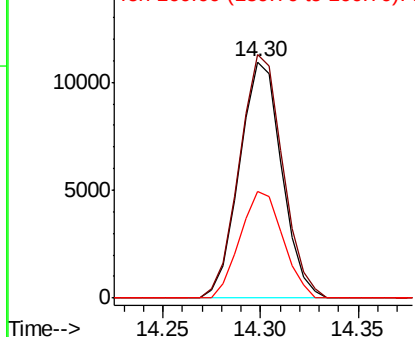

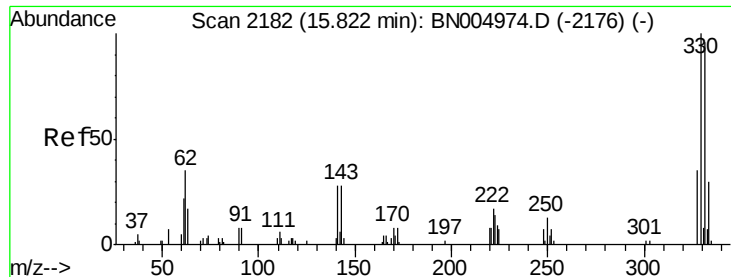

#42

2,4,6-Tribromophenol

Concen: 57.128 ng

RT: 15.80 min Scan# 2178

Delta R.T. -0.01 min

Lab File: BN005086.D

Acq: 04 Apr 2019 09:52

Instrument :

BNA_N

ClientSampleId :

PB118559BL


Tot Ion:330 Resp: 15140

Ion Ratio Lower Upper




330 100

332 96.8 77.4 116.2

141 24.7 20.3 30.5

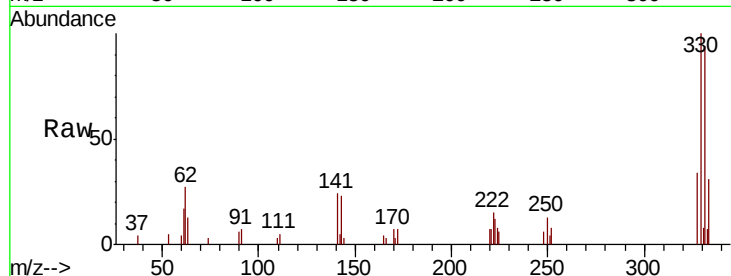

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

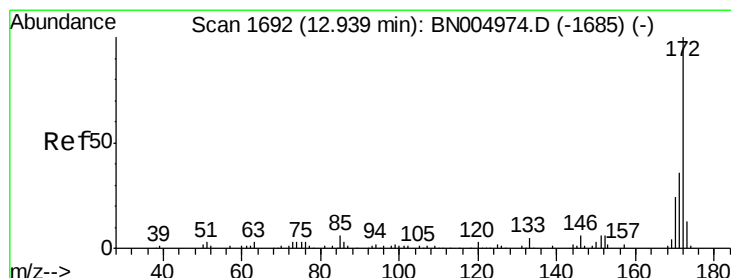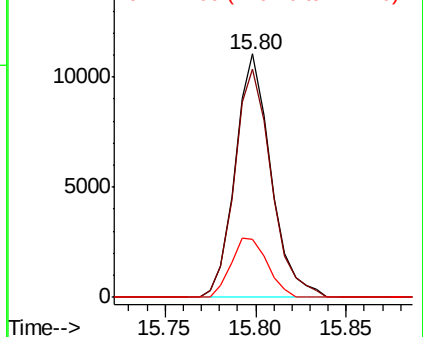

#45

2-Fluorobiphenyl

Concen: 68.822 ng

RT: 12.91 min Scan# 1687

Delta R.T. -0.01 min

Lab File: BN005086.D

Acq: 04 Apr 2019 09:52


Tgt Ion:172 Resp: 85342

Ion Ratio Lower Upper



172 100


171 35.7 28.7 43.1

170 23.4 18.8 28.2

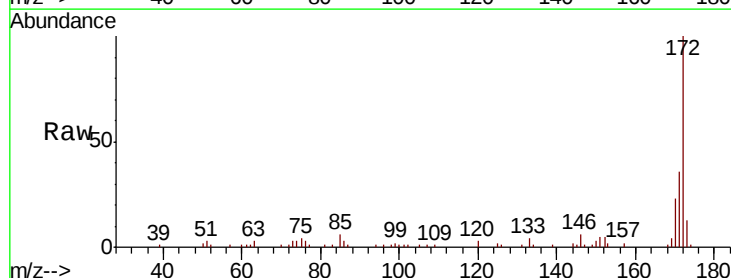

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

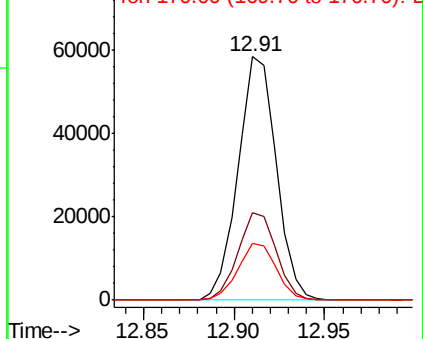


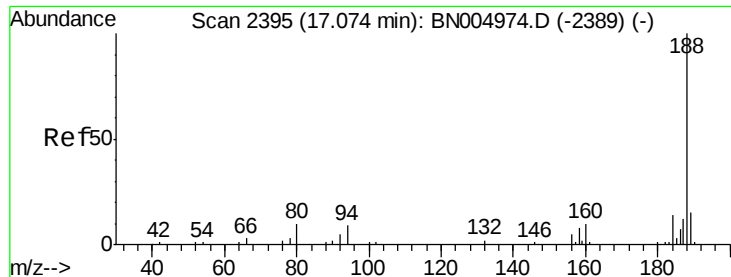




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.05 min Scan# 2391
Delta R.T. -0.01 min
Lab File: BN005086.D
Acq: 04 Apr 2019 09:52

Instrument :
BNA_N
ClientSampleId :
PB118559BL

Tot Ion:188 Resp: 39655
Ion Ratio Lower Upper
188 100
94 8.5 6.6 10.0
80 9.4 7.1 10.7

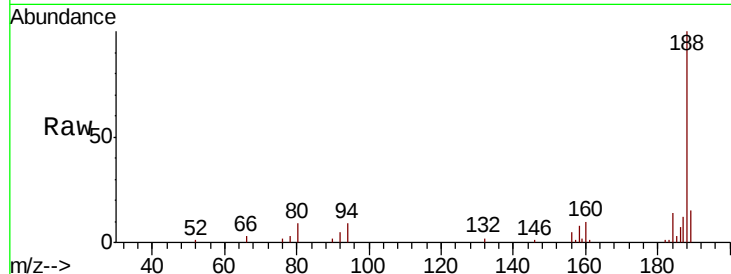


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BNC
Ion 80.00 (79.70 to 80.70): BNC

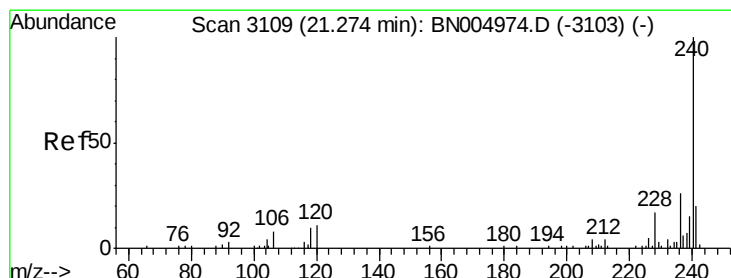
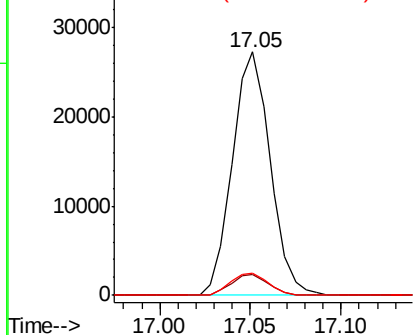



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.25 min Scan# 3105
Delta R.T. -0.01 min
Lab File: BN005086.D
Acq: 04 Apr 2019 09:52

Tgt Ion:240 Resp: 47327
Ion Ratio Lower Upper
240 100
120 10.1 8.1 12.1
236 25.5 20.4 30.6

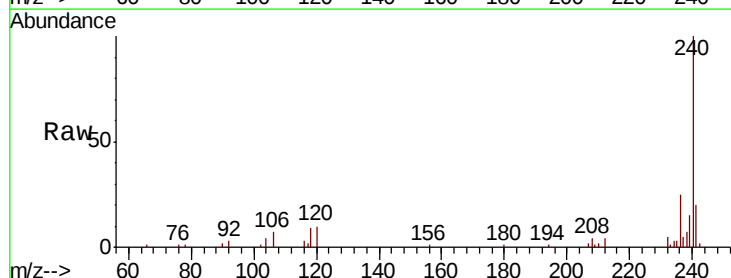

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

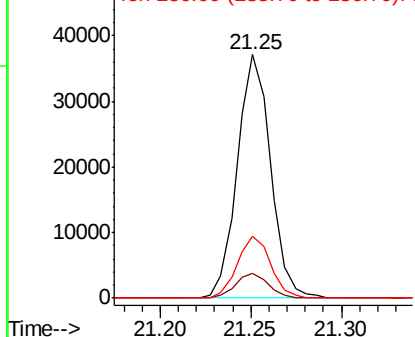

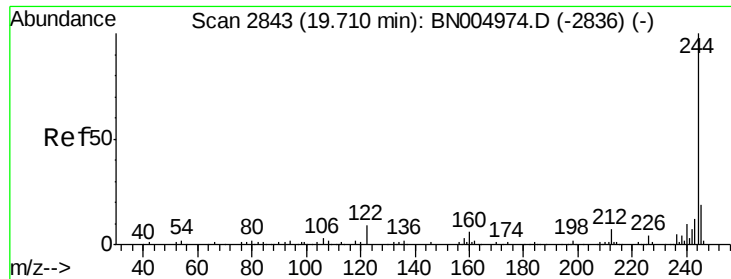

#79

Terphenyl-d14

Concen: 60.299 ng

RT: 19.69 min Scan# 2839

Delta R.T. -0.01 min

Lab File: BN005086.D

Acq: 04 Apr 2019 09:52

Instrument :

BNA_N

ClientSampleId :

PB118559BL


Tot Ion:244 Resp: 148229

Ion Ratio Lower Upper




244 100

212 6.5 5.3 7.9

122 9.6 7.8 11.6

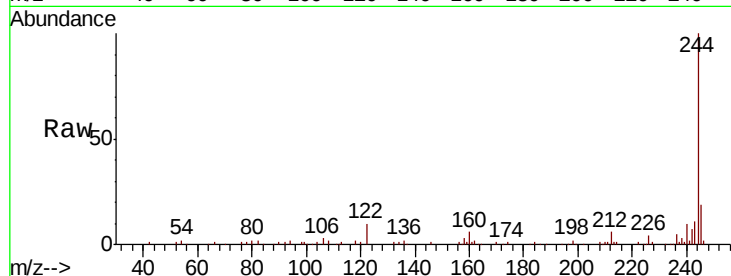

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

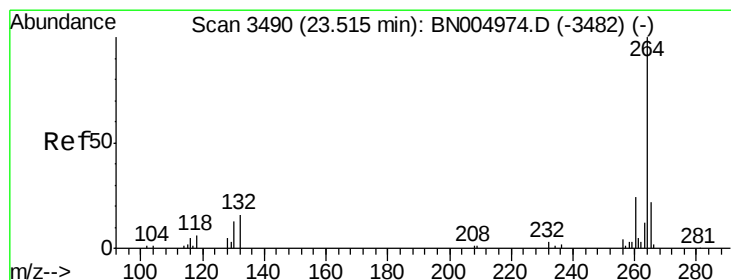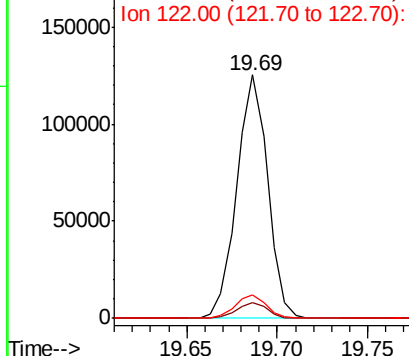

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.48 min Scan# 3484

Delta R.T. -0.01 min

Lab File: BN005086.D

Acq: 04 Apr 2019 09:52


Tgt Ion:264 Resp: 49021

Ion Ratio Lower Upper

264 100

260 24.0 18.9 28.3

265 21.6 17.4 26.2

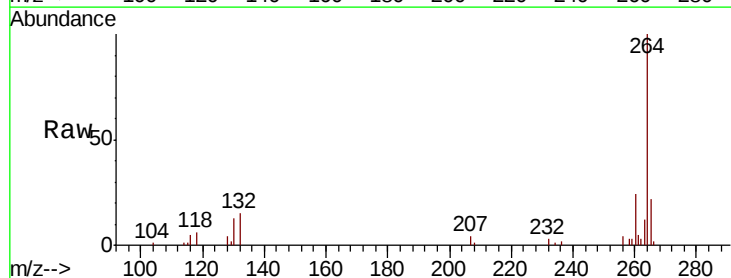

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

