

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040319\
 Data File : BN005067.D
 Acq On : 03 Apr 2019 18:53
 Operator : JU/SJ
 Sample : PB118575BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118575BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	379	384	391	rBB	121343	163180	42.42%	7.575%
2	6.834	647	654	661	rBB	113719	171555	44.60%	7.964%
3	7.187	708	714	720	rBV	127838	189335	49.22%	8.789%
4	7.652	788	793	798	rBB	30564	43711	11.36%	2.029%
5	7.969	841	847	853	rBB	96752	144071	37.45%	6.688%
6	8.816	985	991	998	rBB	65237	102229	26.58%	4.746%
7	10.434	1261	1266	1274	rBB	40570	65351	16.99%	3.034%
8	12.916	1682	1688	1695	rBB	205749	285768	74.29%	13.266%
9	14.304	1919	1924	1929	rBB2	63277	90822	23.61%	4.216%
10	15.798	2173	2178	2185	rBB	152964	205170	53.34%	9.525%
11	17.051	2386	2391	2398	rBB2	79399	105475	27.42%	4.896%
12	19.686	2834	2839	2844	rBV	318357	384672	100.00%	17.857%
13	21.251	3101	3105	3113	rBV	87558	107969	28.07%	5.012%
14	23.480	3477	3484	3493	rBV2	50281	94816	24.65%	4.402%




Sum of corrected areas: 2154124

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040319\
Data File : BN005067.D
Acq On : 03 Apr 2019 18:53
Operator : JU/SJ
Sample : PB118575BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118575BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

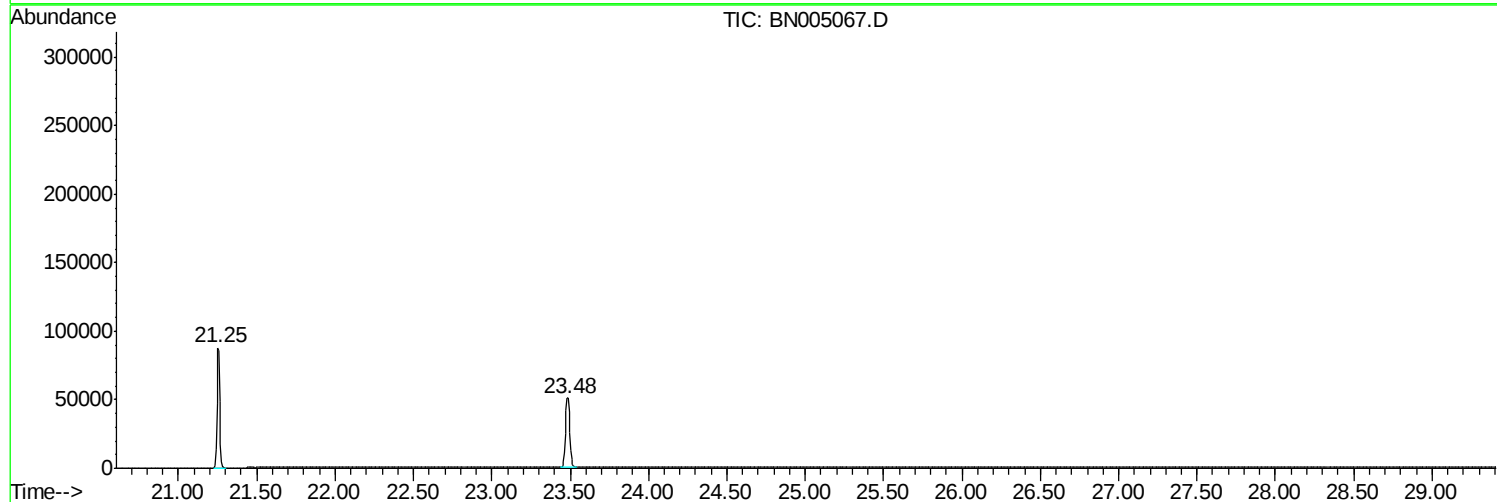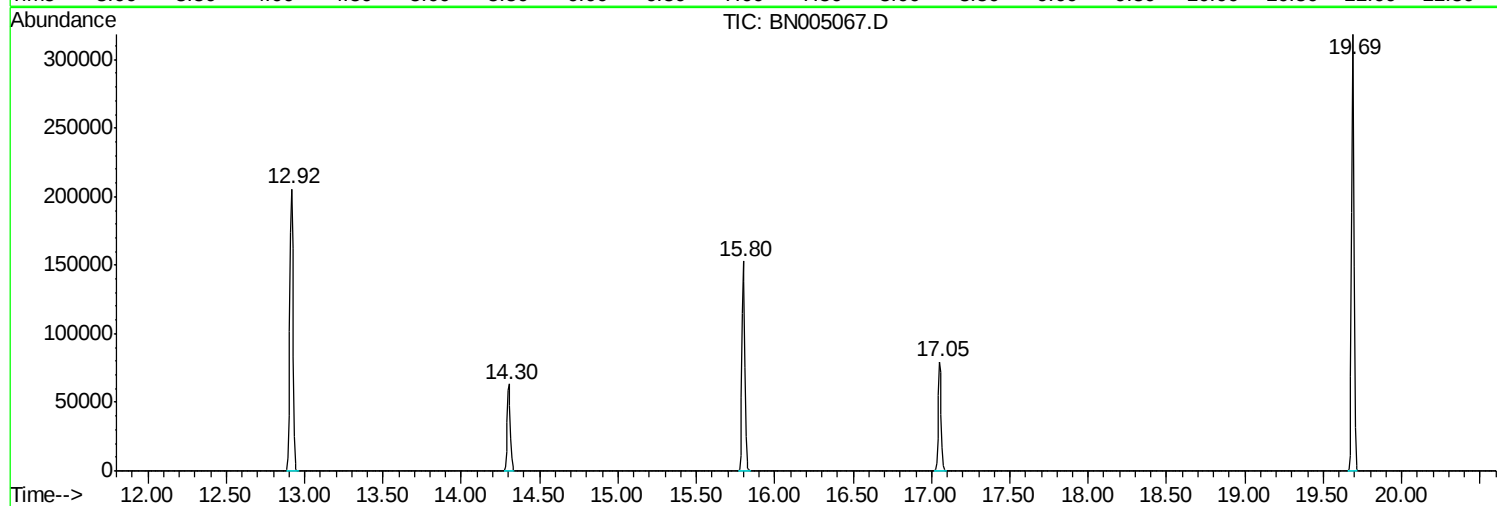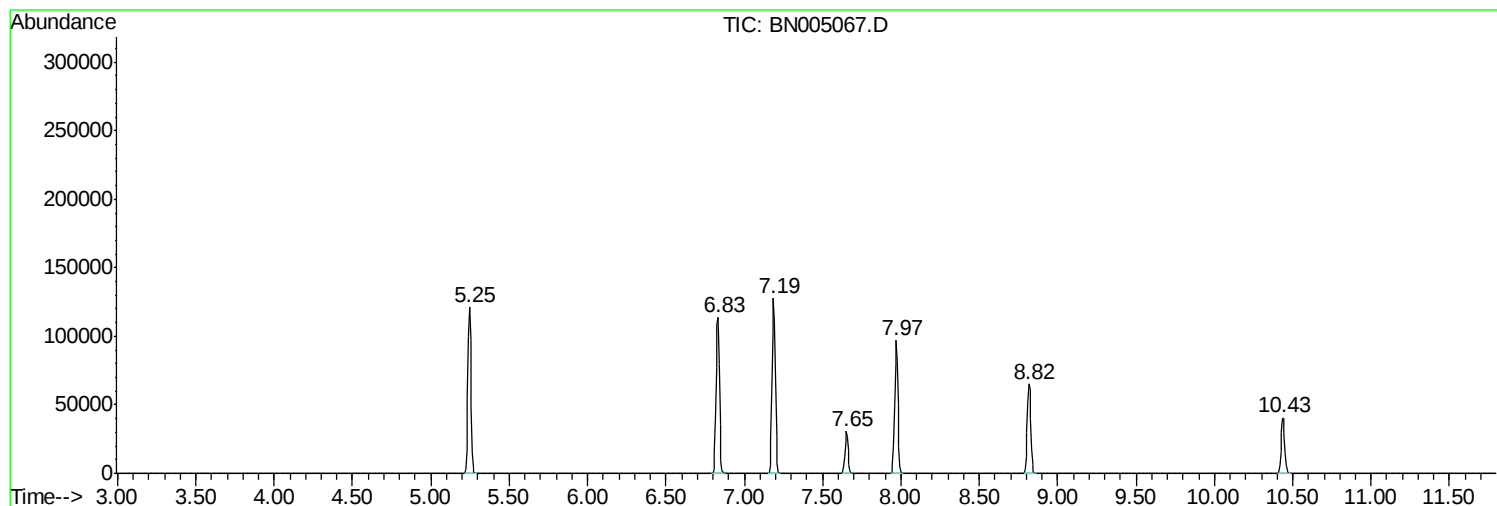

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040319\
Data File : BN005067.D
Acq On : 03 Apr 2019 18:53
Operator : JU/SJ
Sample : PB118575BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118575BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	86.63 ng	189335	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Amphetaminil	250	C17H18N2	017590-01-1	12
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

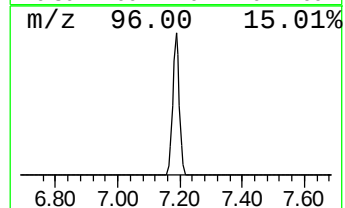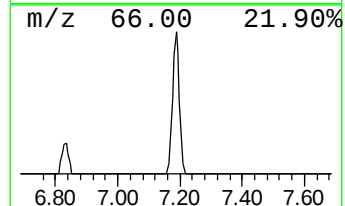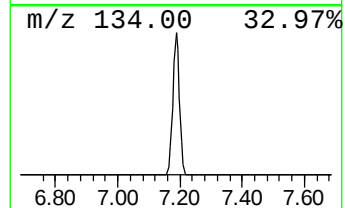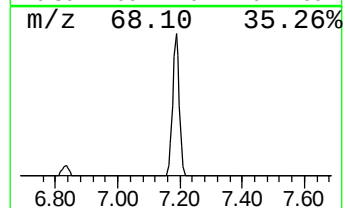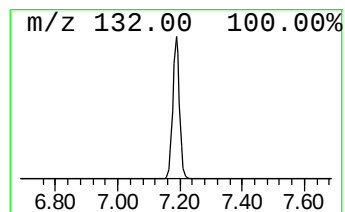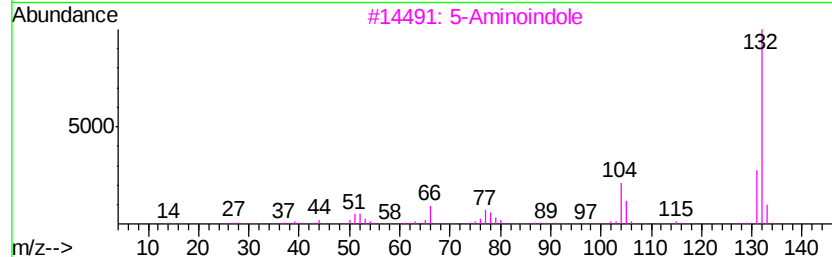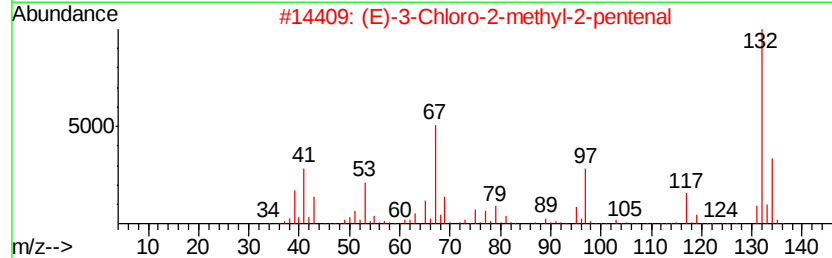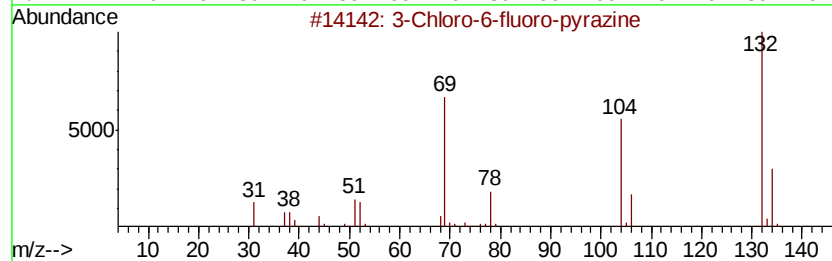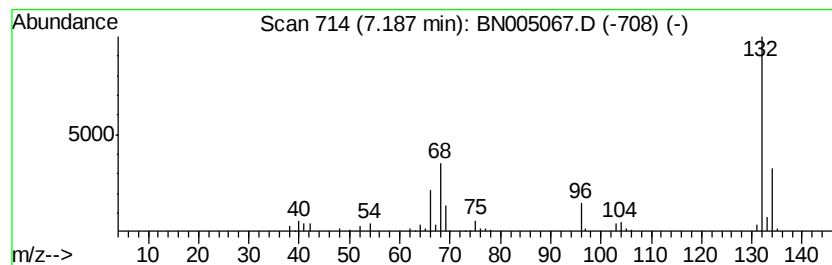

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040319\
Data File : BN005067.D
Acq On : 03 Apr 2019 18:53
Operator : JU/SJ
Sample : PB118575BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118575BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.19	7.19	86.6	ng	189335	1	7.65	43711	20.0