

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040319\
 Data File : BN005086.D
 Acq On : 04 Apr 2019 09:52
 Operator : JU/SJ
 Sample : PB118559BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118559BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.787	302	306	310	rBB	4349	5363	1.51%	0.354%
2	5.240	379	383	390	rBB	55808	77065	21.75%	5.084%
3	6.828	647	653	660	rBB	54338	80038	22.59%	5.281%
4	7.181	708	713	720	rBB	59868	88123	24.87%	5.814%
5	7.652	788	793	798	rBB	21394	29730	8.39%	1.961%
6	7.963	841	846	852	rBB	68790	105868	29.87%	6.985%
7	8.816	985	991	997	rBB	47539	73715	20.80%	4.863%
8	10.434	1261	1266	1273	rBB	28173	43217	12.20%	2.851%
9	12.910	1682	1687	1694	rBB	156256	216539	61.11%	14.286%
10	14.298	1918	1923	1929	rBB2	43027	63989	18.06%	4.222%
11	15.798	2173	2178	2185	rBB	58801	77558	21.89%	5.117%
12	17.051	2386	2391	2398	rBB	59478	81825	23.09%	5.398%
13	19.686	2834	2839	2844	rBV	309974	354370	100.00%	23.380%
14	21.251	3100	3105	3112	rBV	89986	109636	30.94%	7.233%
15	23.480	3477	3484	3495	rVB2	60312	108675	30.67%	7.170%


Sum of corrected areas: 1515711

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040319\
Data File : BN005086.D
Acq On : 04 Apr 2019 09:52
Operator : JU/SJ
Sample : PB118559BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118559BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

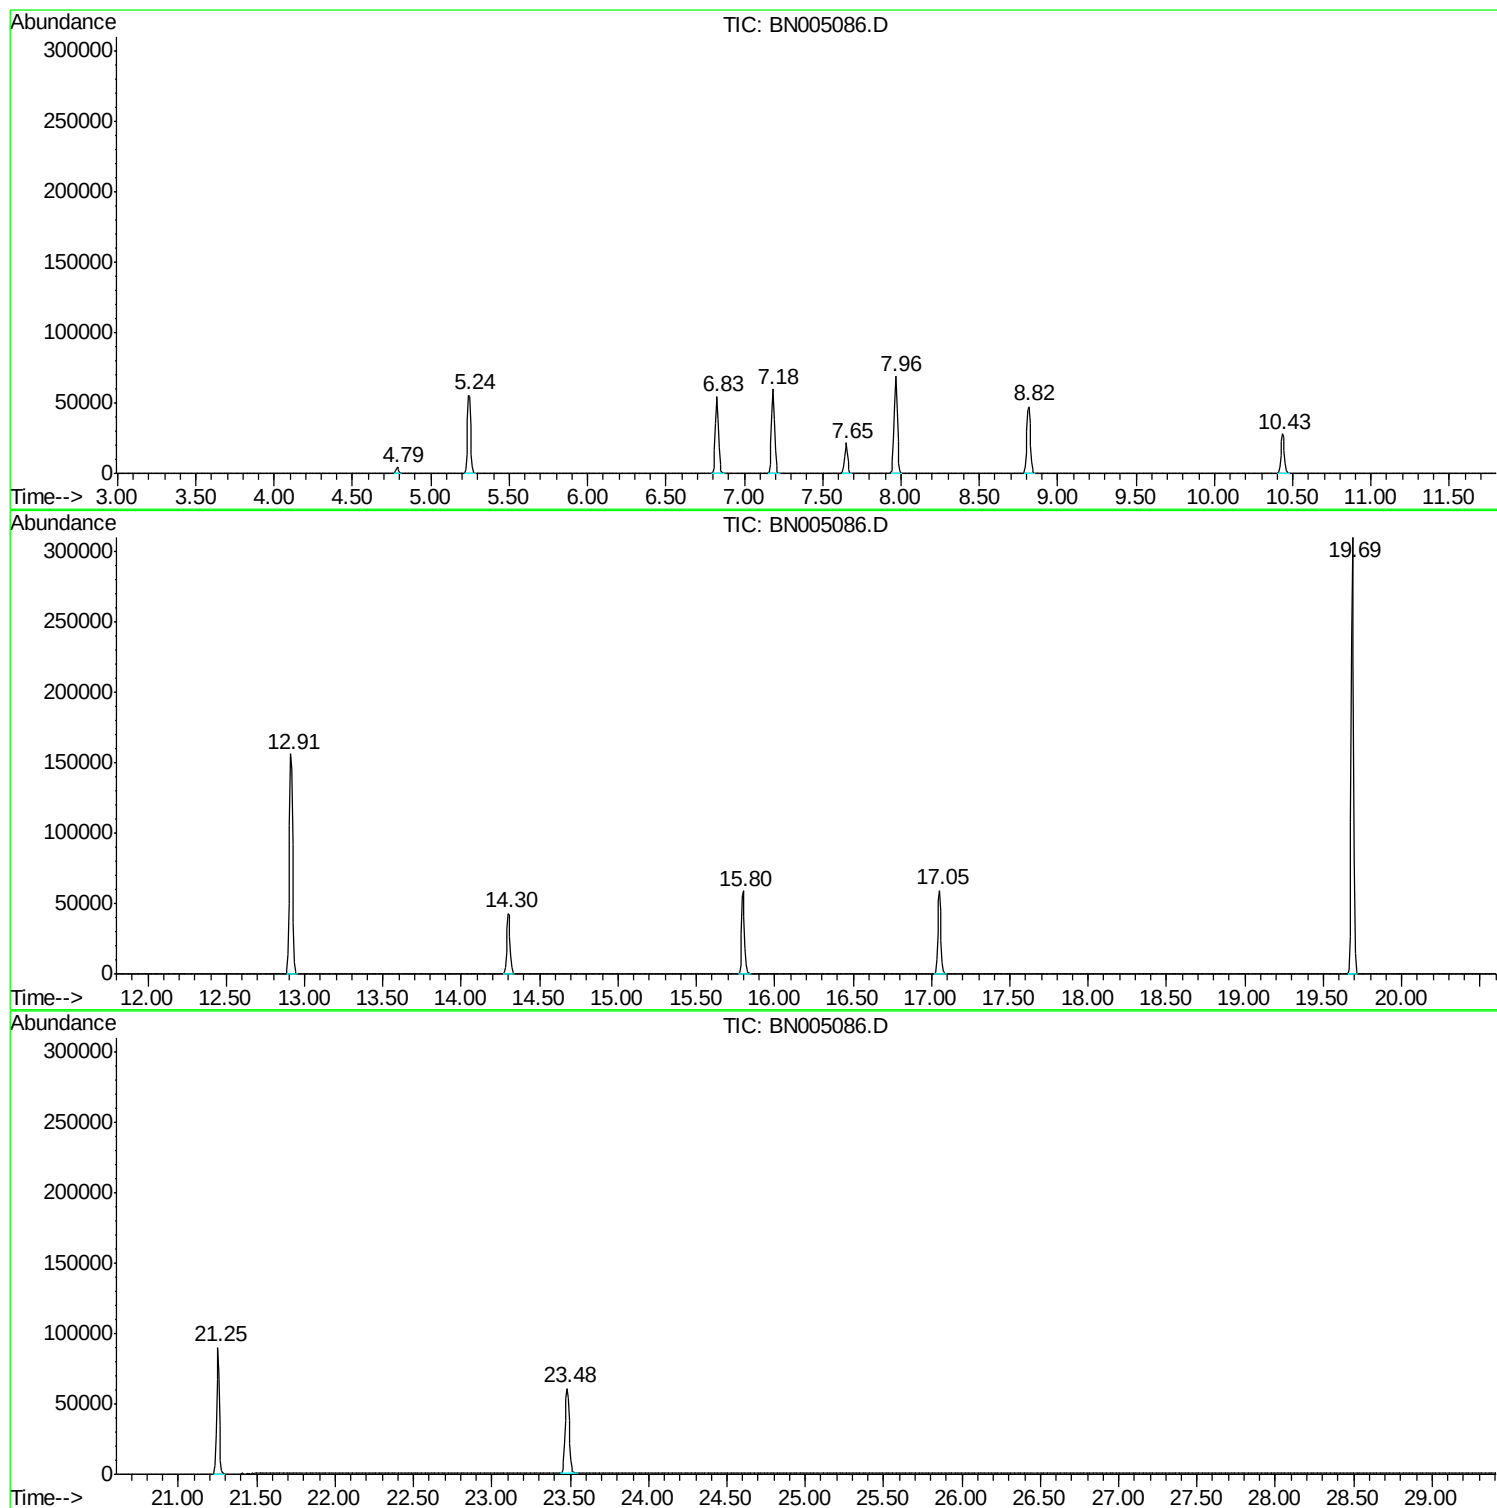

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040319\
Data File : BN005086.D
Acq On : 04 Apr 2019 09:52
Operator : JU/SJ
Sample : PB118559BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118559BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown4.79 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.79	3.61 ng	5363	1,4-Dichlorobenzene-d4	7.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Oxirane, [(1-methylethoxy)methyl]-	116	C6H12O2	004016-14-2	9
2			Guanidine	59	CH5N3	000113-00-8	4
3			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	4
4			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	4
5			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	4

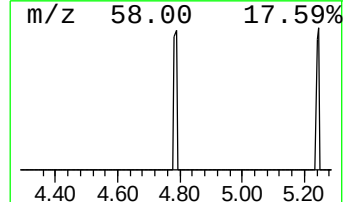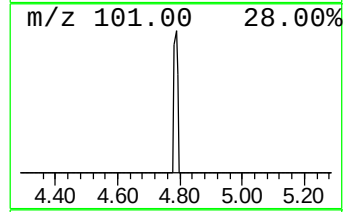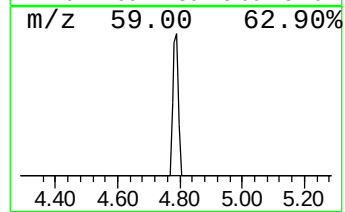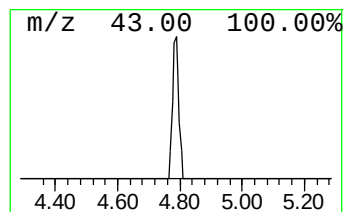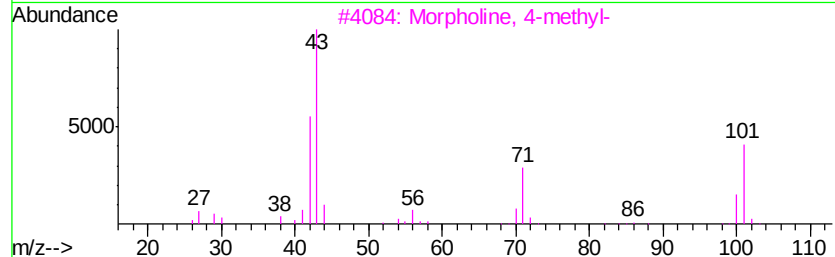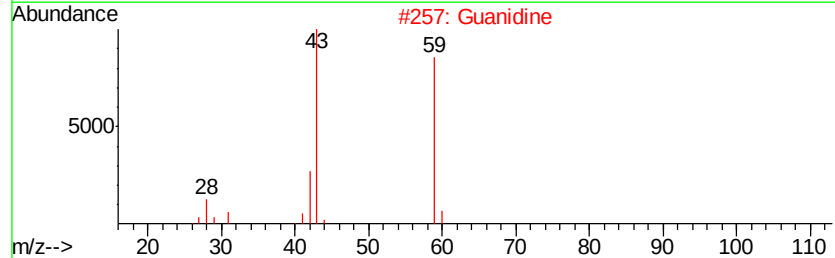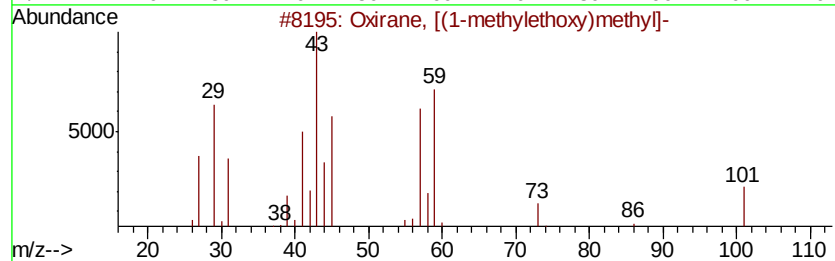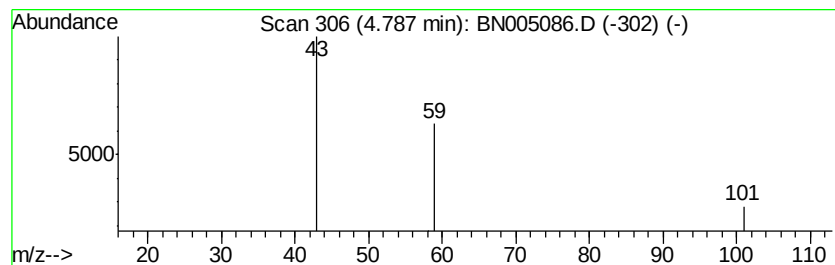

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040319\
Data File : BN005086.D
Acq On : 04 Apr 2019 09:52
Operator : JU/SJ
Sample : PB118559BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118559BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.18 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.18	59.28 ng	88123	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

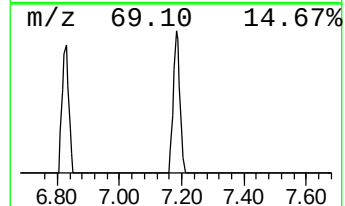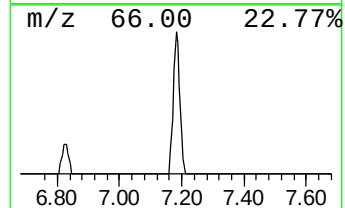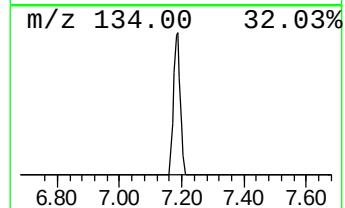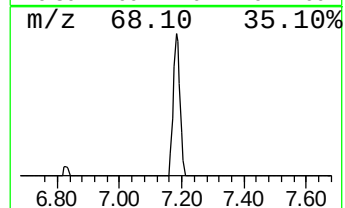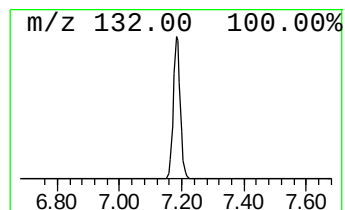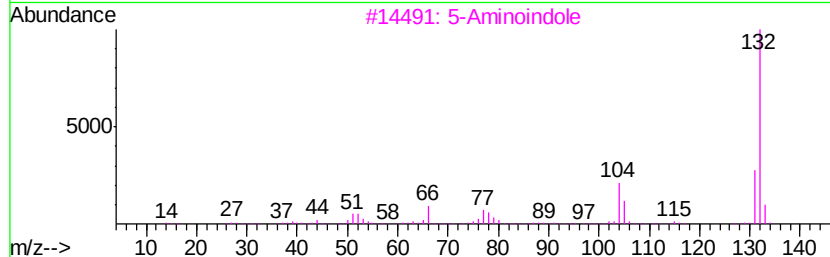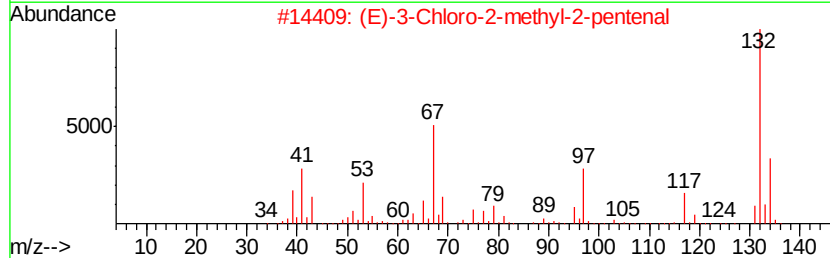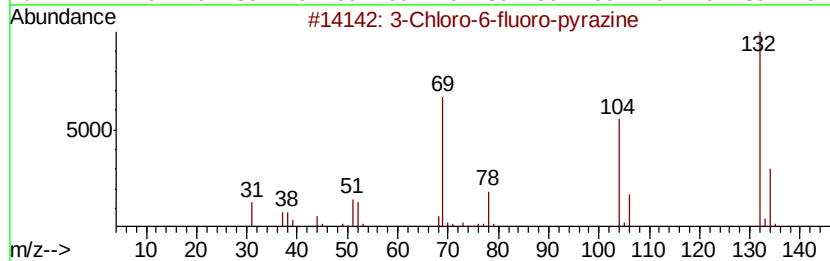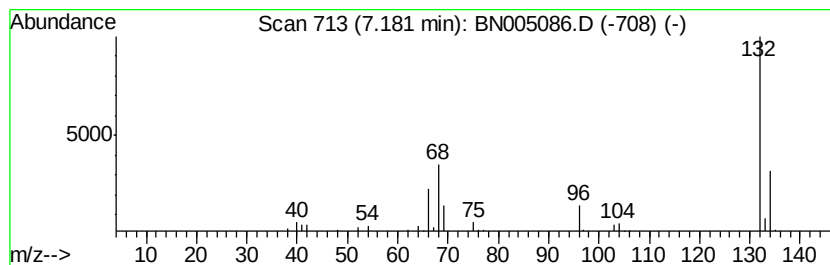

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040319\
Data File : BN005086.D
Acq On : 04 Apr 2019 09:52
Operator : JU/SJ
Sample : PB118559BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118559BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown4.79	4.79	3.6	ng	5363	1	7.65	29730	20.0
unknown7.18	7.18	59.3	ng	88123	1	7.65	29730	20.0