

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030645.D
 Acq On : 04 Apr 2024 02:39
 Operator : MA/JU
 Sample : P1948-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH4

Quant Time: Apr 04 03:08:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	308428	20.000	ng/u1	0.00
20) Naphthalene-d8	10.475	136	1370837	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.340	164	875269	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.086	188	1699103	20.000	ng/u1	0.00
79) Chrysene-d12	21.322	240	1100444	20.000	ng/u1	0.00
88) Perylene-d12	24.274	264	1207969	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	34587	5.258	ng/uL	0.00
4) Pyridine-d5	3.605	84	109090	5.531	ng/u1	0.00
7) Phenol-d5	6.863	99	169700	6.802	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.034	67	556754	36.128	ng/u1	0.00
11) 2-Chlorophenol-d4	7.228	132	580462	30.668	ng/u1	0.00
15) 4-Methylphenol-d8	8.399	113	353623	16.911	ng/u1	0.00
21) Nitrobenzene-d5	8.852	128	405651	42.658	ng/u1	0.00
24) 2-Nitrophenol-d4	9.569	143	415789	47.796	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	682631	35.843	ng/u1	0.00
31) 4-Chloroaniline-d4	10.616	131	643378	20.520	ng/u1	0.00
46) Dimethylphthalate-d6	13.757	166	2363255	40.440	ng/u1	0.00
49) Acenaphthylene-d8	14.028	160	2702995	40.229	ng/u1	0.00
54) 4-Nitrophenol-d4	14.540	143	76753	6.866	ng/u1	0.00
60) Fluorene-d10	15.334	176	1986569	38.847	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	272495	36.334	ng/u1	0.00
73) Anthracene-d10	17.186	188	3305491	45.152	ng/u1	0.00
81) Pyrene-d10	19.486	212	3228336	54.566	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.074	264	2725251	48.962	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.234	88	8761	1.243	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030645.D
Acq On : 04 Apr 2024 02:39
Operator : MA/JU
Sample : P1948-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH4


Quant Time: Apr 04 03:08:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

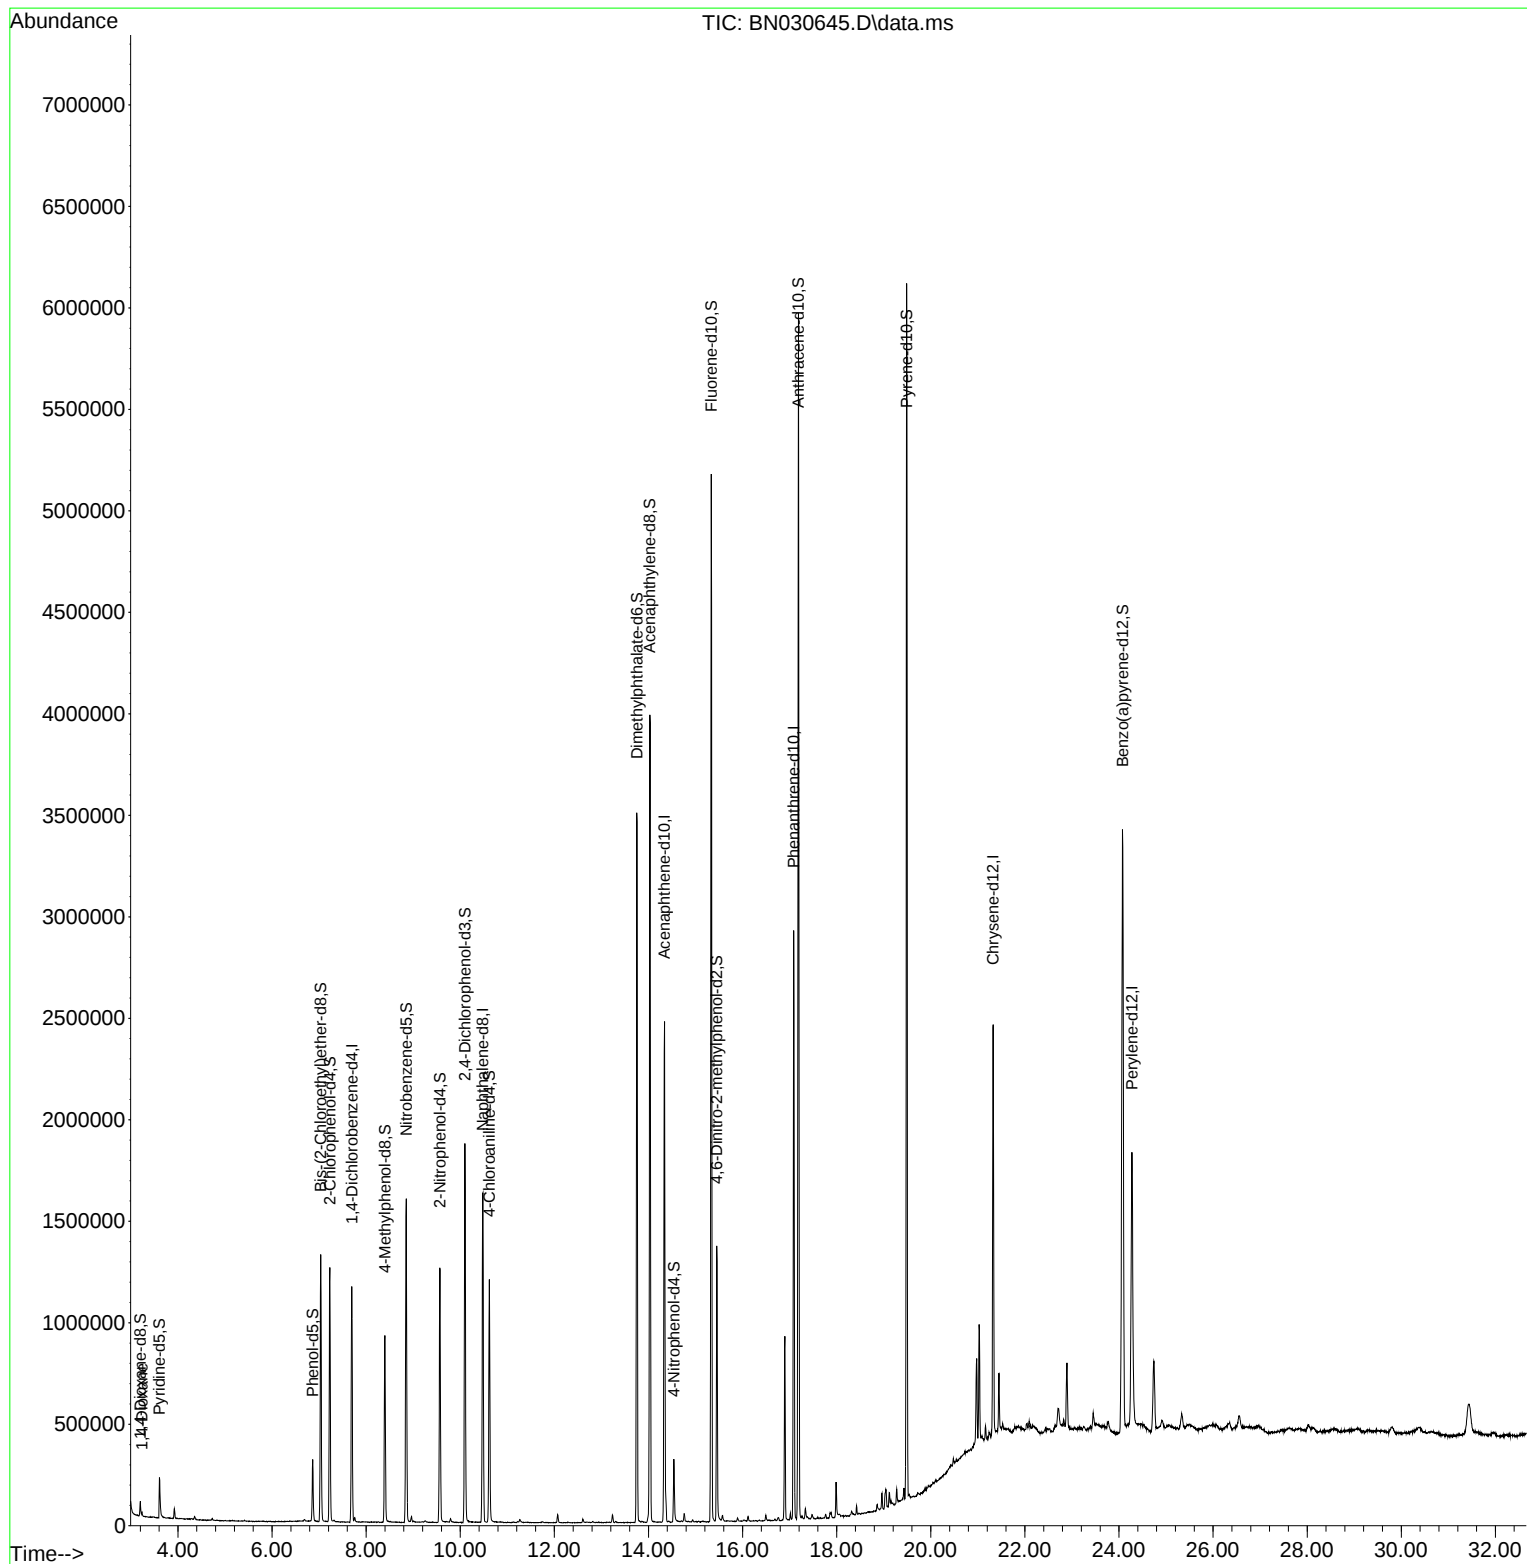

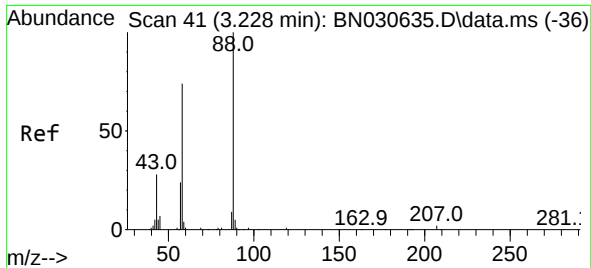

#2
 1,4-Dioxane
 Concen: 1.243 ng/uL
 RT: 3.234 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BN030645.D
 Acq: 04 Apr 2024 02:39

Instrument :
 BNA_N
 ClientSampleId :
 C0AH4

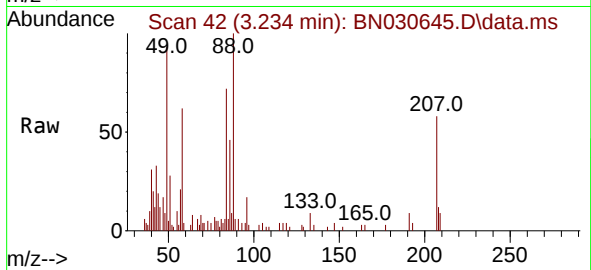

Tgt Ion:	88	Resp:	8761
Ion	Ratio	Lower	Upper
88	100		
43	32.8	23.8	35.8
58	61.5	56.6	84.8

