

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030647.D
 Acq On : 04 Apr 2024 03:58
 Operator : MA/JU
 Sample : P1948-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH6

Quant Time: Apr 04 04:28:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	91244	20.000	ng/u1	0.00
20) Naphthalene-d8	10.475	136	414599	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.334	164	268459	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.086	188	514664	20.000	ng/u1	0.00
79) Chrysene-d12	21.327	240	330782	20.000	ng/u1	0.00
88) Perylene-d12	24.274	264	360819	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	31444	16.157	ng/uL	0.00
4) Pyridine-d5	3.605	84	120079	20.579	ng/u1	0.00
7) Phenol-d5	6.863	99	169547	22.970	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.034	67	547302	120.049	ng/u1	0.00
11) 2-Chlorophenol-d4	7.228	132	560366	100.076	ng/u1	0.00
15) 4-Methylphenol-d8	8.399	113	341167	55.150	ng/u1	0.00
21) Nitrobenzene-d5	8.852	128	393275	136.742	ng/u1	0.00
24) 2-Nitrophenol-d4	9.563	143	403816	153.481	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	661231	114.797	ng/u1	0.00
31) 4-Chloroaniline-d4	10.616	131	891203	93.982	ng/u1	0.00
46) Dimethylphthalate-d6	13.751	166	2287444	127.620	ng/u1	0.00
49) Acenaphthylene-d8	14.028	160	2632239	127.728	ng/u1	0.00
54) 4-Nitrophenol-d4	14.539	143	64077	18.690	ng/u1	0.00
60) Fluorene-d10	15.334	176	1895566	120.854	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	247362	108.889	ng/u1	0.00
73) Anthracene-d10	17.186	188	2946813	132.889	ng/u1	0.00
81) Pyrene-d10	19.486	212	2870224	161.392	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.074	264	2343925	140.982	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.234	88	8686	4.167	ng/uL	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030647.D
Acq On : 04 Apr 2024 03:58
Operator : MA/JU
Sample : P1948-04
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH6


Quant Time: Apr 04 04:28:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

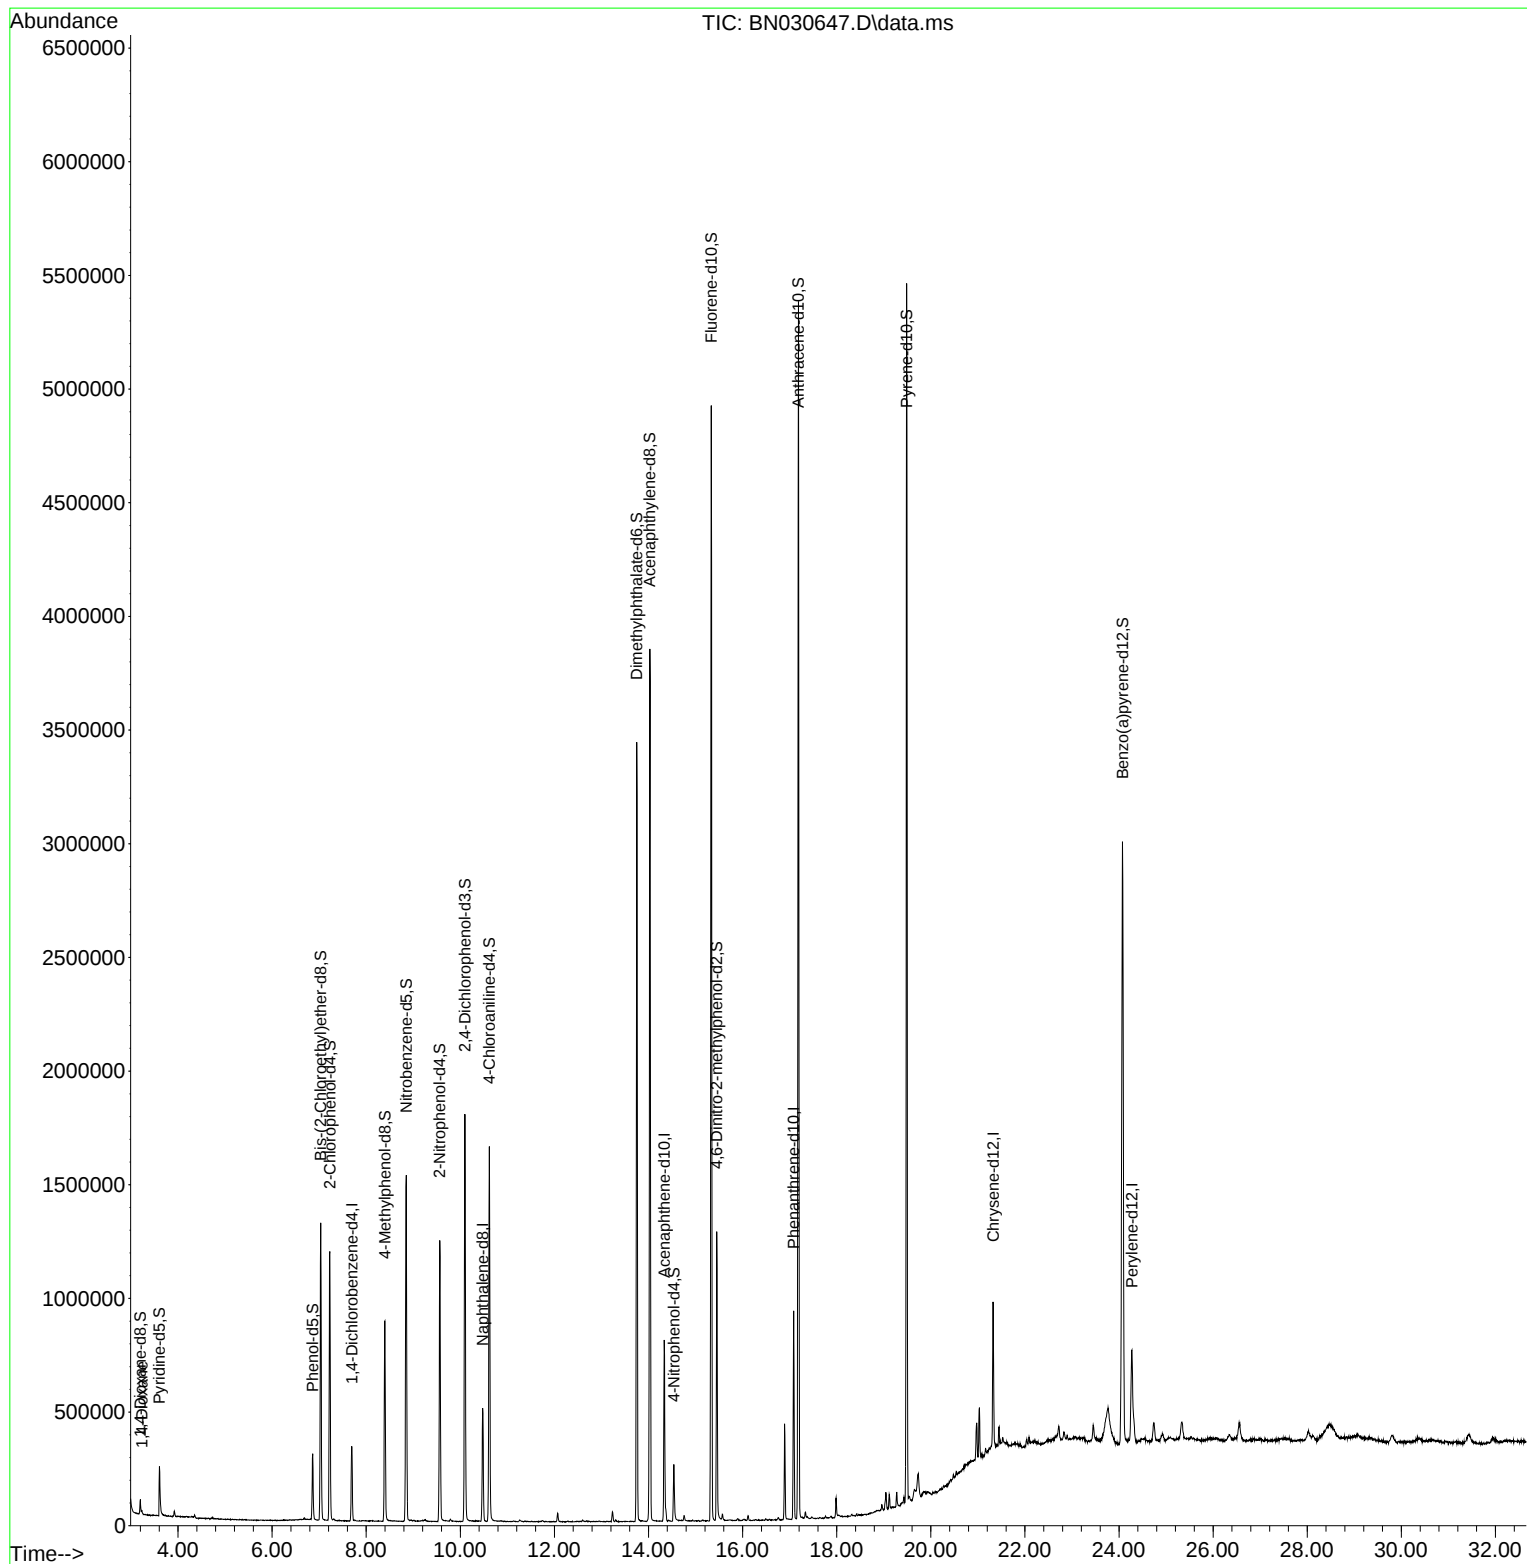

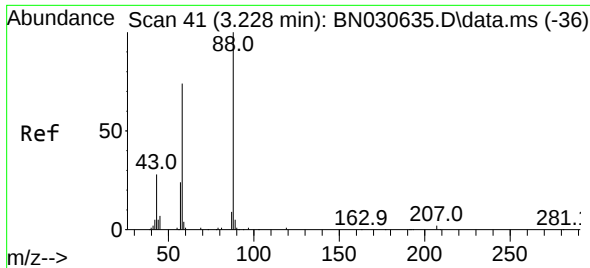

#2
 1,4-Dioxane
 Concen: 4.167 ng/uL
 RT: 3.234 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BN030647.D
 Acq: 04 Apr 2024 03:58

Instrument :
 BNA_N
 ClientSampleId :
 C0AH6

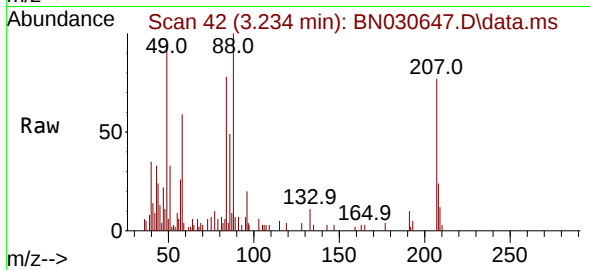

Tgt Ion:	88	Resp:	8686
Ion	Ratio	Lower	Upper
88	100		
43	33.4	23.8	35.8
58	59.4	56.6	84.8

