

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030609.D
 Acq On : 02 Apr 2024 10:23
 Operator : MA/JU
 Sample : PB159894BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK894

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	44	rBV	77024	113575	1.37%	0.137%
2	3.605	101	105	123	rBV	820958	1437438	17.38%	1.735%
3	3.928	155	160	165	rVB	15622	24775	0.30%	0.030%
4	6.863	651	659	673	rBV	1347477	2181277	26.38%	2.633%
5	7.034	681	688	698	rBV	1165381	1809173	21.88%	2.184%
6	7.228	714	721	733	rBV	1345531	2197096	26.57%	2.652%
7	7.693	792	800	812	rBV	1033169	1650825	19.96%	1.993%
8	8.393	910	919	934	rBV	1723656	2772805	33.53%	3.347%
9	8.846	989	996	1007	rBV	1300912	2165862	26.19%	2.615%
10	9.563	1111	1118	1133	rBV	1047341	1689850	20.43%	2.040%
11	10.093	1199	1208	1219	rBV	1700085	2832234	34.25%	3.419%
12	10.475	1264	1273	1283	rBV	1509932	2504787	30.29%	3.024%
13	10.616	1288	1297	1317	rBV	957564	1645054	19.89%	1.986%
14	12.069	1538	1544	1551	rBV2	31173	50291	0.61%	0.061%
15	13.234	1737	1742	1747	rVB	20723	31101	0.38%	0.038%
16	13.751	1821	1830	1840	rBV	3151816	4298929	51.98%	5.190%
17	14.028	1870	1877	1889	rBV	3695478	5312668	64.24%	6.413%
18	14.334	1922	1929	1938	rBV	2384191	3455450	41.78%	4.171%
19	14.534	1956	1963	1983	rBV	1472513	2172571	26.27%	2.623%
20	14.751	1996	2000	2006	rVB9	5954	11975	0.14%	0.014%
21	15.333	2091	2099	2112	rBV	4450948	6523850	78.89%	7.875%
22	15.445	2112	2118	2128	rBV	1179447	1611527	19.49%	1.945%
23	15.569	2135	2139	2146	rVB2	23431	36421	0.44%	0.044%
24	16.110	2227	2231	2236	rBV4	14376	21867	0.26%	0.026%
25	16.763	2339	2342	2347	rVB6	7328	10243	0.12%	0.012%
26	16.863	2357	2359	2368	rVB5	5182	9069	0.11%	0.011%
27	17.080	2390	2396	2406	rBV	2833073	4140831	50.07%	4.999%
28	17.180	2407	2413	2428	rVV2	5053597	7213964	87.23%	8.708%
29	17.980	2546	2549	2554	rBV5	6604	9581	0.12%	0.012%
30	19.045	2725	2730	2736	rVB2	66561	83457	1.01%	0.101%
31	19.116	2736	2742	2748	rBV	52200	80631	0.98%	0.097%
32	19.322	2774	2777	2781	rVB5	8492	13323	0.16%	0.016%
33	19.427	2792	2795	2797	rBV2	9438	11906	0.14%	0.014%
34	19.480	2798	2804	2814	rVV	5854032	8269689	100.00%	9.983%
35	21.316	3111	3116	3129	rBV2	2978573	4351095	52.61%	5.253%
36	24.062	3573	3583	3598	rBV2	3255318	7766312	93.91%	9.375%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030609.D
Acq On : 02 Apr 2024 10:23
Operator : MA/JU
Sample : PB159894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK894

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	24.262	3608	3617	3635	rVB	1722234	4326808	52.32%	5.223%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 82838310

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030609.D
Acq On : 02 Apr 2024 10:23
Operator : MA/JU
Sample : PB159894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK894

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

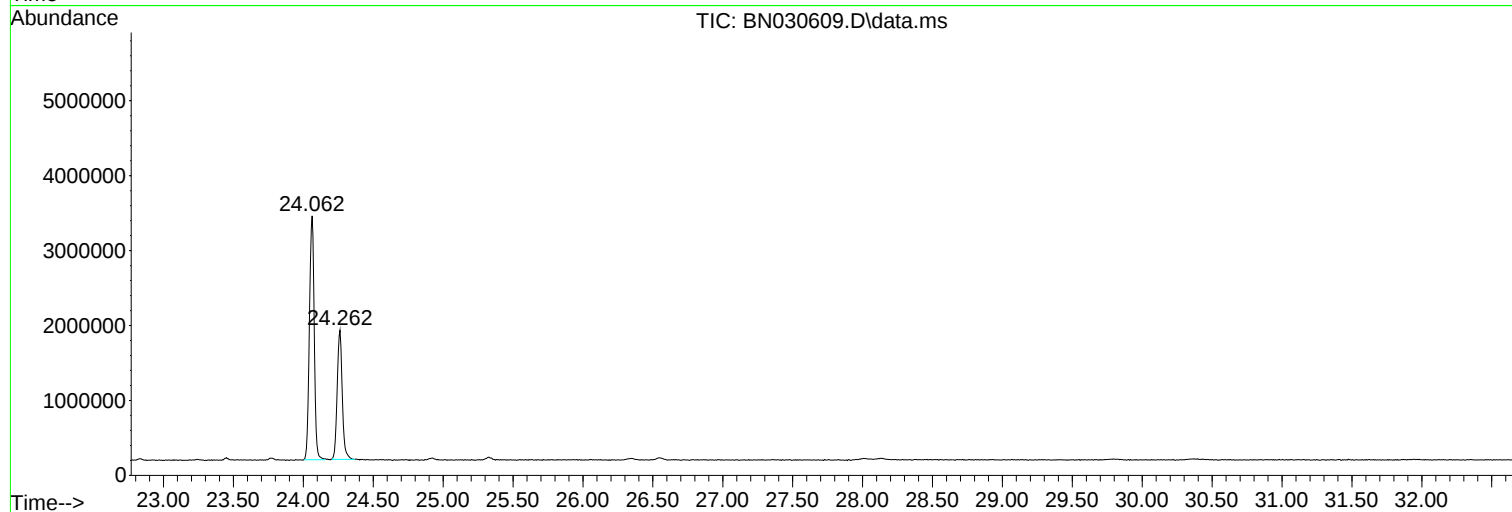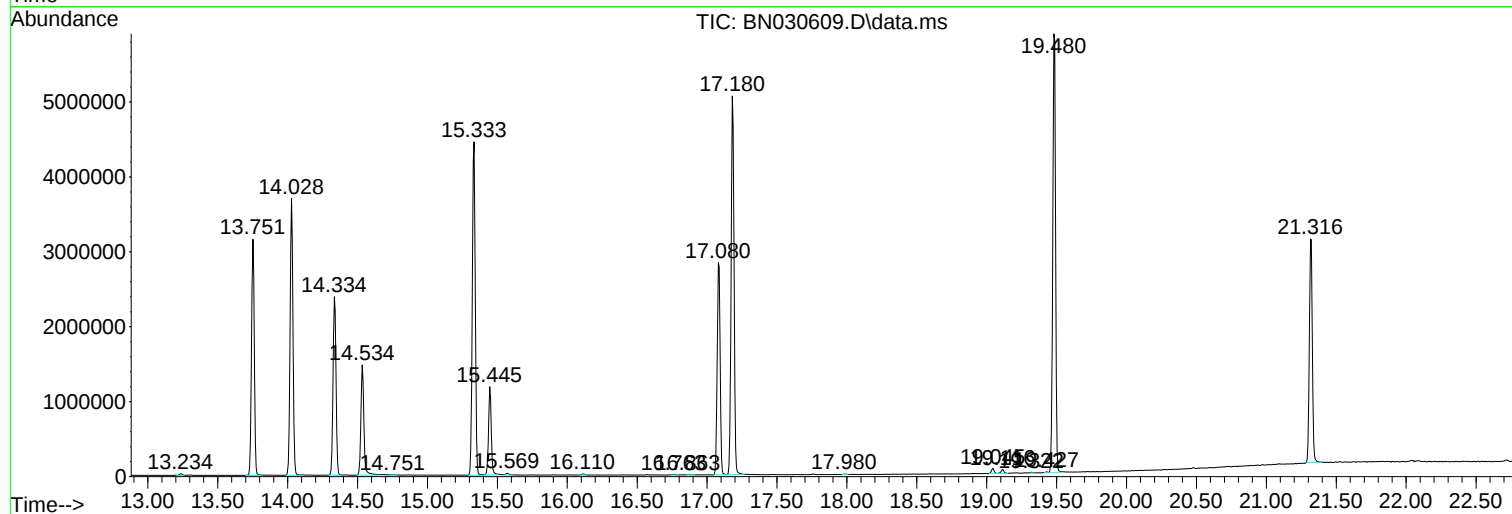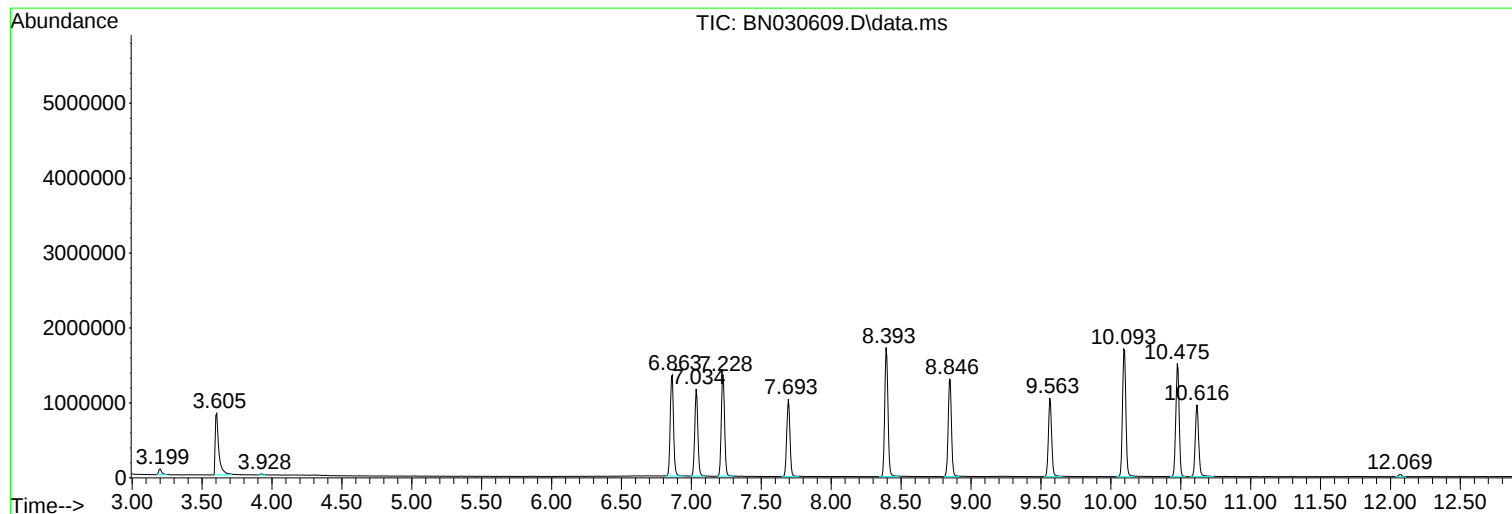

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030609.D
Acq On : 02 Apr 2024 10:23
Operator : MA/JU
Sample : PB159894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK894

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030609.D
Acq On : 02 Apr 2024 10:23
Operator : MA/JU
Sample : PB159894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK894

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc